

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
 Data File : BM031825.D
 Acq On : 19 Aug 2021 13:05
 Operator : CG/JU
 Sample : M3426-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-10-0205

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031825.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.734	276	280	287	rVB	17948	25692	1.60%	0.270%
2	5.169	348	354	371	rVB	623308	901214	56.18%	9.471%
3	6.728	612	619	633	rBV	581654	923717	57.58%	9.707%
4	7.534	748	756	763	rBV	151192	232622	14.50%	2.445%
5	8.687	944	952	966	rBV	347464	578317	36.05%	6.078%
6	10.110	1189	1194	1203	rBV4	7895	19175	1.20%	0.202%
7	10.292	1218	1225	1238	rVB	182195	295511	18.42%	3.106%
8	12.786	1642	1649	1663	rVB	716390	1071890	66.82%	11.265%
9	14.174	1878	1885	1893	rBV	232537	349961	21.82%	3.678%
10	15.674	2134	2140	2150	rBV	621773	874392	54.51%	9.189%
11	16.927	2347	2353	2357	rBV	302060	434489	27.09%	4.566%
12	16.968	2357	2360	2367	rVB2	25947	40220	2.51%	0.423%
13	17.845	2504	2509	2517	rBV	173647	288334	17.97%	3.030%
14	18.992	2700	2704	2710	rBV	90654	148662	9.27%	1.562%
15	19.133	2724	2728	2735	rBV	117239	179803	11.21%	1.890%
16	19.356	2763	2766	2770	rVB	66500	80965	5.05%	0.851%
17	19.574	2798	2803	2809	rVB	1319397	1604138	100.00%	16.858%
18	20.868	3019	3023	3030	rBV2	172548	236524	14.74%	2.486%
19	21.127	3062	3067	3071	rBV	428707	567742	35.39%	5.966%
20	21.750	3170	3173	3179	rVB2	143291	182673	11.39%	1.920%
21	23.274	3428	3432	3439	rVB2	291822	479467	29.89%	5.039%




Sum of corrected areas: 9515508

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031825.D
Acq On : 19 Aug 2021 13:05
Operator : CG/JU
Sample : M3426-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-10-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

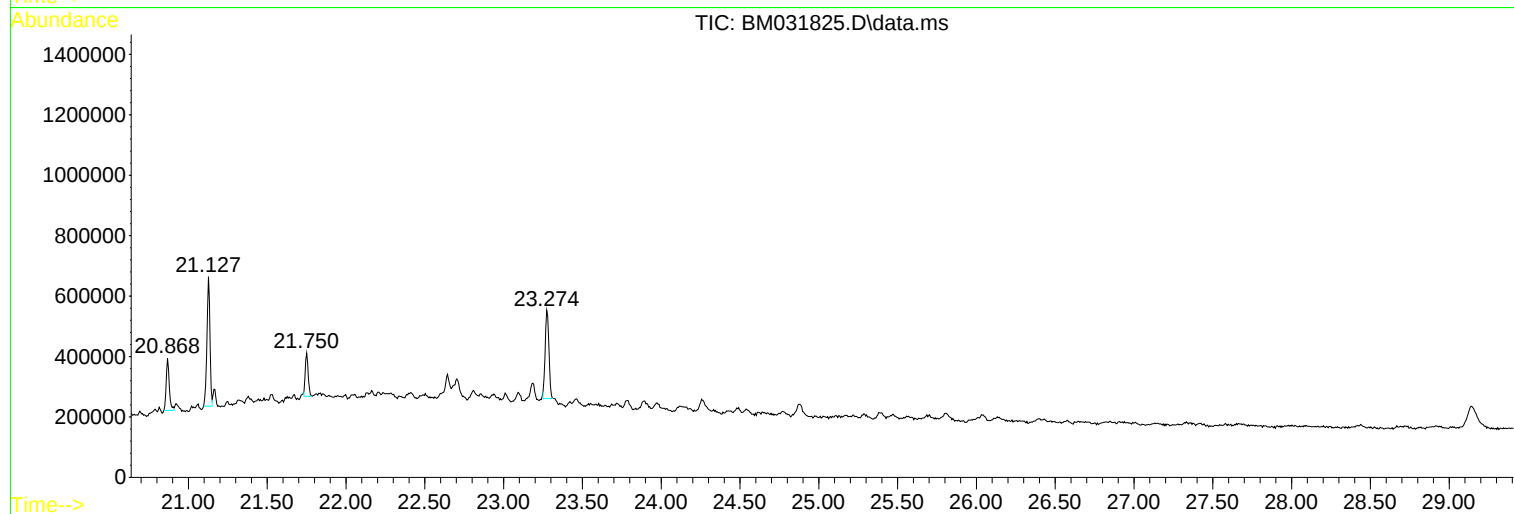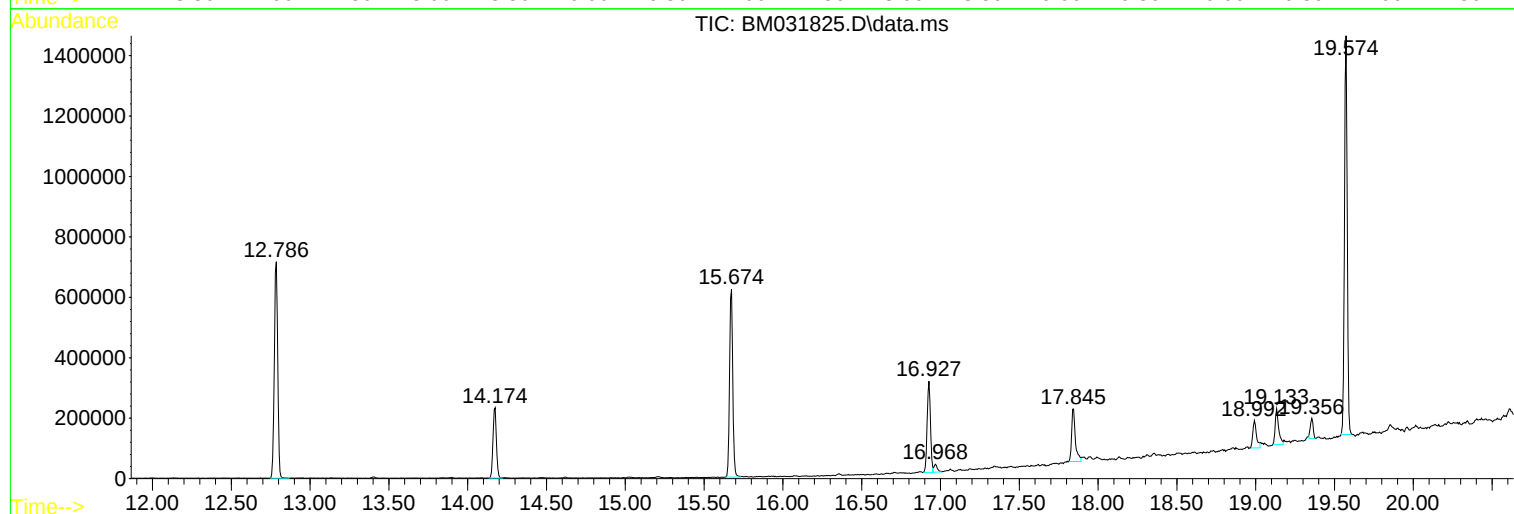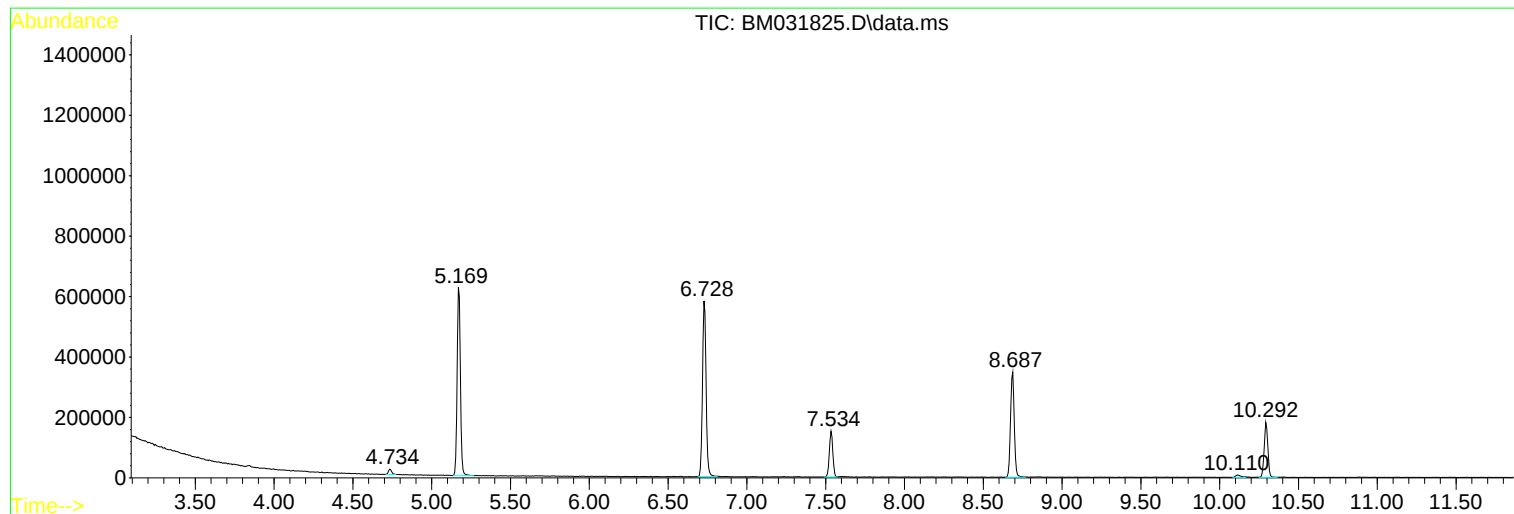

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031825.D
Acq On : 19 Aug 2021 13:05
Operator : CG/JU
Sample : M3426-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-10-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031825.D
Acq On : 19 Aug 2021 13:05
Operator : CG/JU
Sample : M3426-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-10-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------