

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
 Data File : BM031826.D
 Acq On : 19 Aug 2021 13:42
 Operator : CG/JU
 Sample : M3434-33
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-15-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031826.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.734	276	280	290	rVB	38315	54093	2.79%	0.273%
2	5.175	348	355	365	rBV	611767	901329	46.42%	4.548%
3	6.728	613	619	633	rBV	585955	941350	48.48%	4.750%
4	7.534	750	756	763	rVB	164524	256779	13.23%	1.296%
5	8.687	943	952	959	rBV	365417	602635	31.04%	3.041%
6	10.292	1218	1225	1231	rBV	203199	337762	17.40%	1.704%
7	12.786	1642	1649	1656	rBV	817878	1185452	61.06%	5.981%
8	13.627	1786	1792	1796	rBV	11196	19457	1.00%	0.098%
9	13.892	1832	1837	1845	rVB	94717	140726	7.25%	0.710%
10	14.174	1878	1885	1891	rBV	272962	417561	21.51%	2.107%
11	15.227	2058	2064	2078	rVB5	17826	42275	2.18%	0.213%
12	15.674	2130	2140	2151	rBV	694011	984777	50.72%	4.969%
13	15.910	2175	2180	2187	rBV7	18416	33964	1.75%	0.171%
14	16.457	2268	2273	2278	rBV	20060	36065	1.86%	0.182%
15	16.586	2291	2295	2301	rVB2	19008	30047	1.55%	0.152%
16	16.745	2318	2322	2330	rVB	17265	30720	1.58%	0.155%
17	16.927	2347	2353	2357	rBV	359894	530302	27.31%	2.676%
18	16.968	2357	2360	2368	rVV	259897	362742	18.68%	1.830%
19	17.057	2368	2375	2380	rVB	87802	138482	7.13%	0.699%
20	17.121	2382	2386	2390	rVV3	13958	21611	1.11%	0.109%
21	17.310	2414	2418	2420	rBV3	14885	21567	1.11%	0.109%
22	17.339	2420	2423	2428	rVB	26015	41240	2.12%	0.208%
23	17.445	2437	2441	2445	rBV3	14999	22225	1.14%	0.112%
24	17.510	2449	2452	2460	rVB8	13145	21293	1.10%	0.107%
25	17.721	2484	2488	2492	rBV6	11622	20886	1.08%	0.105%
26	17.798	2494	2501	2504	rVV	50586	85029	4.38%	0.429%
27	17.845	2504	2509	2518	rVV2	246792	386957	19.93%	1.952%
28	17.927	2520	2523	2528	rVV	34640	64154	3.30%	0.324%
29	17.992	2529	2534	2539	rVV3	79192	163393	8.42%	0.824%
30	18.033	2539	2541	2546	rVV	40020	47568	2.45%	0.240%
31	18.133	2550	2558	2563	rBV9	18842	45930	2.37%	0.232%
32	18.198	2566	2569	2574	rVB6	13877	22849	1.18%	0.115%
33	18.310	2584	2588	2592	rBV	35849	46956	2.42%	0.237%
34	18.357	2592	2596	2601	rVB2	43406	56698	2.92%	0.286%
35	18.557	2627	2630	2635	rBV4	14516	21437	1.10%	0.108%
36	18.604	2635	2638	2643	rVV2	19984	27960	1.44%	0.141%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
 Data File : BM031826.D
 Acq On : 19 Aug 2021 13:42
 Operator : CG/JU
 Sample : M3434-33
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-15-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.727	2654	2659	2665	rBV4	53890	101888	5.25%	0.514%
38	18.786	2665	2669	2673	rVV4	28256	55536	2.86%	0.280%
39	18.821	2673	2675	2679	rVB2	21051	24571	1.27%	0.124%
40	18.868	2679	2683	2691	rBV3	43678	81114	4.18%	0.409%
41	18.992	2696	2704	2712	rBV	671186	935276	48.17%	4.719%
42	19.139	2724	2729	2735	rBV2	145138	232177	11.96%	1.171%
43	19.356	2757	2766	2771	rBV	594467	905989	46.66%	4.571%
44	19.439	2776	2780	2785	rVB3	39830	65378	3.37%	0.330%
45	19.574	2795	2803	2814	rVB	1532659	1941570	100.00%	9.796%
46	19.686	2818	2822	2830	rVB4	43975	99627	5.13%	0.503%
47	19.827	2841	2846	2848	rBV4	47714	81917	4.22%	0.413%
48	19.862	2849	2852	2856	rVB	72820	101299	5.22%	0.511%
49	19.962	2865	2869	2872	rBV2	58251	66237	3.41%	0.334%
50	20.015	2874	2878	2883	rVB2	68050	99632	5.13%	0.503%
51	20.156	2899	2902	2905	rVB	46993	50409	2.60%	0.254%
52	20.203	2906	2910	2920	rVV2	39266	91189	4.70%	0.460%
53	20.609	2976	2979	2986	rVB	66076	95974	4.94%	0.484%
54	20.774	3004	3007	3011	rVB3	53280	69912	3.60%	0.353%
55	20.815	3011	3014	3017	rBV	54027	58981	3.04%	0.298%
56	20.868	3017	3023	3027	rBV3	225980	353607	18.21%	1.784%
57	21.062	3053	3056	3059	rVB	58000	58077	2.99%	0.293%
58	21.127	3061	3067	3071	rVV2	630519	1208283	62.23%	6.096%
59	21.168	3071	3074	3081	rVB	366506	485309	25.00%	2.449%
60	21.721	3164	3168	3170	rBV	147724	178170	9.18%	0.899%
61	21.750	3170	3173	3180	rVB	186310	288185	14.84%	1.454%
62	22.386	3277	3281	3295	rVB3	178006	308286	15.88%	1.555%
63	22.645	3320	3325	3330	rBV	500126	942541	48.55%	4.756%
64	22.697	3331	3334	3344	rVB2	331763	621978	32.03%	3.138%
65	23.092	3397	3401	3408	rVB	212279	366986	18.90%	1.852%
66	23.186	3412	3417	3423	rVB	334546	564031	29.05%	2.846%
67	23.280	3427	3433	3438	rBV	304232	542165	27.92%	2.735%
68	23.786	3515	3519	3528	rVB	164177	320915	16.53%	1.619%
69	23.891	3532	3537	3546	rVB5	108823	258304	13.30%	1.303%




Sum of corrected areas: 19819784

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031826.D
Acq On : 19 Aug 2021 13:42
Operator : CG/JU
Sample : M3434-33
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-15-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

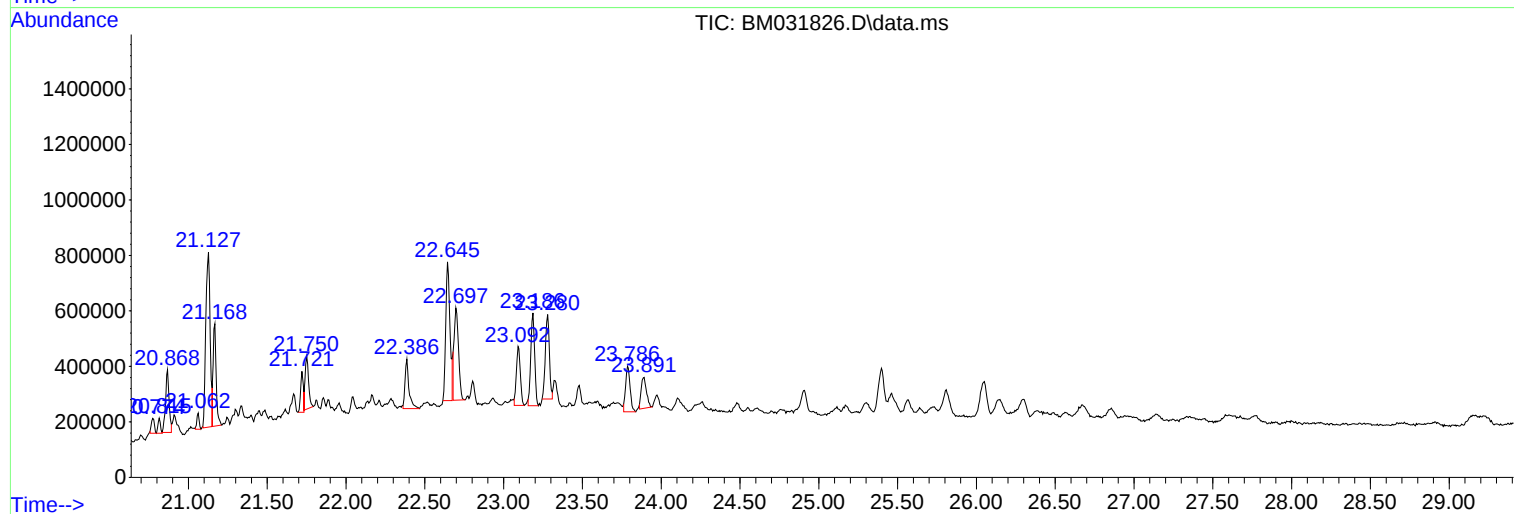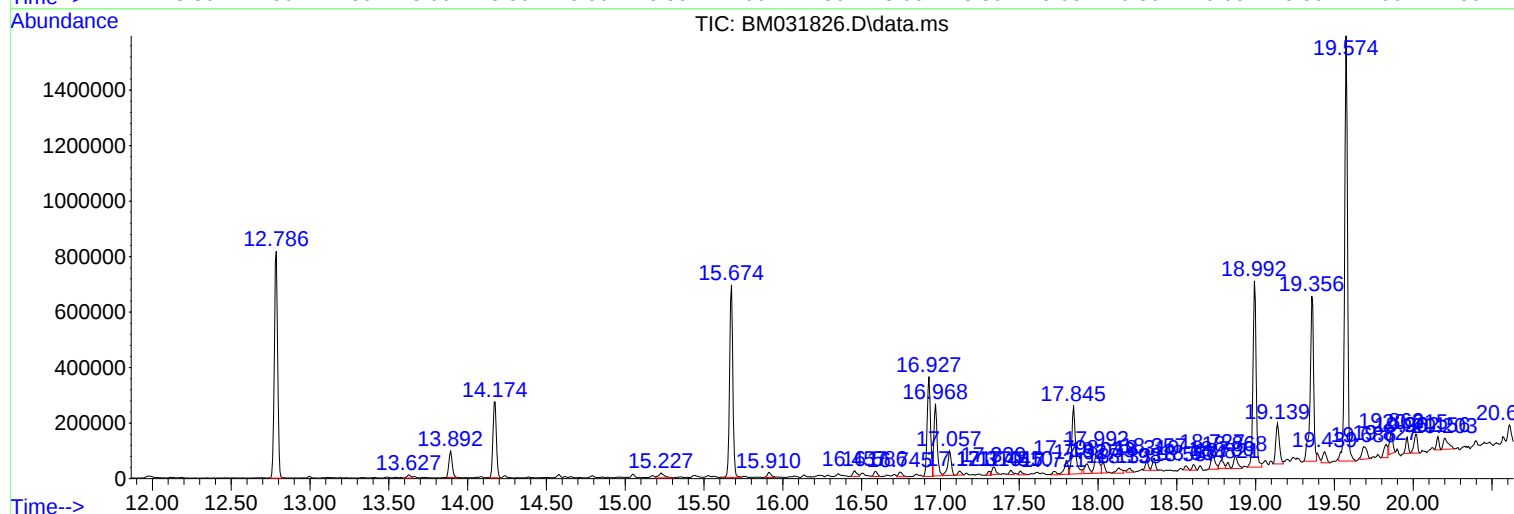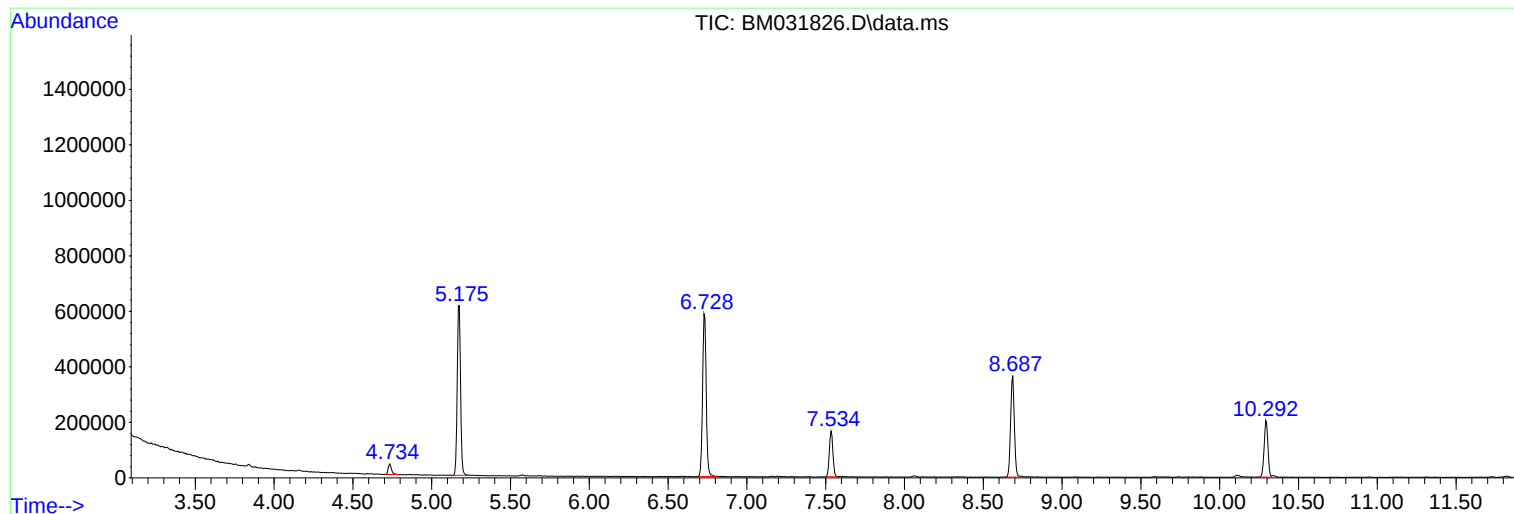

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031826.D
Acq On : 19 Aug 2021 13:42
Operator : CG/JU
Sample : M3434-33
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-15-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031826.D
Acq On : 19 Aug 2021 13:42
Operator : CG/JU
Sample : M3434-33
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-15-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------