

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
 Data File : BM031827.D
 Acq On : 19 Aug 2021 14:19
 Operator : CG/JU
 Sample : M3435-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-24-0003

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031827.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.840	124	128	135	rVB	128916	170943	9.50%	0.564%
2	4.734	277	280	286	rVB	15334	20821	1.16%	0.069%
3	5.175	348	355	363	rBV	645614	930353	51.72%	3.067%
4	6.593	589	596	601	rBV	19449	31133	1.73%	0.103%
5	6.734	612	620	632	rBV	623322	997046	55.43%	3.287%
6	7.534	749	756	764	rVB	171894	265852	14.78%	0.876%
7	8.310	876	888	900	rBV2	44853	94225	5.24%	0.311%
8	8.687	945	952	959	rBV	384543	621587	34.56%	2.049%
9	10.098	1183	1192	1206	rBV	170005	320344	17.81%	1.056%
10	10.292	1218	1225	1231	rBV	212179	353081	19.63%	1.164%
11	10.345	1231	1234	1240	rVB	12822	19627	1.09%	0.065%
12	11.969	1504	1510	1524	rBV4	15336	35196	1.96%	0.116%
13	12.133	1528	1538	1543	rBV5	13073	35227	1.96%	0.116%
14	12.786	1642	1649	1657	rVB	888946	1254256	69.73%	4.135%
15	12.998	1680	1685	1693	rBV7	15227	30409	1.69%	0.100%
16	13.110	1700	1704	1708	rVB2	12686	19821	1.10%	0.065%
17	13.486	1760	1768	1774	rBV6	9895	20442	1.14%	0.067%
18	13.663	1793	1798	1805	rVB	64545	97909	5.44%	0.323%
19	13.816	1817	1824	1827	rBV8	9663	21206	1.18%	0.070%
20	13.892	1832	1837	1845	rVB	45245	74001	4.11%	0.244%
21	14.063	1862	1866	1868	rBV3	11827	20119	1.12%	0.066%
22	14.174	1876	1885	1893	rBV	306165	455898	25.35%	1.503%
23	14.786	1983	1989	1997	rVB6	10185	20911	1.16%	0.069%
24	15.045	2030	2033	2040	rVB3	16105	23315	1.30%	0.077%
25	15.157	2047	2052	2057	rBV6	10231	21749	1.21%	0.072%
26	15.204	2057	2060	2071	rVB10	7945	21840	1.21%	0.072%
27	15.439	2095	2100	2108	rVB9	7463	18050	1.00%	0.060%
28	15.610	2125	2129	2132	rBV3	25697	34511	1.92%	0.114%
29	15.674	2133	2140	2150	rVV	737194	1038797	57.75%	3.425%
30	15.916	2175	2181	2188	rBV6	27567	54819	3.05%	0.181%
31	15.986	2189	2193	2200	rVB6	14576	21864	1.22%	0.072%
32	16.074	2200	2208	2213	rBV6	15763	31293	1.74%	0.103%
33	16.133	2214	2218	2225	rBV2	35775	53458	2.97%	0.176%
34	16.351	2249	2255	2264	rBV3	71656	126277	7.02%	0.416%
35	16.451	2269	2272	2279	rVB	14046	23251	1.29%	0.077%
36	16.586	2290	2295	2300	rBV3	25316	38332	2.13%	0.126%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
 Data File : BM031827.D
 Acq On : 19 Aug 2021 14:19
 Operator : CG/JU
 Sample : M3435-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-24-0003

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	16.704	2312	2315	2319	rBV2	13720	20175	1.12%	0.067%
38	16.745	2319	2322	2327	rVB3	13249	18112	1.01%	0.060%
39	16.851	2335	2340	2342	rBV3	29318	43066	2.39%	0.142%
40	16.927	2347	2353	2357	rBV	363883	532312	29.59%	1.755%
41	16.968	2357	2360	2368	rVB2	104191	202463	11.26%	0.667%
42	17.033	2368	2371	2374	rBV2	42060	59197	3.29%	0.195%
43	17.121	2382	2386	2390	rBV6	18408	25955	1.44%	0.086%
44	17.163	2390	2393	2398	rVV4	13315	18015	1.00%	0.059%
45	17.310	2414	2418	2419	rBV2	31914	35241	1.96%	0.116%
46	17.333	2419	2422	2430	rVB2	46825	80890	4.50%	0.267%
47	17.510	2450	2452	2459	rVB7	14064	22928	1.27%	0.076%
48	17.586	2459	2465	2467	rBV7	15338	26935	1.50%	0.089%
49	17.615	2467	2470	2475	rVB	39678	49230	2.74%	0.162%
50	17.727	2483	2489	2492	rBV6	25314	43227	2.40%	0.143%
51	17.798	2495	2501	2504	rVV3	23061	44523	2.48%	0.147%
52	17.845	2504	2509	2518	rBV	443103	619649	34.45%	2.043%
53	17.992	2530	2534	2539	rBV2	32282	57777	3.21%	0.190%
54	18.033	2539	2541	2549	rVB	23086	33140	1.84%	0.109%
55	18.139	2554	2559	2564	rBV5	45631	90330	5.02%	0.298%
56	18.310	2585	2588	2591	rBV2	25434	29709	1.65%	0.098%
57	18.357	2592	2596	2603	rVB2	38202	54002	3.00%	0.178%
58	18.527	2620	2625	2635	rBV6	42880	100134	5.57%	0.330%
59	18.727	2654	2659	2663	rBV2	49711	102737	5.71%	0.339%
60	18.774	2664	2667	2669	rVV2	38695	52117	2.90%	0.172%
61	18.798	2669	2671	2674	rVV	66374	65355	3.63%	0.215%
62	18.874	2678	2684	2692	rVB6	34713	64999	3.61%	0.214%
63	18.962	2696	2699	2700	rBV	32129	30231	1.68%	0.100%
64	18.992	2700	2704	2714	rVV	228108	418608	23.27%	1.380%
65	19.139	2724	2729	2737	rBV2	198162	299851	16.67%	0.988%
66	19.356	2759	2766	2770	rBV	211951	302798	16.83%	0.998%
67	19.574	2798	2803	2812	rVB	1489472	1798678	100.00%	5.930%
68	19.651	2813	2816	2819	rBV4	31267	36907	2.05%	0.122%
69	19.874	2849	2854	2856	rBV2	108194	156358	8.69%	0.515%
70	19.898	2856	2858	2864	rVB	102725	110340	6.13%	0.364%
71	20.015	2876	2878	2883	rVB2	29559	33577	1.87%	0.111%
72	20.080	2886	2889	2893	rVB3	34367	40975	2.28%	0.135%
73	20.192	2904	2908	2910	rBV	85110	104390	5.80%	0.344%
74	20.221	2911	2913	2920	rVB3	88526	130293	7.24%	0.430%
75	20.398	2938	2943	2948	rBV3	61212	103389	5.75%	0.341%
76	20.574	2970	2973	2976	rBV2	45399	46585	2.59%	0.154%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
 Data File : BM031827.D
 Acq On : 19 Aug 2021 14:19
 Operator : CG/JU
 Sample : M3435-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-24-0003

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	20.862	3018	3022	3031	rBV	1028192	1407463	78.25%	4.640%
78	21.062	3053	3056	3061	rVB	145789	152551	8.48%	0.503%
79	21.127	3061	3067	3071	rBV2	477543	759886	42.25%	2.505%
80	21.168	3071	3074	3084	rVB	278966	415872	23.12%	1.371%
81	21.309	3094	3098	3108	rVB9	82456	232435	12.92%	0.766%
82	21.474	3124	3126	3132	rVB4	71151	77220	4.29%	0.255%
83	21.721	3164	3168	3170	rBV	747308	924450	51.40%	3.048%
84	21.745	3170	3172	3181	rVB	1191062	1700684	94.55%	5.607%
85	22.045	3219	3223	3232	rBV	205877	353686	19.66%	1.166%
86	22.203	3247	3250	3256	rVB2	135570	201906	11.23%	0.666%
87	22.380	3277	3280	3291	rVB2	201226	298078	16.57%	0.983%
88	22.650	3320	3326	3330	rBV2	1031894	1557243	86.58%	5.134%
89	22.697	3330	3334	3343	rVB2	675628	1172528	65.19%	3.865%
90	23.180	3412	3416	3422	rVB2	170450	287017	15.96%	0.946%
91	23.280	3428	3433	3438	rVB2	301221	537952	29.91%	1.773%
92	23.474	3462	3466	3473	rVB	276211	489362	27.21%	1.613%
93	23.786	3514	3519	3527	rVB	470464	911338	50.67%	3.004%
94	23.886	3530	3536	3546	rVV	514729	1126092	62.61%	3.712%
95	24.909	3704	3710	3720	rVB	420378	939292	52.22%	3.096%
96	25.456	3796	3803	3814	rVV	586798	1648259	91.64%	5.434%
97	25.568	3816	3822	3836	rVB2	274572	745890	41.47%	2.459%
98	26.144	3913	3920	3936	rVB5	266019	871680	48.46%	2.874%




Sum of corrected areas: 30334045

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031827.D
Acq On : 19 Aug 2021 14:19
Operator : CG/JU
Sample : M3435-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-24-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

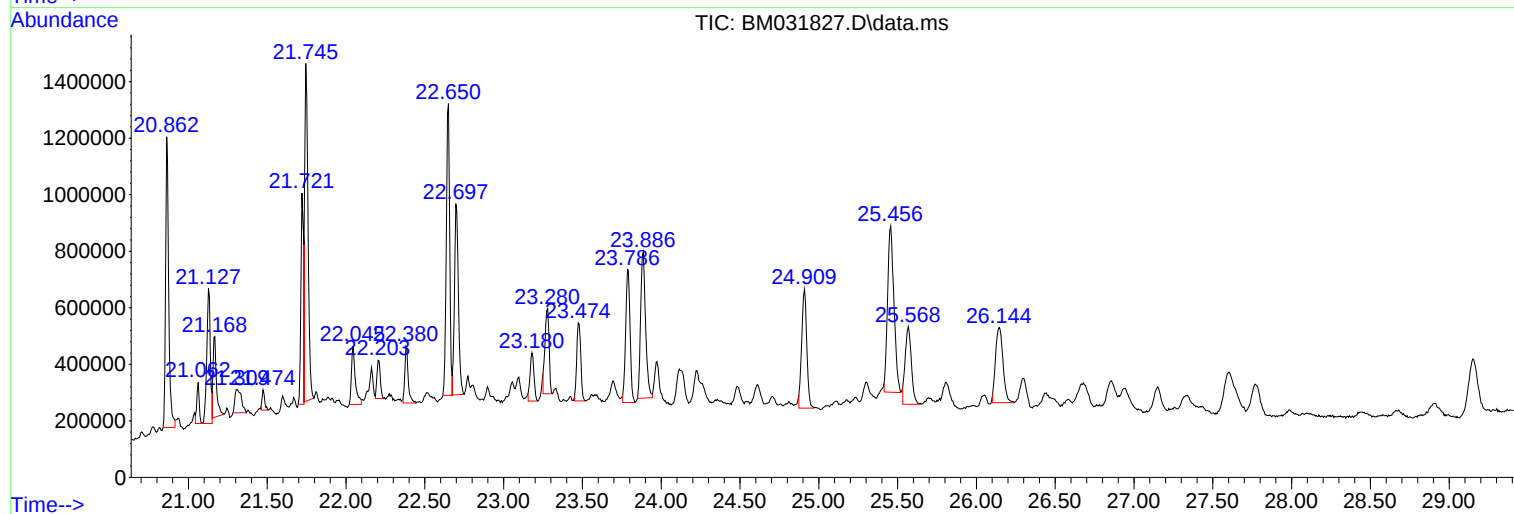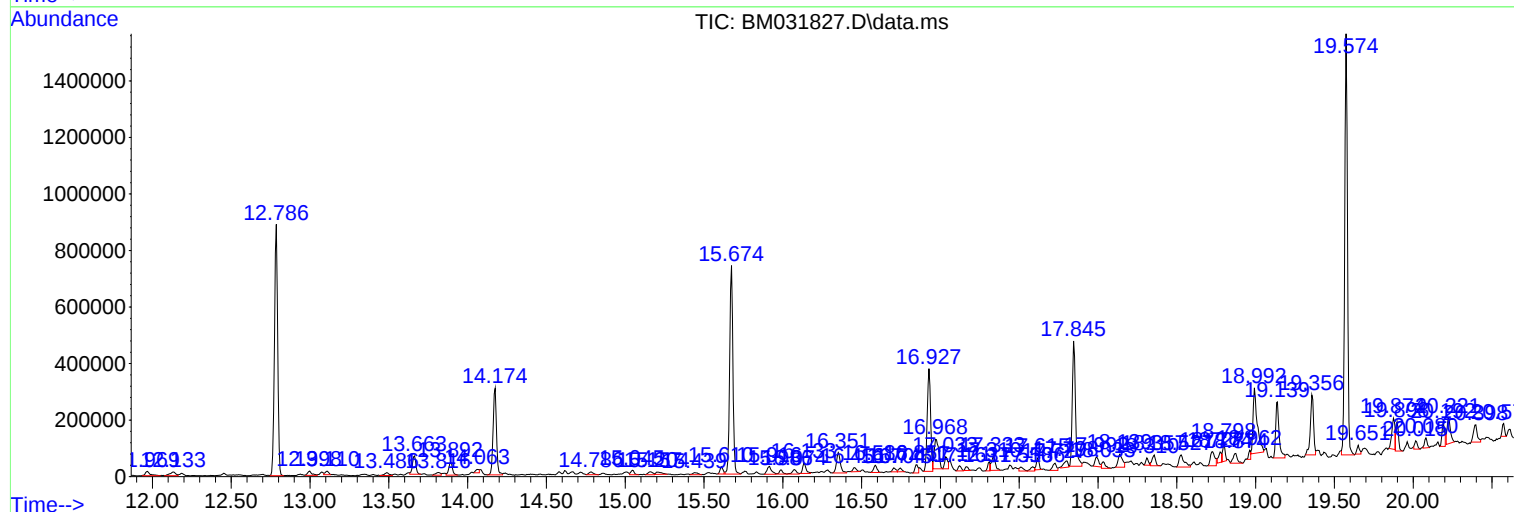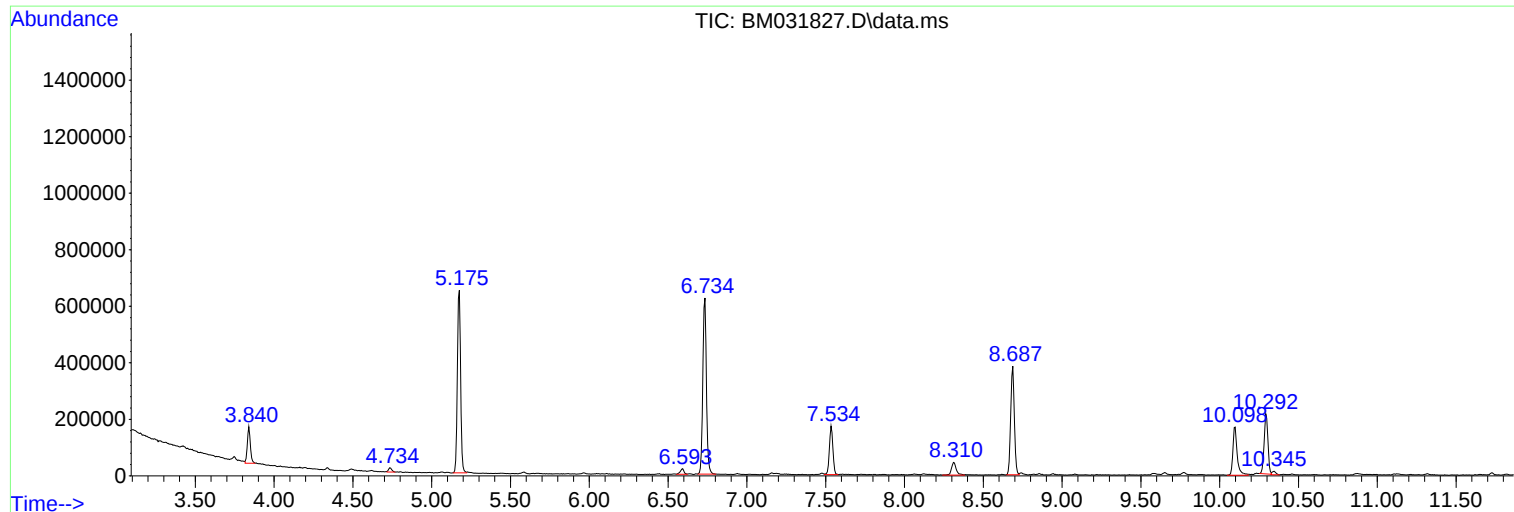

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031827.D
Acq On : 19 Aug 2021 14:19
Operator : CG/JU
Sample : M3435-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-24-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031827.D
Acq On : 19 Aug 2021 14:19
Operator : CG/JU
Sample : M3435-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-24-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------