

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
 Data File : BM031829.D
 Acq On : 19 Aug 2021 15:34
 Operator : CG/JU
 Sample : M3435-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-21-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031829.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.840	124	128	137	rVB	55057	84944	5.15%	0.520%
2	4.734	276	280	287	rVB	23843	35654	2.16%	0.218%
3	5.175	349	355	365	rBV	698876	1013156	61.44%	6.200%
4	6.234	530	535	541	rVB	27821	42530	2.58%	0.260%
5	6.734	611	620	633	rBV	726719	1140390	69.16%	6.978%
6	7.534	749	756	763	rBV	171547	266271	16.15%	1.629%
7	8.310	883	888	897	rBV2	24932	46560	2.82%	0.285%
8	8.686	945	952	967	rVB	454914	731017	44.33%	4.473%
9	10.098	1183	1192	1200	rBV	133279	251247	15.24%	1.537%
10	10.292	1217	1225	1232	rBV	205367	348396	21.13%	2.132%
11	12.133	1529	1538	1544	rBV6	9278	18728	1.14%	0.115%
12	12.786	1642	1649	1657	rBV	897690	1289206	78.19%	7.889%
13	13.892	1832	1837	1844	rVB2	15323	24219	1.47%	0.148%
14	14.174	1878	1885	1892	rBV	307055	433644	26.30%	2.653%
15	15.674	2130	2140	2147	rBV	840792	1148460	69.65%	7.028%
16	15.880	2170	2175	2189	rVB2	72412	170738	10.35%	1.045%
17	16.080	2204	2209	2215	rVB3	16936	31484	1.91%	0.193%
18	16.145	2215	2220	2225	rBV3	18030	32609	1.98%	0.200%
19	16.280	2239	2243	2249	rVB6	20221	38269	2.32%	0.234%
20	16.351	2249	2255	2261	rBV4	30994	59544	3.61%	0.364%
21	16.415	2261	2266	2270	rVV	19411	30960	1.88%	0.189%
22	16.486	2274	2278	2284	rVB2	15071	23096	1.40%	0.141%
23	16.927	2348	2353	2357	rBV	370865	506219	30.70%	3.098%
24	16.968	2357	2360	2367	rVV	73345	128683	7.80%	0.787%
25	17.039	2367	2372	2373	rVV2	15757	22750	1.38%	0.139%
26	17.062	2373	2376	2383	rVB	24913	36827	2.23%	0.225%
27	17.309	2414	2418	2420	rBV3	16172	21860	1.33%	0.134%
28	17.339	2420	2423	2428	rVB3	20291	31246	1.89%	0.191%
29	17.621	2467	2471	2474	rVB2	29954	33070	2.01%	0.202%
30	17.721	2485	2488	2494	rBV7	14594	21001	1.27%	0.129%
31	17.780	2494	2498	2505	rBV3	30538	60287	3.66%	0.369%
32	17.845	2505	2509	2518	rBV2	215856	316092	19.17%	1.934%
33	17.992	2530	2534	2538	rBV4	17005	28350	1.72%	0.173%
34	18.133	2555	2558	2561	rBV3	14109	17778	1.08%	0.109%
35	18.356	2592	2596	2603	rVB3	19934	29810	1.81%	0.182%
36	18.527	2621	2625	2628	rBV5	16746	27599	1.67%	0.169%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
 Data File : BM031829.D
 Acq On : 19 Aug 2021 15:34
 Operator : CG/JU
 Sample : M3435-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-21-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.727	2654	2659	2663	rBV5	20208	41829	2.54%	0.256%
38	18.992	2699	2704	2710	rBV	202159	322924	19.58%	1.976%
39	19.133	2724	2728	2735	rBV2	107899	172157	10.44%	1.053%
40	19.356	2762	2766	2770	rVB	157850	197249	11.96%	1.207%
41	19.397	2770	2773	2778	rVB	70708	86436	5.24%	0.529%
42	19.574	2798	2803	2813	rVB	1322953	1648915	100.00%	10.090%
43	19.874	2850	2854	2856	rBV3	37988	59129	3.59%	0.362%
44	19.897	2856	2858	2862	rVB	63792	68936	4.18%	0.422%
45	20.221	2910	2913	2916	rBV4	52431	57841	3.51%	0.354%
46	20.862	3018	3022	3028	rBV	442620	592467	35.93%	3.625%
47	21.009	3043	3047	3053	rBV	298780	384474	23.32%	2.353%
48	21.062	3054	3056	3061	rVV2	55012	64726	3.93%	0.396%
49	21.127	3062	3067	3071	rVV2	442587	676820	41.05%	4.142%
50	21.168	3071	3074	3081	rVB	169611	221792	13.45%	1.357%
51	21.233	3082	3085	3092	rBV3	86623	137477	8.34%	0.841%
52	21.721	3165	3168	3170	rBV	173764	215205	13.05%	1.317%
53	21.744	3170	3172	3179	rVB	377174	511329	31.01%	3.129%
54	22.386	3278	3281	3291	rVB4	80061	124470	7.55%	0.762%
55	22.644	3321	3325	3330	rBV	373631	565449	34.29%	3.460%
56	22.697	3330	3334	3344	rVB2	285089	520927	31.59%	3.188%
57	23.280	3428	3433	3439	rVB2	285745	496010	30.08%	3.035%
58	23.791	3515	3520	3527	rVB	141927	270356	16.40%	1.654%
59	23.885	3531	3536	3545	rVB	167242	362751	22.00%	2.220%




Sum of corrected areas: 16342363

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031829.D
Acq On : 19 Aug 2021 15:34
Operator : CG/JU
Sample : M3435-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-21-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

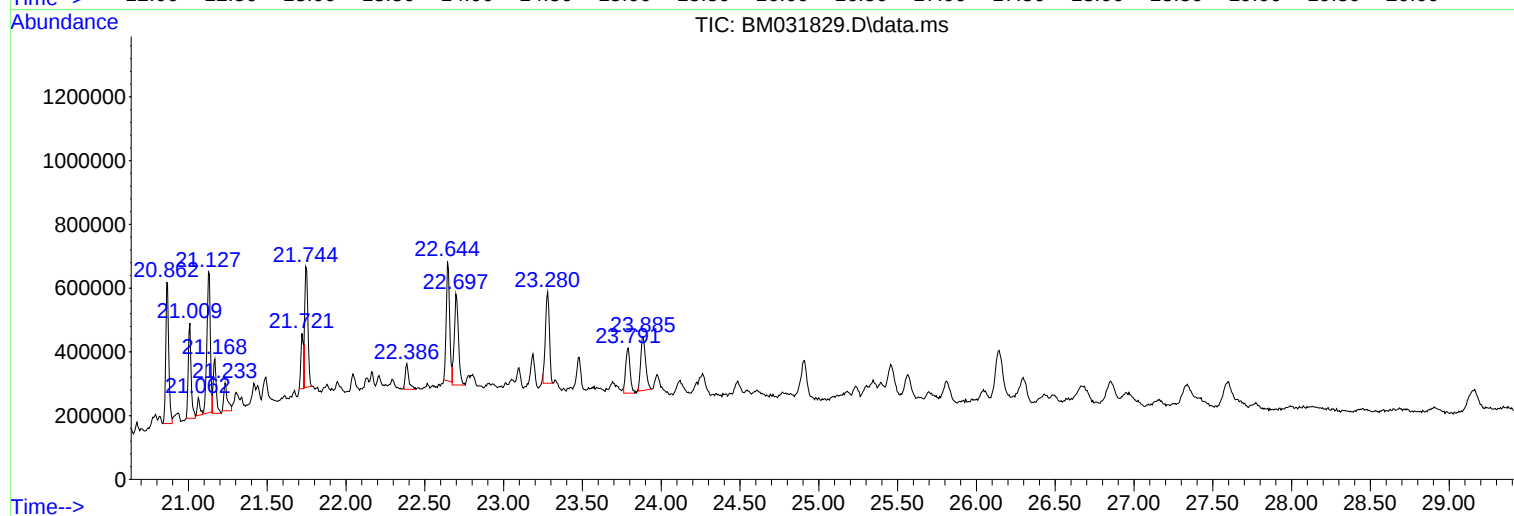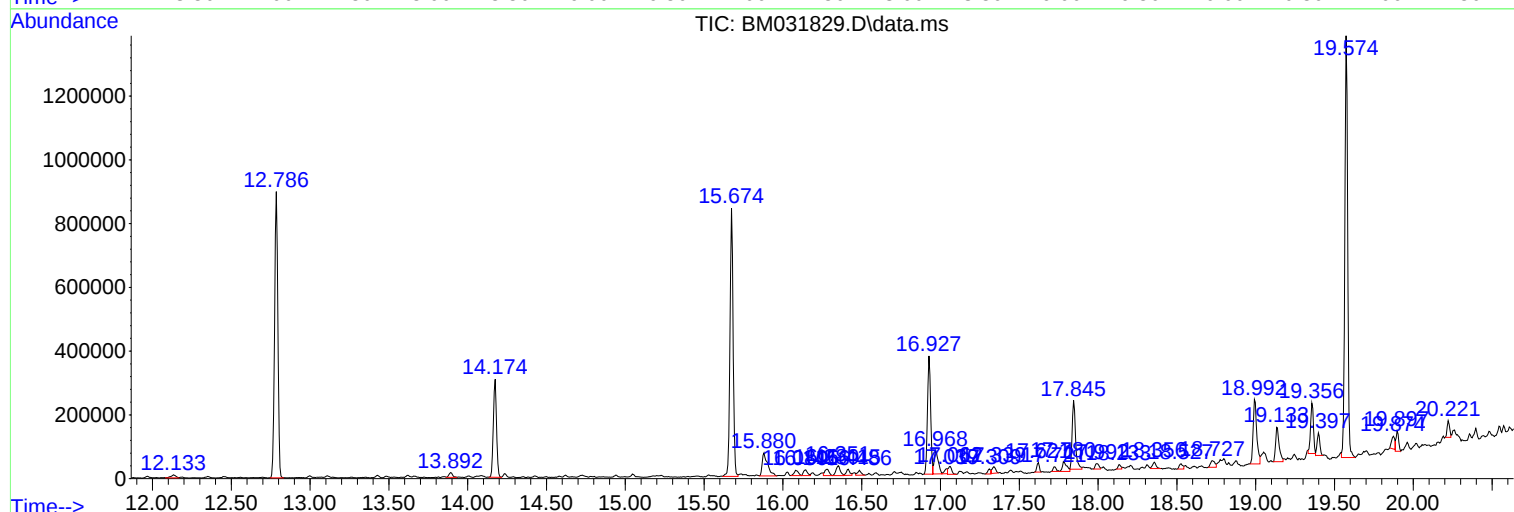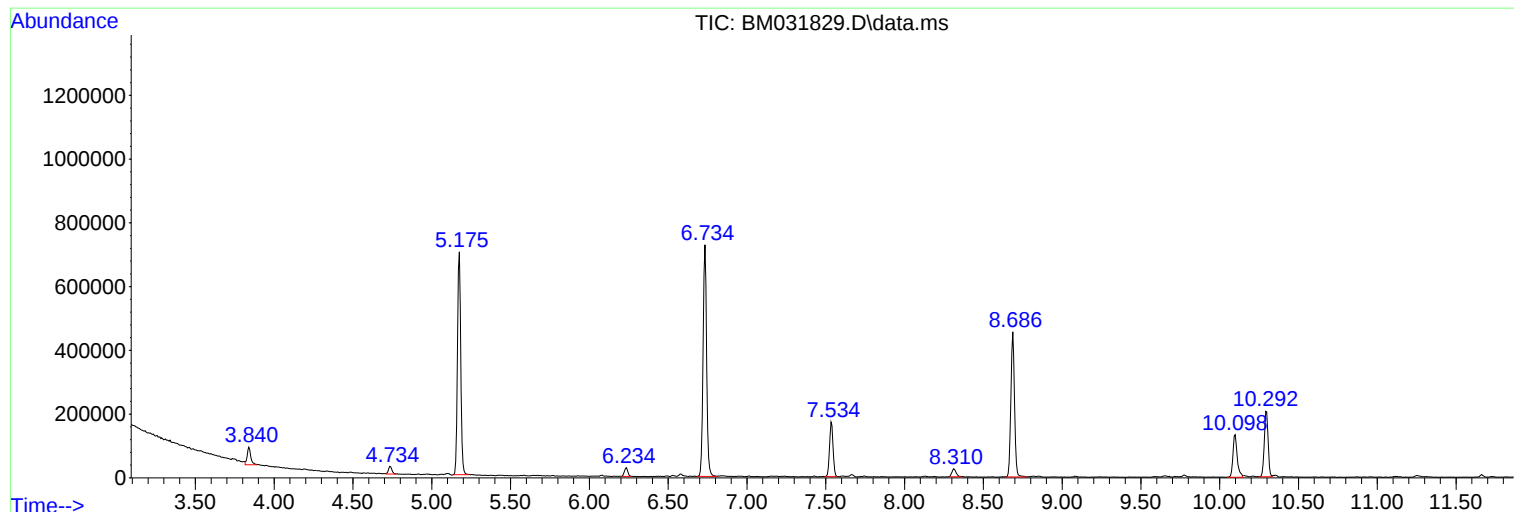

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031829.D
Acq On : 19 Aug 2021 15:34
Operator : CG/JU
Sample : M3435-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-21-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031829.D
Acq On : 19 Aug 2021 15:34
Operator : CG/JU
Sample : M3435-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-21-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
