

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
 Data File : BM031830.D
 Acq On : 19 Aug 2021 16:11
 Operator : CG/JU
 Sample : M3435-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 2021-08-13-FD-04

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031830.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.840	125	128	135	rVB	31828	46994	4.08%	0.214%
2	4.734	277	280	289	rVB2	17396	27248	2.37%	0.124%
3	5.175	349	355	365	rBV	699474	997211	86.68%	4.544%
4	6.528	581	585	589	rBV2	9009	11730	1.02%	0.053%
5	6.734	612	620	632	rBV	660406	1036792	90.12%	4.725%
6	6.952	651	657	663	rBV	37278	59346	5.16%	0.270%
7	7.022	663	669	674	rVB4	14972	24439	2.12%	0.111%
8	7.534	750	756	764	rVB	175911	272590	23.69%	1.242%
9	7.663	772	778	786	rVB	414378	624758	54.30%	2.847%
10	7.746	788	792	797	rVB3	11092	14791	1.29%	0.067%
11	8.316	883	889	896	rBV3	13037	25096	2.18%	0.114%
12	8.687	944	952	960	rBV	396819	660013	57.37%	3.008%
13	9.675	1112	1120	1125	rVB	31786	54874	4.77%	0.250%
14	10.098	1184	1192	1206	rBV	122204	240554	20.91%	1.096%
15	10.210	1206	1211	1218	rVV2	25061	41558	3.61%	0.189%
16	10.293	1219	1225	1232	rVB	207683	348785	30.32%	1.589%
17	11.751	1465	1473	1482	rVB9	7503	14486	1.26%	0.066%
18	12.786	1641	1649	1657	rBV	711927	1030844	89.60%	4.697%
19	13.116	1701	1705	1717	rVB4	6979	15344	1.33%	0.070%
20	13.892	1832	1837	1841	rVB	10365	15771	1.37%	0.072%
21	14.175	1878	1885	1893	rVB	307290	443380	38.54%	2.020%
22	14.733	1972	1980	1982	rBV2	13921	26512	2.30%	0.121%
23	15.675	2131	2140	2150	rVB	691700	980537	85.23%	4.468%
24	15.880	2169	2175	2182	rBV	608146	788370	68.52%	3.592%
25	15.933	2182	2184	2188	rVB2	11292	13855	1.20%	0.063%
26	16.027	2196	2200	2204	rBV	23272	27476	2.39%	0.125%
27	16.086	2204	2210	2215	rVV2	25352	47490	4.13%	0.216%
28	16.145	2215	2220	2225	rVV3	26436	43592	3.79%	0.199%
29	16.192	2225	2228	2232	rVB2	13444	17457	1.52%	0.080%
30	16.251	2232	2238	2239	rBV5	8623	13475	1.17%	0.061%
31	16.280	2239	2243	2249	rVB4	14015	28508	2.48%	0.130%
32	16.351	2249	2255	2261	rBV5	35971	70767	6.15%	0.322%
33	16.416	2262	2266	2270	rBV	20903	27463	2.39%	0.125%
34	16.486	2275	2278	2285	rVB2	18100	25847	2.25%	0.118%
35	16.704	2311	2315	2319	rBV6	7506	11879	1.03%	0.054%
36	16.786	2326	2329	2333	rVB3	8834	11812	1.03%	0.054%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
 Data File : BM031830.D
 Acq On : 19 Aug 2021 16:11
 Operator : CG/JU
 Sample : M3435-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 2021-08-13-FD-04

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	16.927	2347	2353	2358	rBV	370664	530428	46.10%	2.417%
38	16.969	2358	2360	2367	rVB2	43522	75071	6.53%	0.342%
39	17.033	2367	2371	2374	rBV5	10301	16915	1.47%	0.077%
40	17.127	2383	2387	2391	rBV7	8107	13075	1.14%	0.060%

41	17.310	2412	2418	2420	rBV5	14133	23610	2.05%	0.108%
42	17.339	2420	2423	2427	rVV4	17571	28812	2.50%	0.131%
43	17.410	2430	2435	2444	rVV	434030	565146	49.12%	2.575%
44	17.621	2467	2471	2475	rVB	25945	32841	2.85%	0.150%
45	17.727	2484	2489	2494	rBV8	11844	20246	1.76%	0.092%

46	17.845	2504	2509	2518	rBV2	228293	331622	28.82%	1.511%
47	17.916	2518	2521	2526	rVV6	19561	35872	3.12%	0.163%
48	17.992	2530	2534	2539	rVB5	17367	35221	3.06%	0.160%
49	18.098	2549	2552	2556	rBV5	16043	19083	1.66%	0.087%
50	18.151	2556	2561	2567	rVV2	24563	57024	4.96%	0.260%

51	18.210	2567	2571	2579	rVB	38875	80591	7.00%	0.367%
52	18.280	2579	2583	2586	rBV3	34049	48409	4.21%	0.221%
53	18.427	2605	2608	2611	rBV4	13817	16636	1.45%	0.076%
54	18.557	2621	2630	2635	rVB	175913	265397	23.07%	1.209%
55	18.721	2654	2658	2661	rBV5	30327	48966	4.26%	0.223%

56	18.798	2669	2671	2675	rVB3	34711	38364	3.33%	0.175%
57	18.998	2700	2705	2710	rBV	135710	243541	21.17%	1.110%
58	19.057	2710	2715	2720	rVB	187518	268941	23.38%	1.226%
59	19.133	2724	2728	2734	rBV2	143447	218464	18.99%	0.996%
60	19.363	2763	2767	2770	rVV	102045	122702	10.66%	0.559%

61	19.398	2770	2773	2779	rVB	55857	68115	5.92%	0.310%
62	19.574	2798	2803	2811	rVB	955095	1128114	98.05%	5.141%
63	19.880	2852	2855	2857	rBV	41311	46109	4.01%	0.210%
64	19.957	2865	2868	2874	rVB5	59704	85055	7.39%	0.388%
65	20.204	2905	2910	2918	rBV5	176043	355509	30.90%	1.620%

66	20.545	2964	2968	2971	rBV3	72904	105969	9.21%	0.483%
67	20.657	2983	2987	2991	rBV2	166388	225465	19.60%	1.027%
68	20.704	2991	2995	3002	rVV	286686	392297	34.10%	1.788%
69	20.774	3005	3007	3012	rVV6	74040	124840	10.85%	0.569%
70	20.833	3012	3017	3020	rVV	705875	938920	81.61%	4.279%

71	20.868	3020	3023	3031	rVB	452578	628996	54.67%	2.866%
72	20.986	3040	3043	3049	rVB4	70956	81700	7.10%	0.372%
73	21.068	3054	3057	3063	rVV	147144	266056	23.12%	1.212%
74	21.133	3063	3068	3071	rVV	459706	624951	54.32%	2.848%
75	21.168	3071	3074	3081	rVB	120371	169586	14.74%	0.773%

76	21.721	3165	3168	3170	rBV	136788	167569	14.56%	0.764%
----	--------	------	------	------	-----	--------	--------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
 Data File : BM031830.D
 Acq On : 19 Aug 2021 16:11
 Operator : CG/JU
 Sample : M3435-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 2021-08-13-FD-04

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	21.751	3170	3173	3181	rVB2	558202	832241	72.34%	3.792%
78	22.651	3321	3326	3330	rBV	314505	463552	40.29%	2.112%
79	22.703	3331	3335	3343	rVB2	336070	565598	49.16%	2.577%
80	22.774	3345	3347	3351	rVB2	93925	104275	9.06%	0.475%
81	23.280	3429	3433	3439	rVB2	291616	493811	42.92%	2.250%
82	23.792	3516	3520	3528	rVB	150380	265856	23.11%	1.211%
83	23.886	3531	3536	3544	rVB2	159399	342582	29.78%	1.561%
84	26.303	3940	3947	3959	rVB4	365139	1038643	90.28%	4.733%
85	26.668	4002	4009	4023	rVB7	321455	1150513	100.00%	5.243%




Sum of corrected areas: 21944943

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031830.D
Acq On : 19 Aug 2021 16:11
Operator : CG/JU
Sample : M3435-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
2021-08-13-FD-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

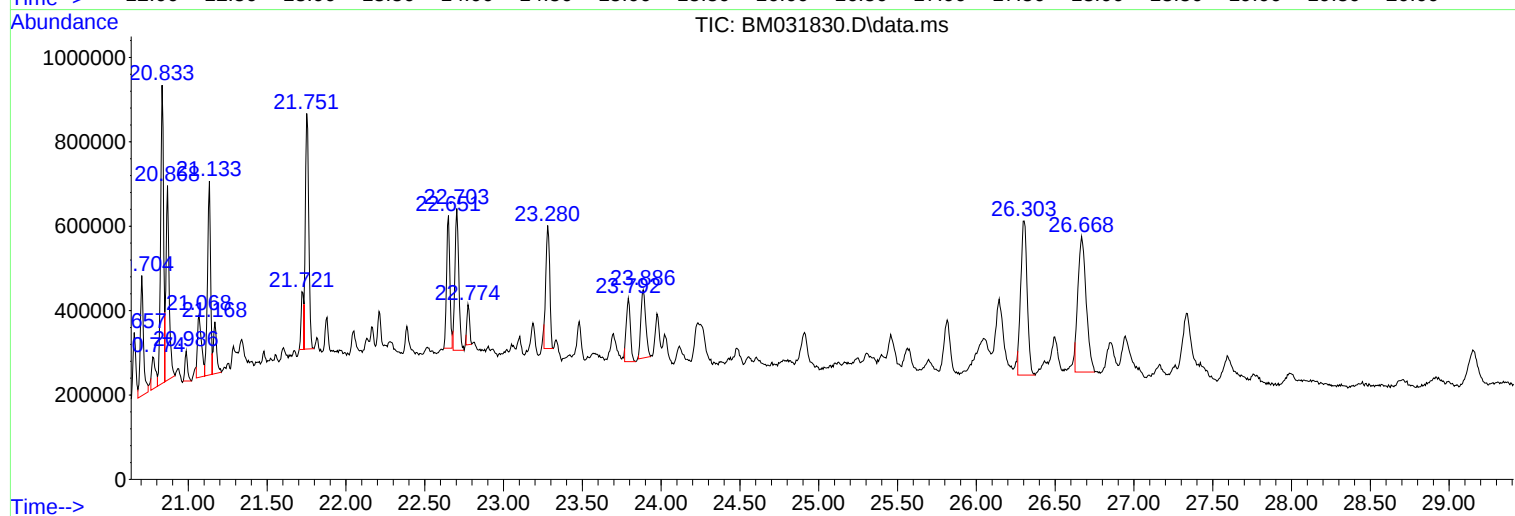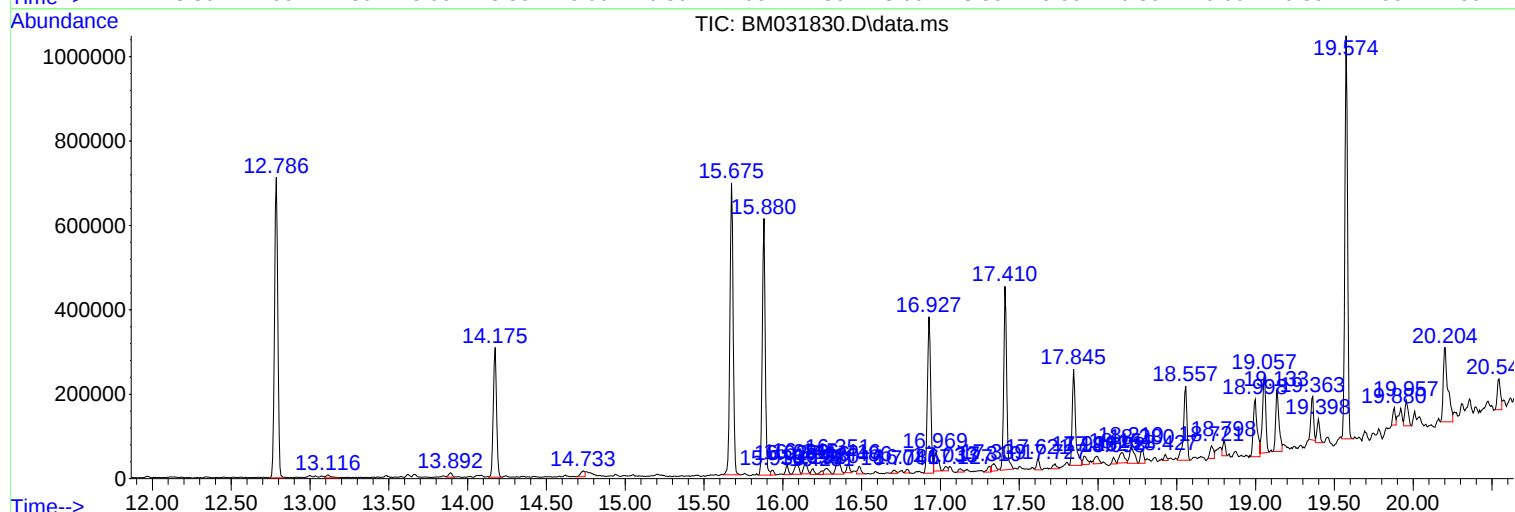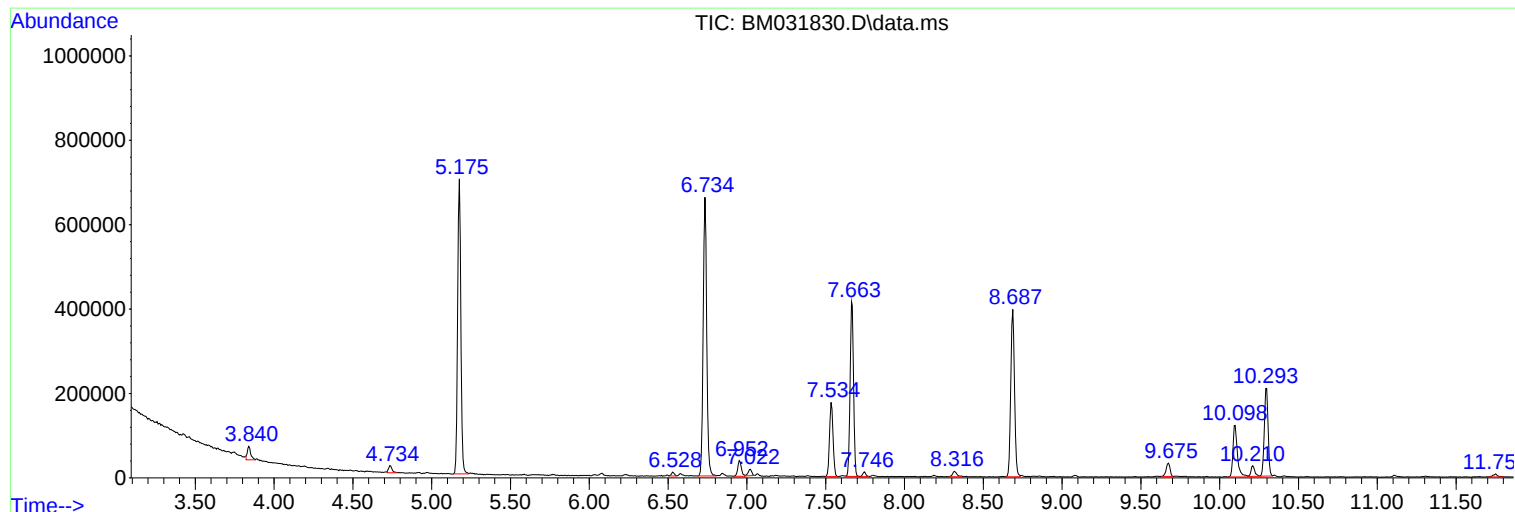

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031830.D
Acq On : 19 Aug 2021 16:11
Operator : CG/JU
Sample : M3435-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
2021-08-13-FD-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031830.D
Acq On : 19 Aug 2021 16:11
Operator : CG/JU
Sample : M3435-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
2021-08-13-FD-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------