


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
 Data File : BM031820.D
 Acq On : 19 Aug 2021 09:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 18 14:13:35 2021

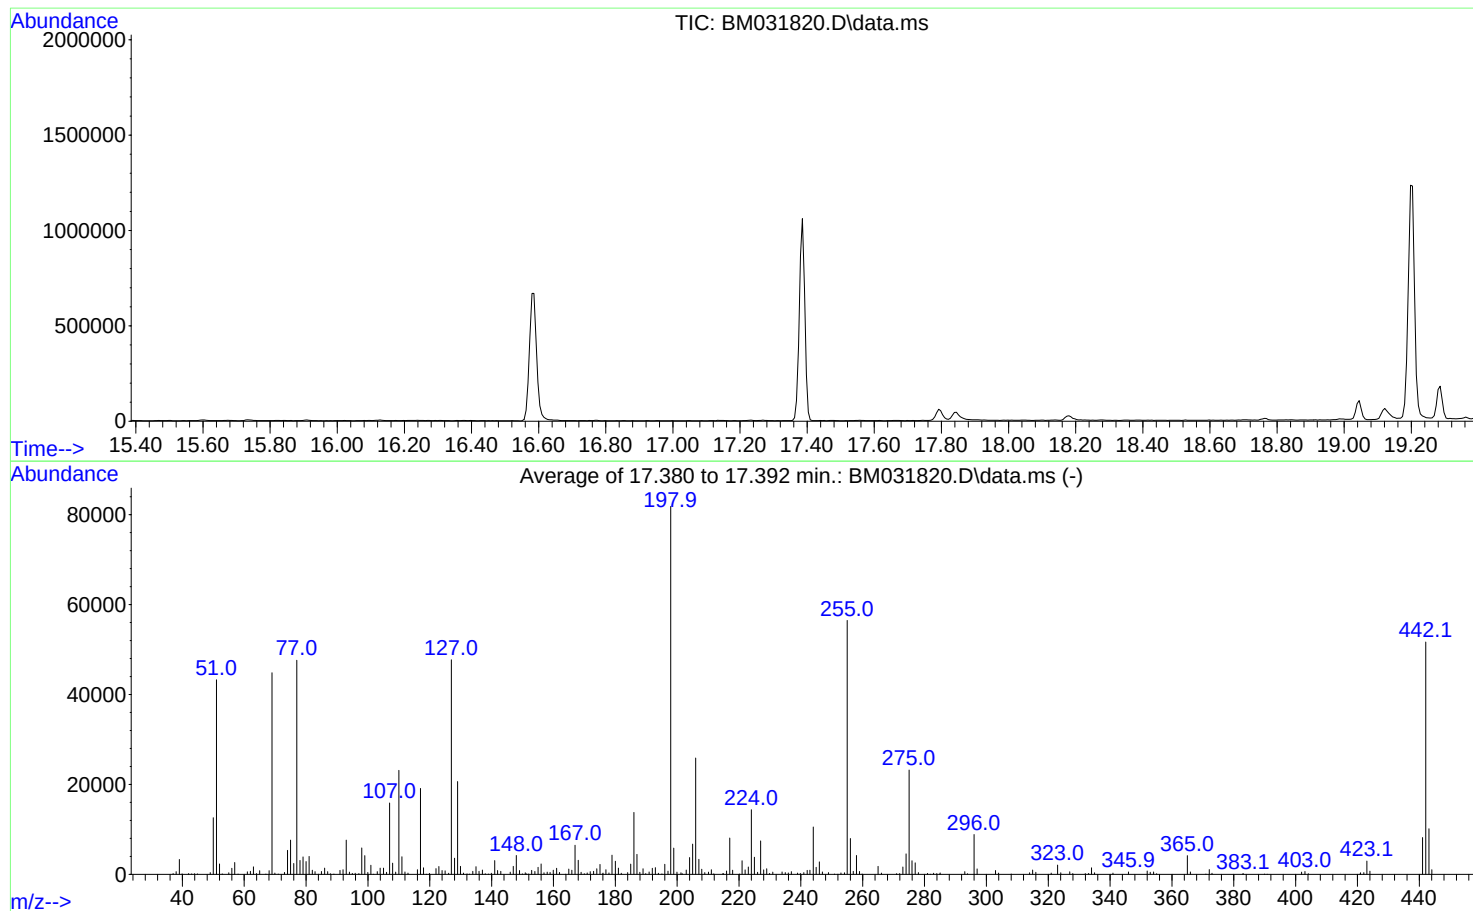




AutoFind: Scans 2430, 2431, 2432; Background Corrected with Scan 2423

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.9	43256	PASS
68	69	0.00	2	1.8	826	PASS
69	198	0.00	100	54.8	44840	PASS
70	69	0.00	2	0.7	297	PASS
127	198	10	80	58.3	47720	PASS
197	198	0.00	2	0.9	730	PASS
198	198	100	100	100.0	81816	PASS
199	198	5	9	7.1	5845	PASS
275	198	10	60	28.4	23197	PASS
365	198	1	100	5.1	4180	PASS
441	198	0.01	100	10.0	8183	PASS
442	442	50	100	100.0	51685	PASS
443	442	15	24	19.6	10137	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031820.D
Acq On : 19 Aug 2021 09:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 19 11:48:54 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 18 14:13:35 2021
Response via : Initial Calibration

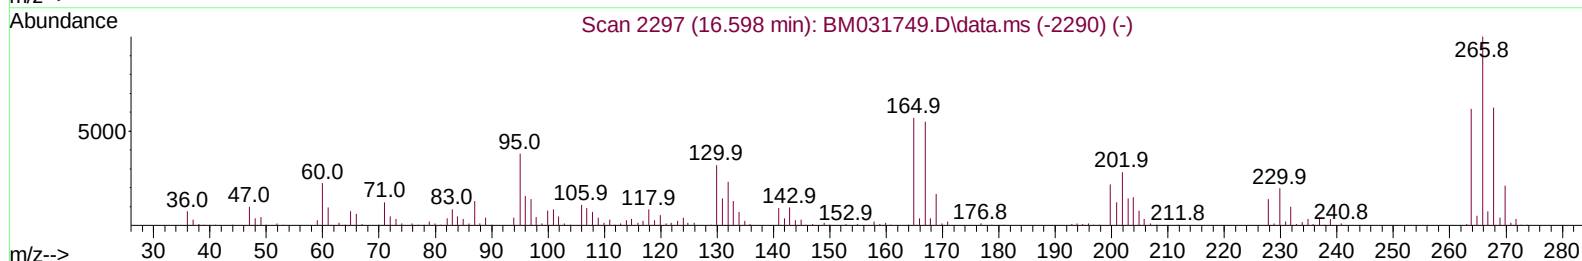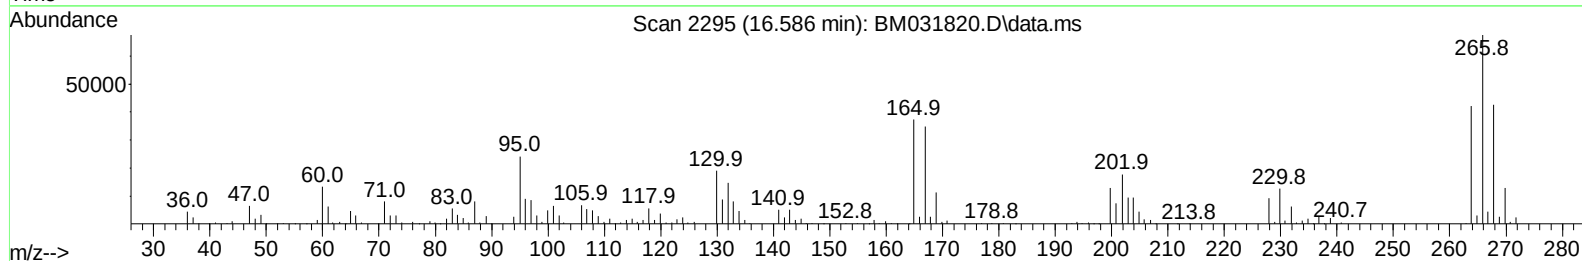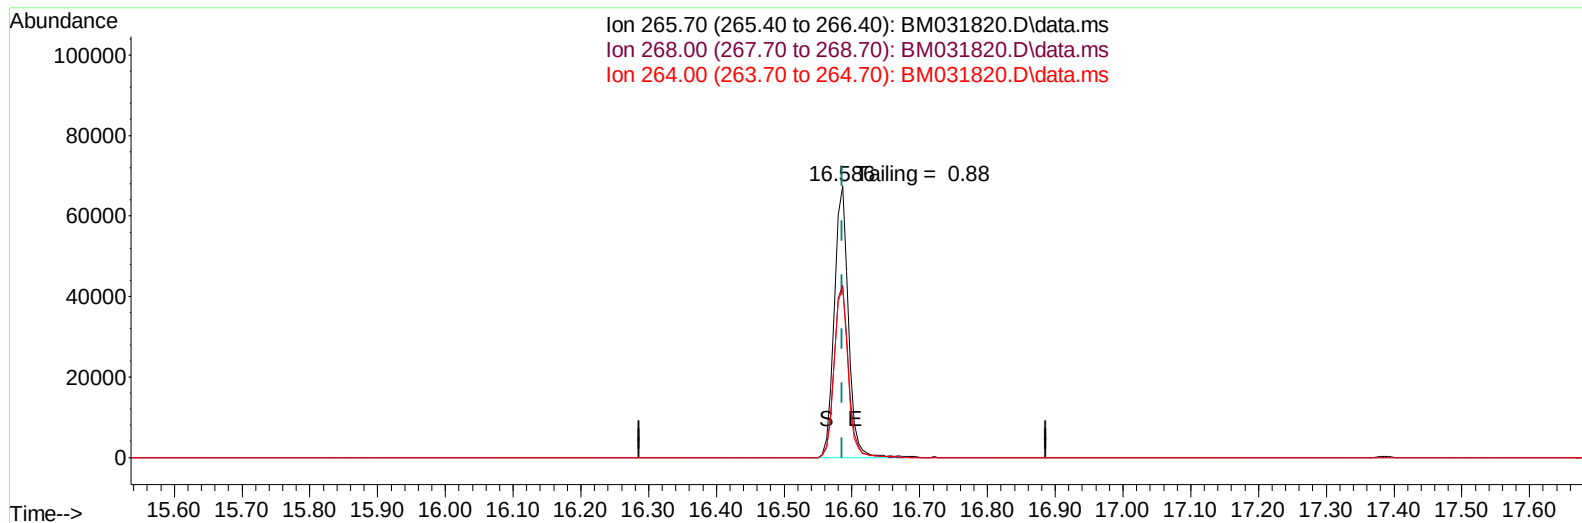

TIC: BM031820.D\data.ms

(70) Pentachlorophenol (C)

16.586min (-0.000) 0.00 ng




response 97116

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	63.22
264.00	64.90	62.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031820.D
Acq On : 19 Aug 2021 09:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 19 11:48:54 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 18 14:13:35 2021
Response via : Initial Calibration

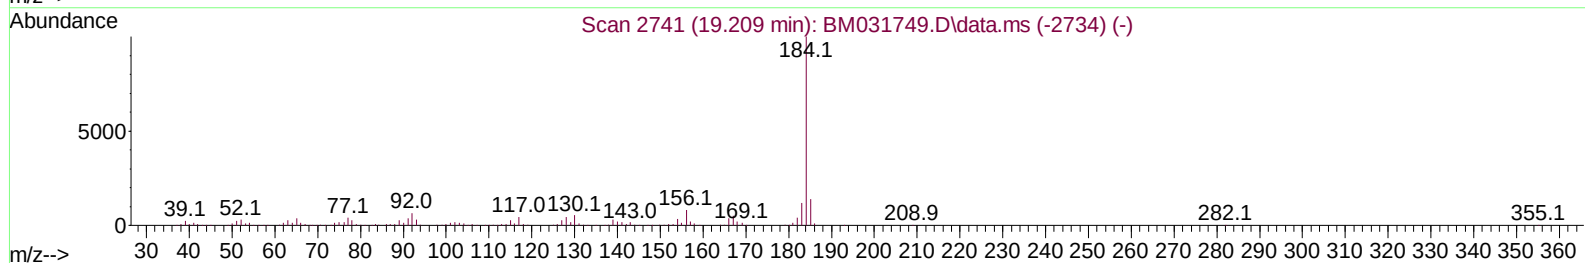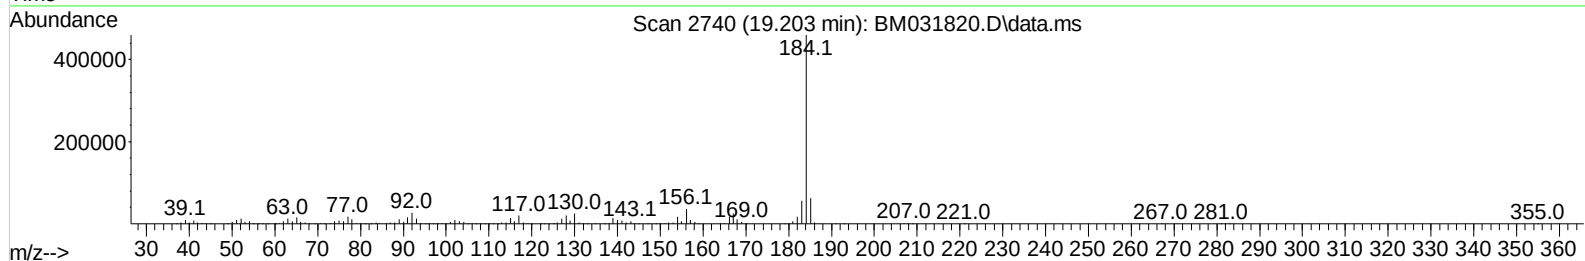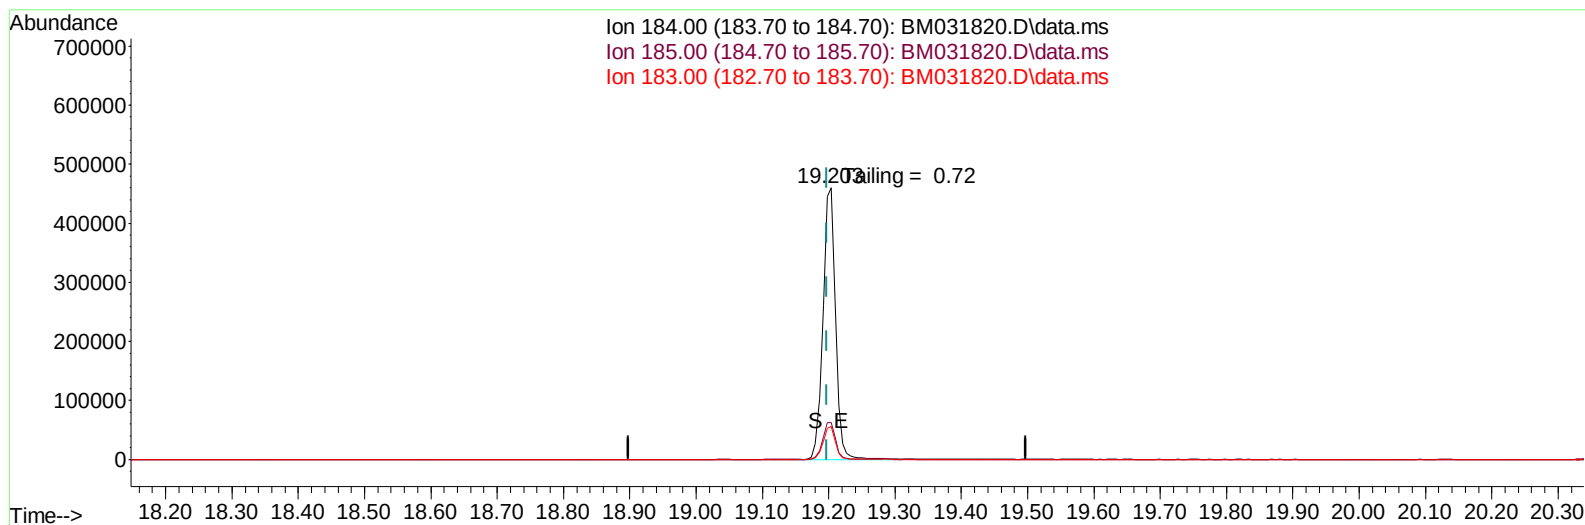

TIC: BM031820.D\data.ms

(77) Benzidine

19.203min (+ 0.006) 54312.25 ng

response 611707

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.63
183.00	12.30	12.11
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_M
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
8/19/2021	BNA_M	<u>BM031820.D</u>
Compound Name	Response	Retention Time
DDT	353178	20.43
DDD	912	19.99
DDE	386	19.48
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1298	354476	0.37