

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081922\
 Data File : BM036353.D
 Acq On : 19 Aug 2022 11:16
 Operator : CG/JU
 Sample : PB146666BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK666

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036353.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.204	17	20	34	rVB	74756	97512	2.17%	0.192%
2	3.628	89	92	117	rBV	598847	956605	21.32%	1.881%
3	3.951	143	147	153	rVB	17852	26694	0.59%	0.053%
4	6.969	654	660	675	rBV	877846	1446808	32.24%	2.845%
5	7.128	681	687	700	rBV	765388	1227817	27.36%	2.415%
6	7.322	713	720	732	rBV	933467	1493420	33.28%	2.937%
7	7.792	790	800	809	rBV	812075	1289652	28.74%	2.536%
8	8.516	916	923	939	rBV	1060695	1798925	40.09%	3.538%
9	8.963	992	999	1010	rBV	894975	1466253	32.67%	2.884%
10	9.680	1114	1121	1138	rBV	677409	1173799	26.16%	2.309%
11	10.222	1204	1213	1236	rBV	965512	1760411	39.23%	3.462%
12	10.592	1269	1276	1287	rBV	1169530	1902787	42.40%	3.742%
13	10.745	1295	1302	1329	rBV	903569	1759524	39.21%	3.461%
14	11.957	1502	1508	1510	rBV5	2154	4606	0.10%	0.009%
15	12.204	1543	1550	1559	rBV	12313	27192	0.61%	0.053%
16	13.415	1752	1756	1761	rVB6	2940	5164	0.12%	0.010%
17	13.857	1824	1831	1844	rBV	1830236	2545395	56.72%	5.006%
18	14.133	1871	1878	1891	rBV	2124242	3128454	69.71%	6.153%
19	14.439	1923	1930	1938	rBV	1626819	2378022	52.99%	4.677%
20	14.498	1938	1940	1945	rVB5	6691	8965	0.20%	0.018%
21	14.668	1963	1969	1995	rBV	432658	1055396	23.52%	2.076%
22	15.433	2089	2099	2105	rBV	2627575	3813874	84.99%	7.501%
23	15.562	2115	2121	2136	rBV	615269	971399	21.65%	1.910%
24	15.674	2136	2140	2152	rVV4	29655	60710	1.35%	0.119%
25	15.774	2154	2157	2161	rVB4	3096	4488	0.10%	0.009%
26	16.215	2229	2232	2236	rVB4	5916	8218	0.18%	0.016%
27	16.645	2301	2305	2309	rBV6	4730	6351	0.14%	0.012%
28	16.862	2338	2342	2346	rVB5	3195	5058	0.11%	0.010%
29	17.180	2390	2396	2406	rBV	1875214	2487704	55.43%	4.893%
30	17.280	2407	2413	2432	rVB	2941423	3923778	87.44%	7.717%
31	17.780	2495	2498	2503	rBV4	3266	7254	0.16%	0.014%
32	17.850	2506	2510	2514	rBV7	5207	10160	0.23%	0.020%
33	18.150	2559	2561	2564	rBV3	5208	5689	0.13%	0.011%
34	18.656	2644	2647	2652	rBV6	4323	8861	0.20%	0.017%
35	19.139	2725	2729	2735	rBV3	28631	43924	0.98%	0.086%
36	19.209	2738	2741	2745	rBV2	24097	30779	0.69%	0.061%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081922\
Data File : BM036353.D
Acq On : 19 Aug 2022 11:16
Operator : CG/JU
Sample : PB146666BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK666

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Title : SVOA CALIBRATION

37	19.574	2797	2803	2814	rBV	3257775	4244984	94.59%	8.349%
38	20.574	2970	2973	2979	rBV	114211	142133	3.17%	0.280%
39	21.368	3103	3108	3120	rBV	1853931	2513896	56.02%	4.944%
40	23.544	3471	3478	3493	rBV2	2156336	4487640	100.00%	8.826%
41	23.691	3497	3503	3515	rVB2	1240184	2515205	56.05%	4.947%




Sum of corrected areas: 50845506

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081922\
Data File : BM036353.D
Acq On : 19 Aug 2022 11:16
Operator : CG/JU
Sample : PB146666BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK666

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

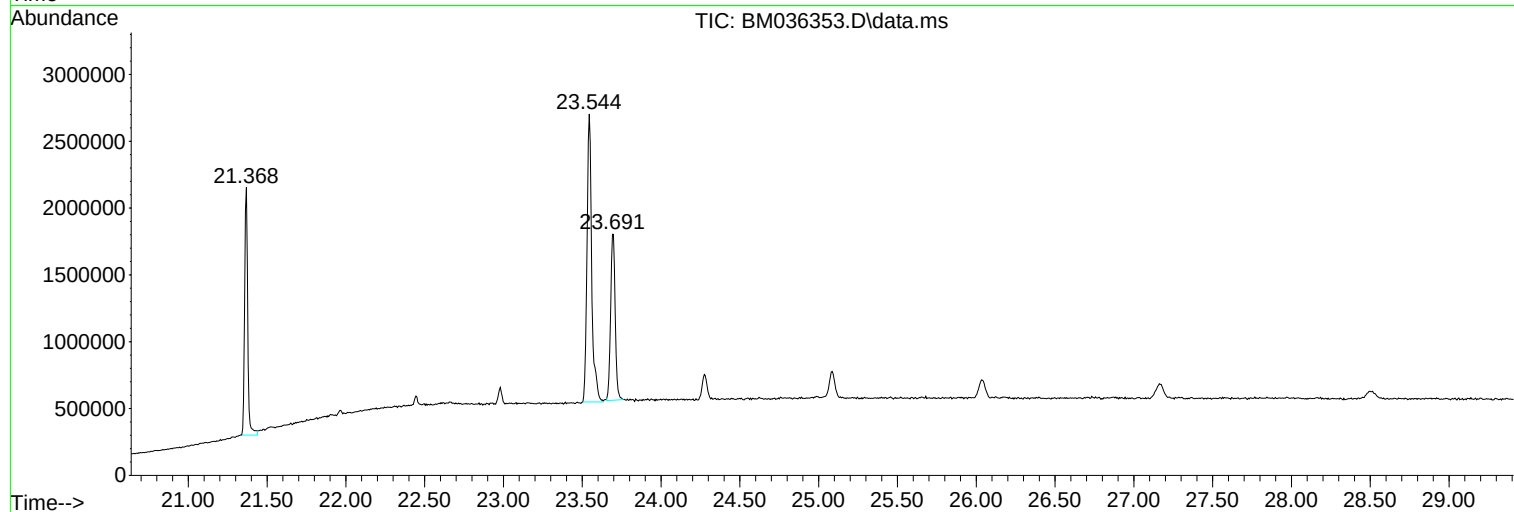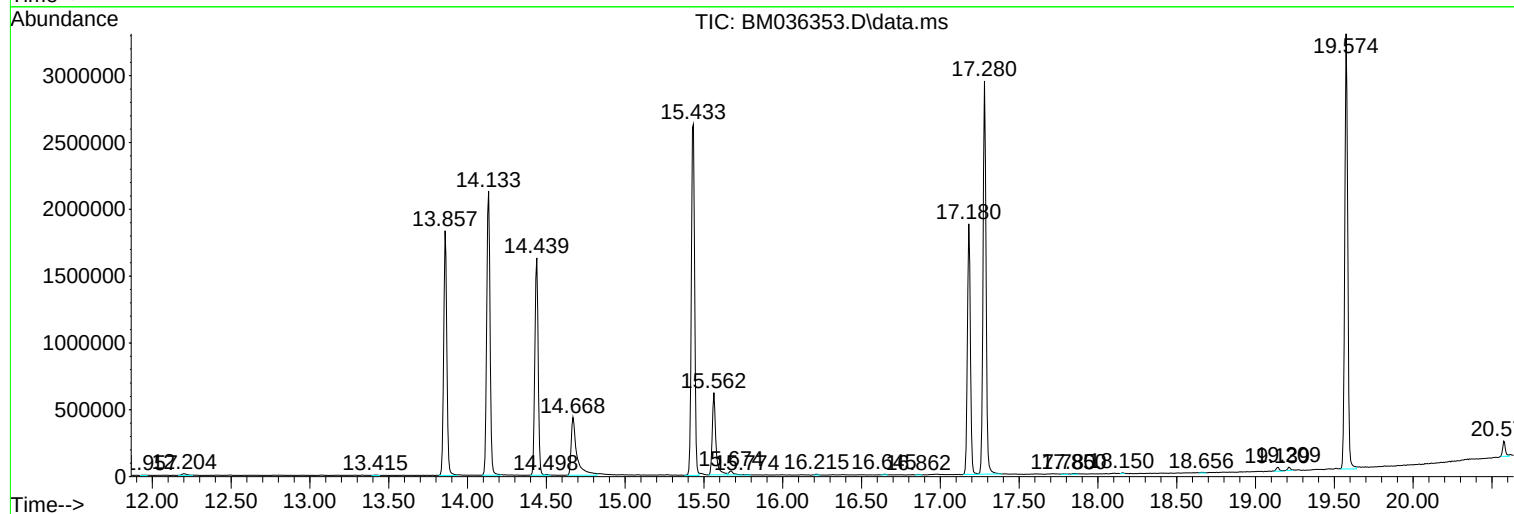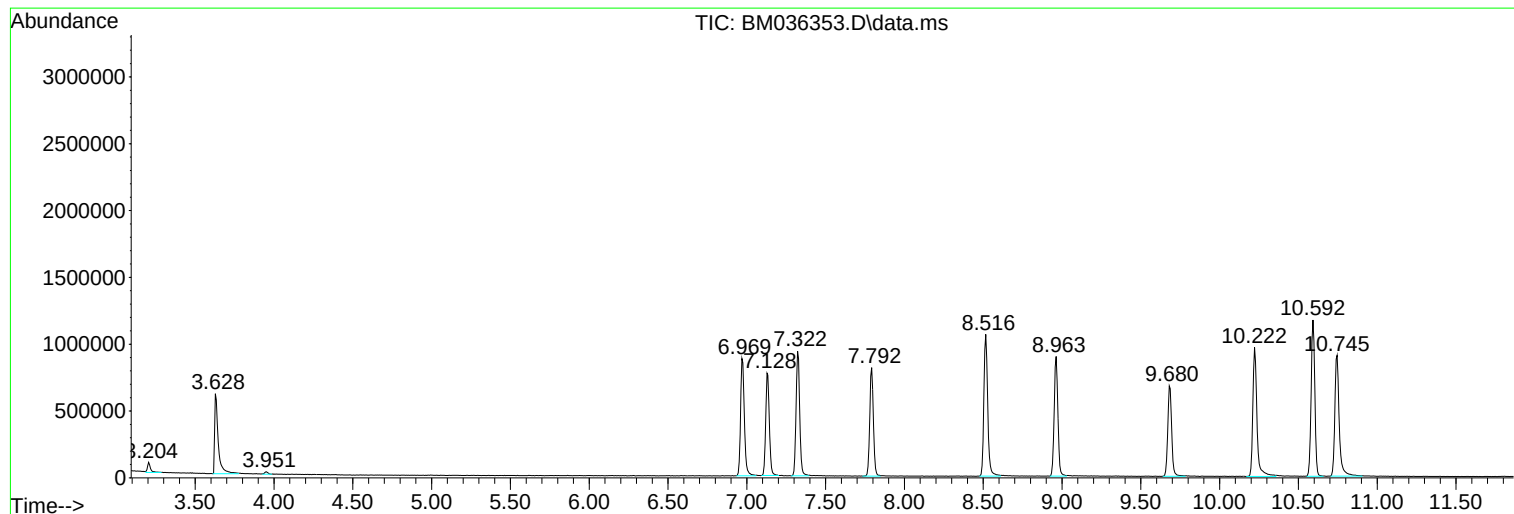

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081922\
Data File : BM036353.D
Acq On : 19 Aug 2022 11:16
Operator : CG/JU
Sample : PB146666BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK666

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081922\
Data File : BM036353.D
Acq On : 19 Aug 2022 11:16
Operator : CG/JU
Sample : PB146666BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK666

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc