
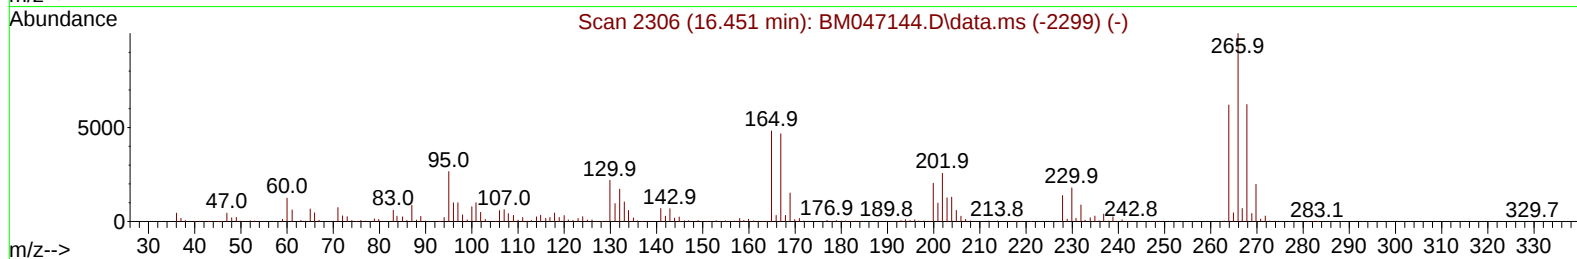
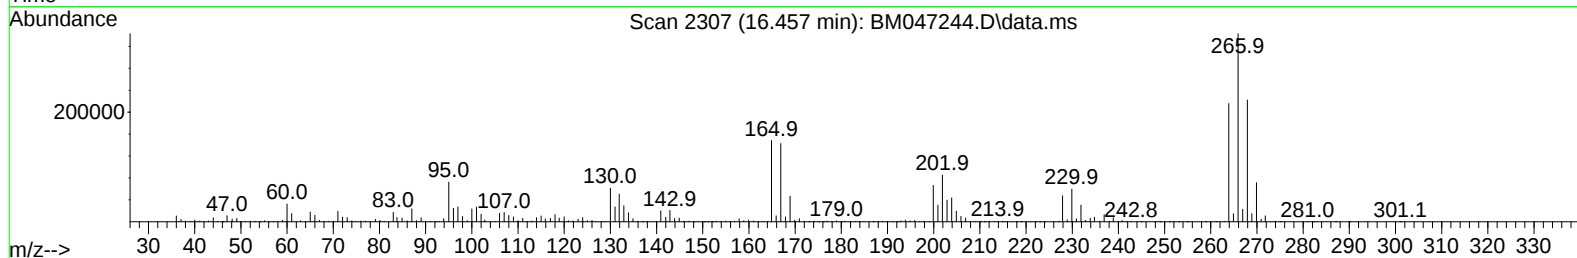


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081924\
Data File : BM047244.D
Acq On : 19 Aug 2024 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 11:15:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

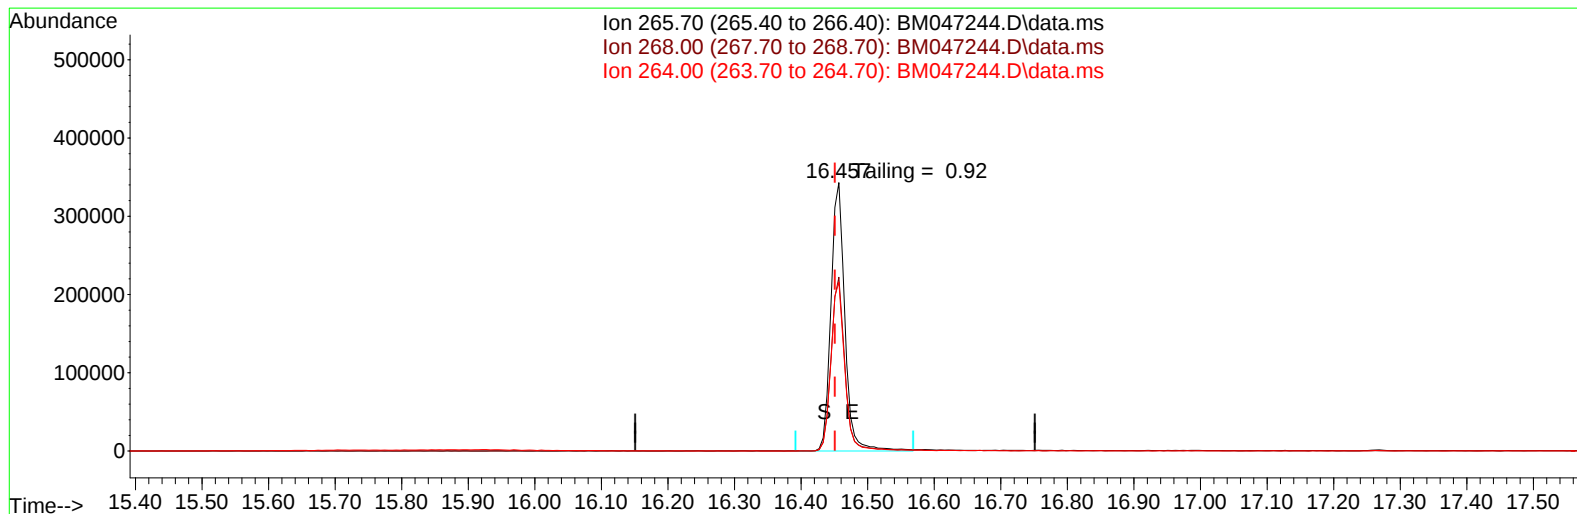

TIC: BM047244.D\data.ms

(70) Pentachlorophenol (C)




16.457min (+ 0.006) 216859.29 ng

response 499995

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.77
264.00	62.00	62.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081924\
Data File : BM047244.D
Acq On : 19 Aug 2024 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 11:15:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

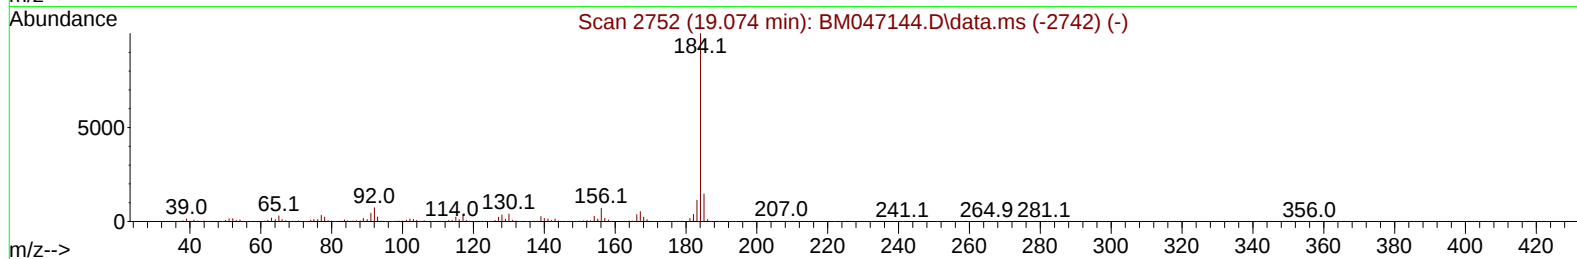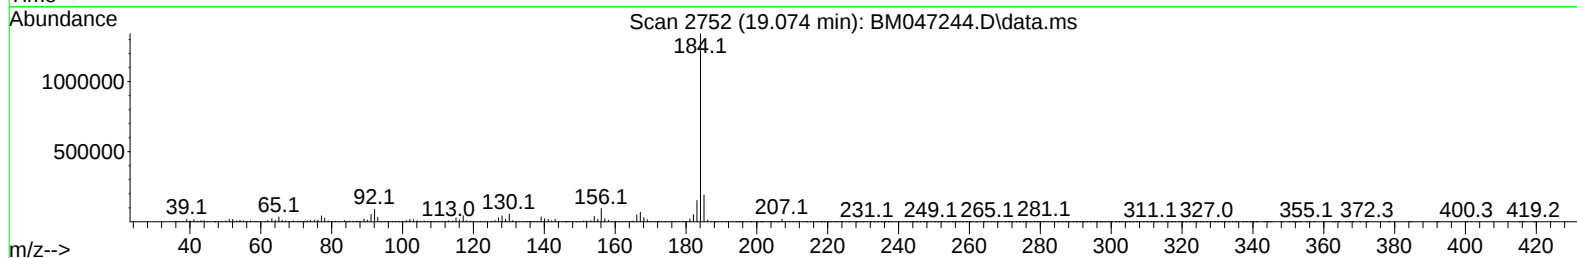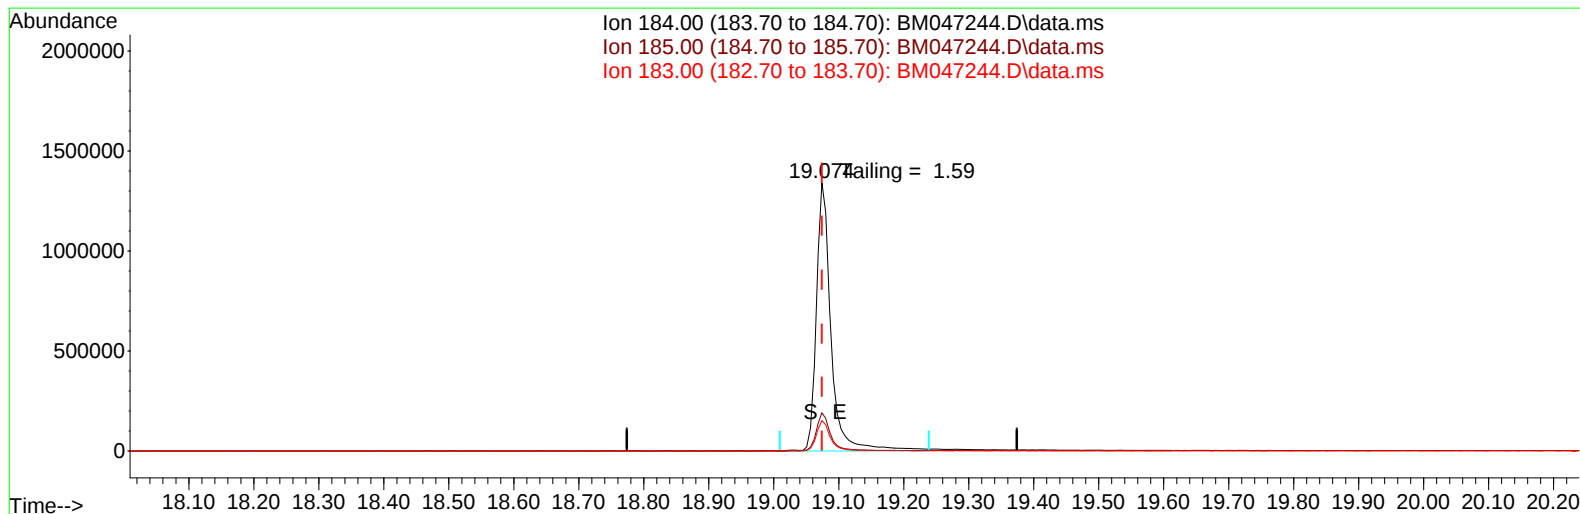

TIC: BM047244.D\data.ms

(77) Benzidine

19.074min (-0.000) 40695.55 ng m

response 2114570

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.26
183.00	11.30	11.34
0.00	0.00	0.00