
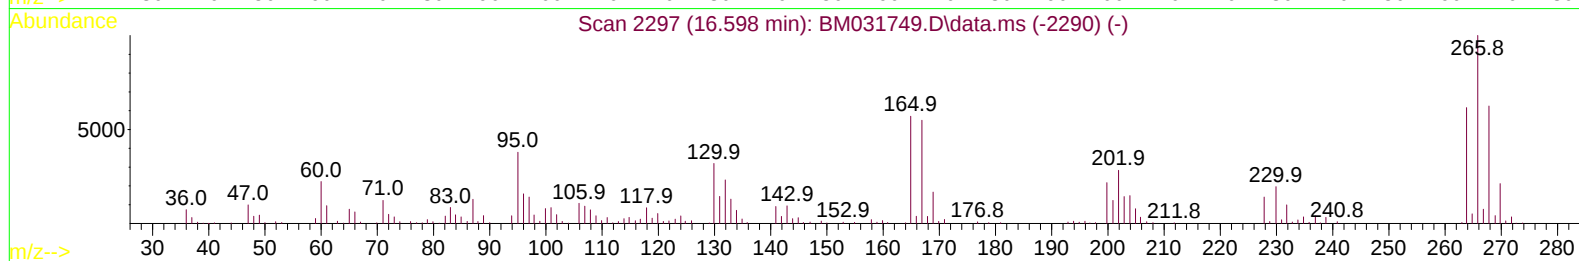
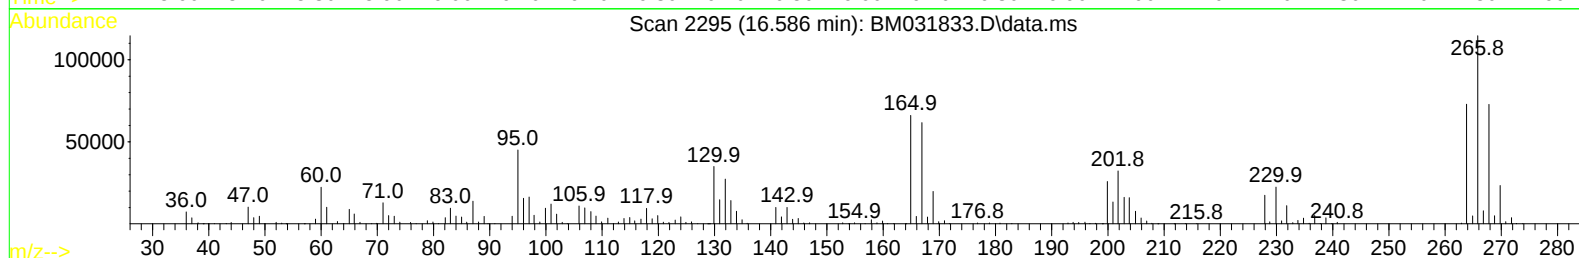


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031833.D
Acq On : 20 Aug 2021 08:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 11:05:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 18 14:13:35 2021
Response via : Initial Calibration

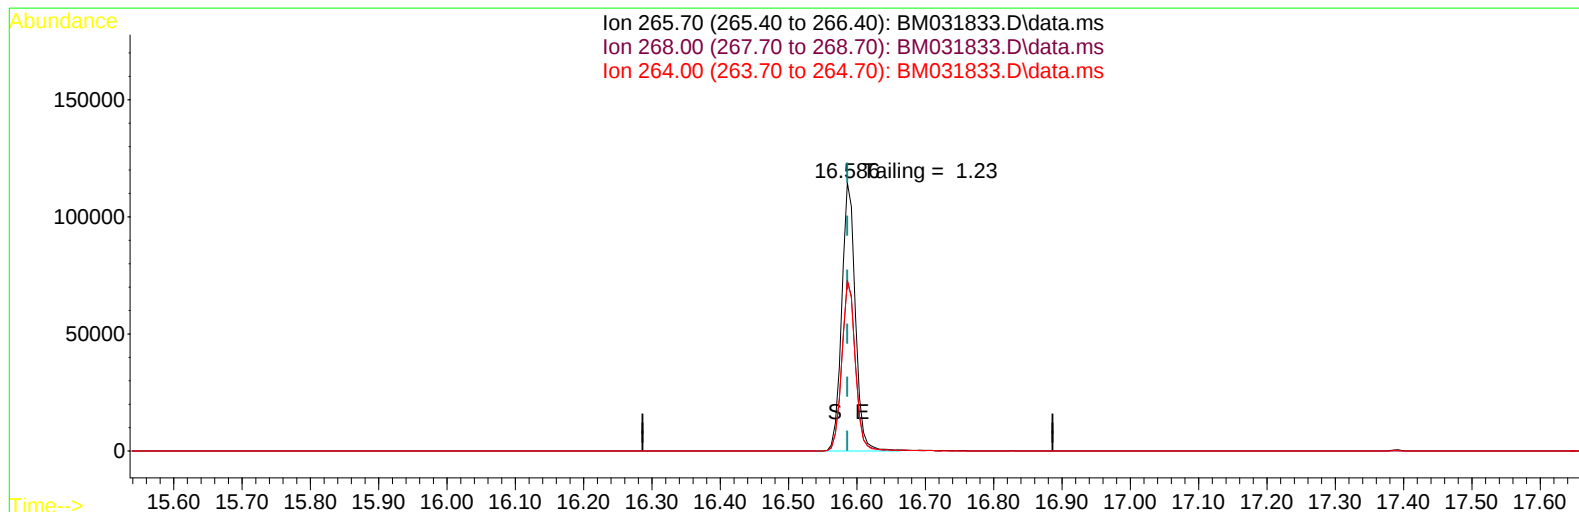

TIC: BM031833.D\data.ms

(70) Pentachlorophenol (C)




16.586min (-0.000) 175864.21 ng

response 158174

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	63.53
264.00	64.90	63.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031833.D
 Acq On : 20 Aug 2021 08:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 11:05:31 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 18 14:13:35 2021
 Response via : Initial Calibration

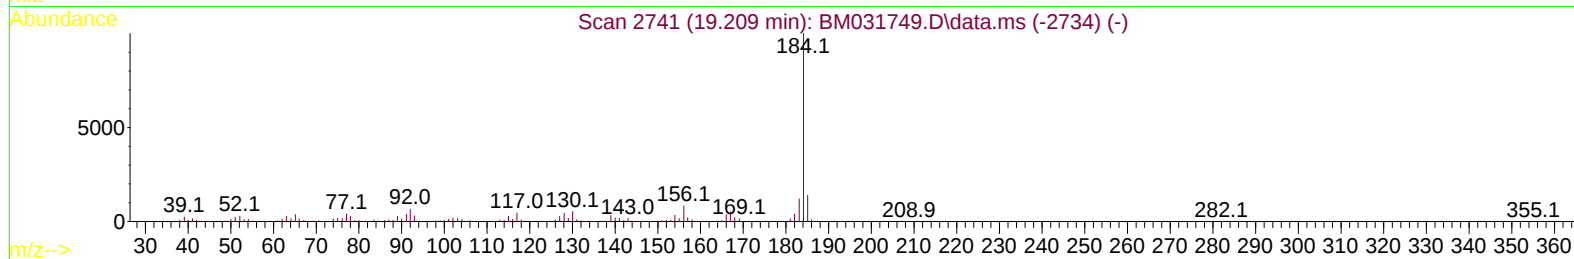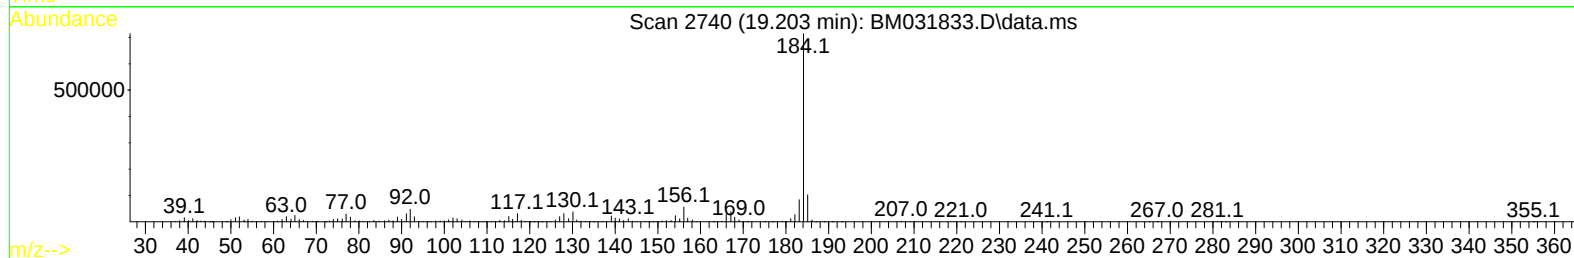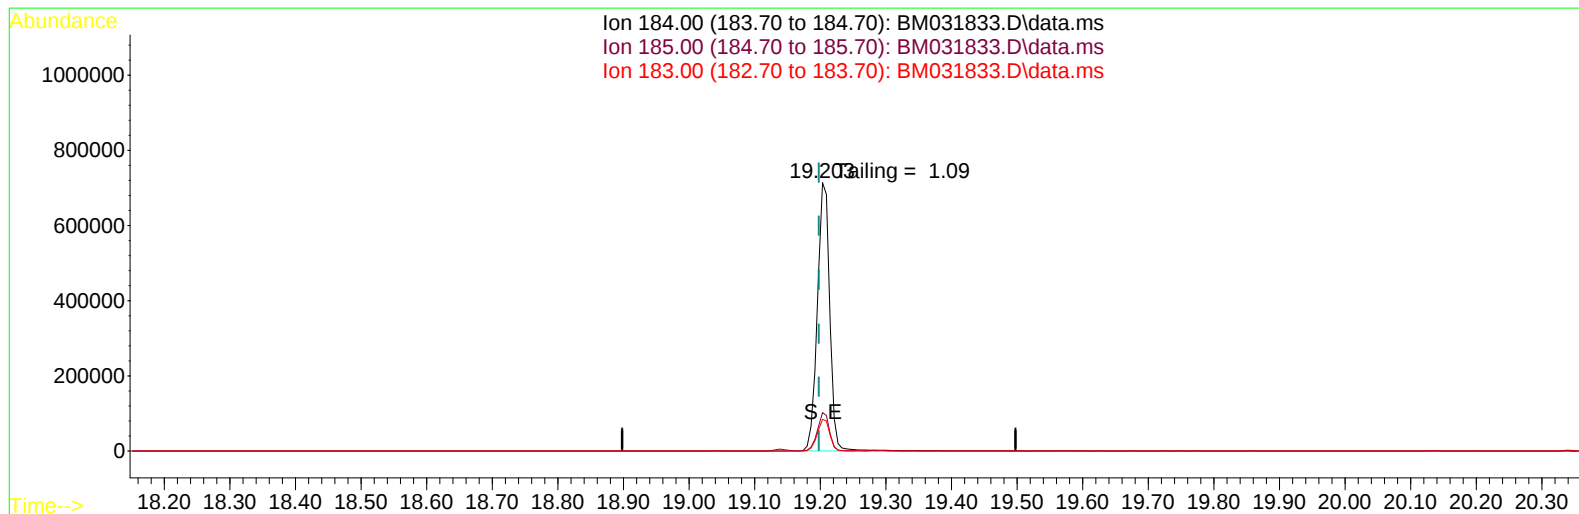

TIC: BM031833.D\data.ms

(77) Benzidine**19.203min (+ 0.006) 215966.00 ng****response 937011**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.30
183.00	12.30	11.80
0.00	0.00	0.00