
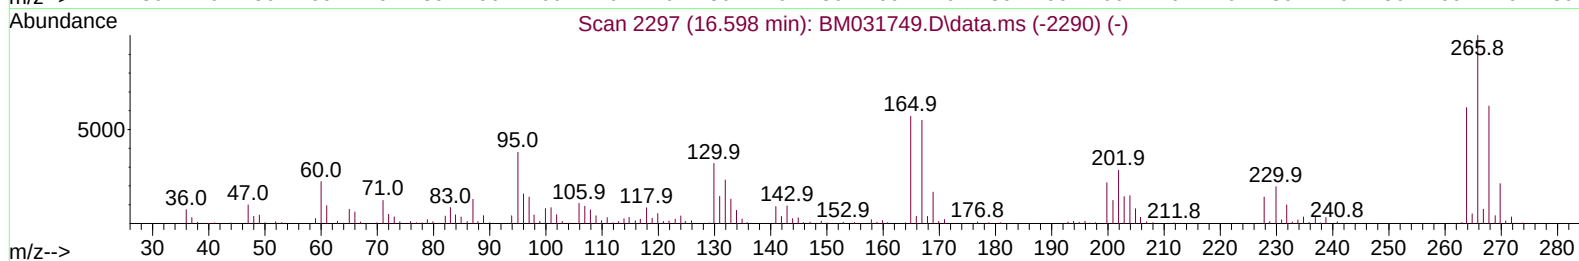
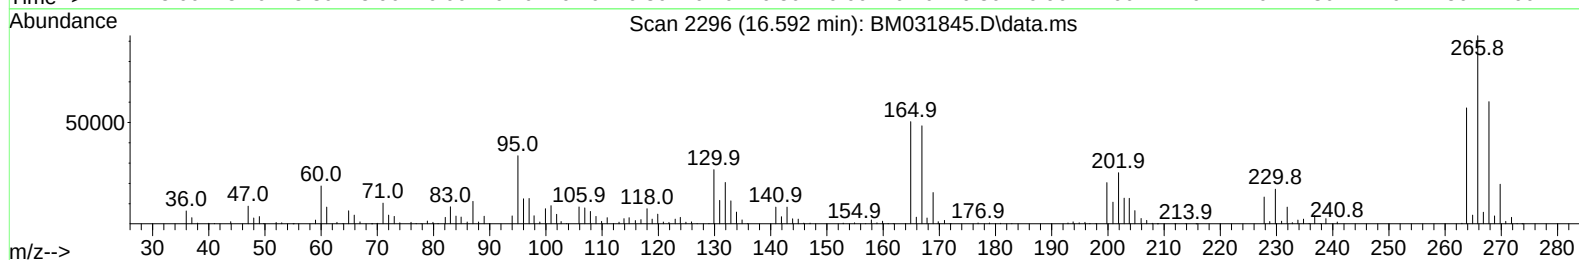


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031845.D
Acq On : 20 Aug 2021 17:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 08:08:02 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 18 14:13:35 2021
Response via : Initial Calibration

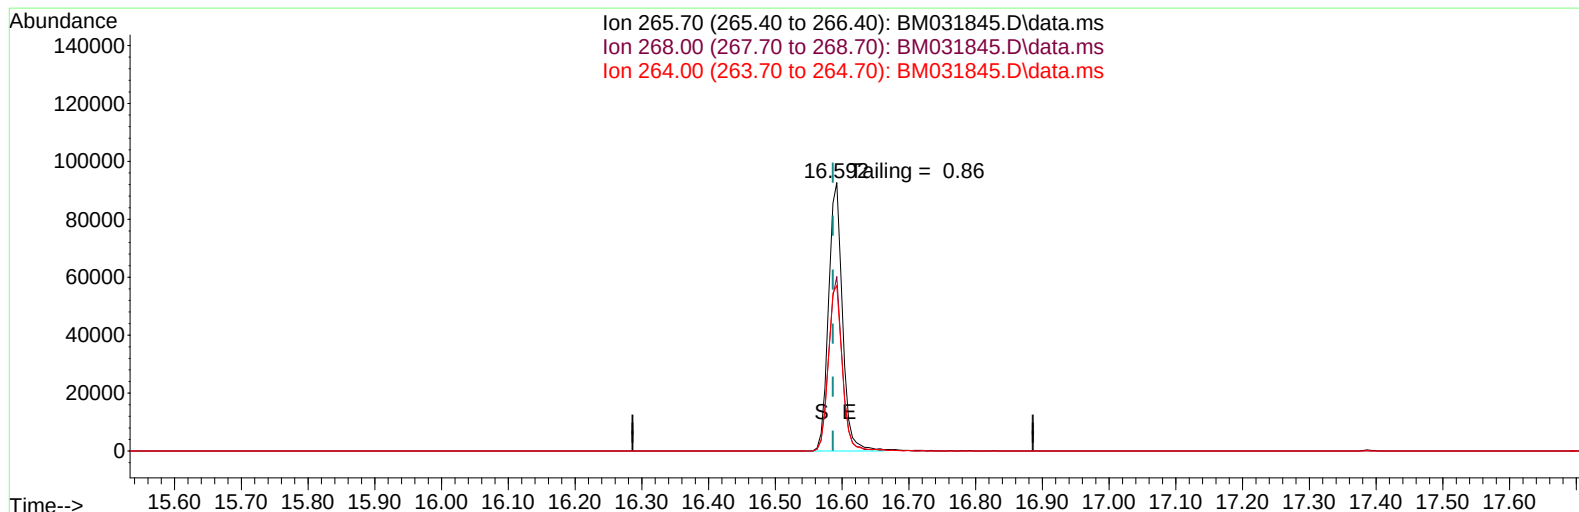

TIC: BM031845.D\data.ms

(70) Pentachlorophenol (C)




16.592min (+ 0.006) 0.00 ng

response 135237

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	65.02
264.00	64.90	61.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031845.D
Acq On : 20 Aug 2021 17:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 08:08:02 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 18 14:13:35 2021
Response via : Initial Calibration

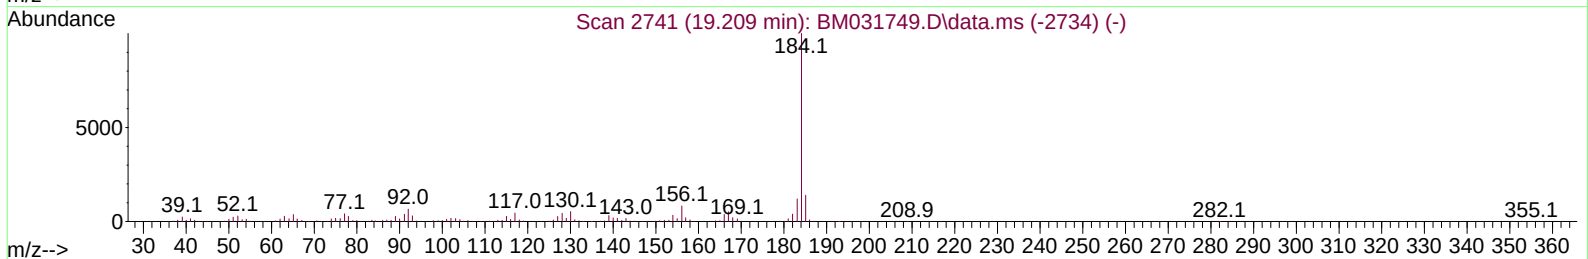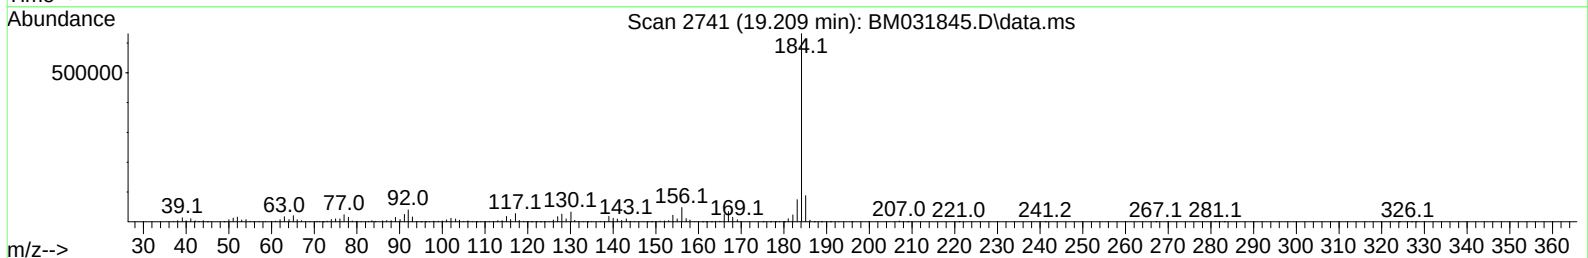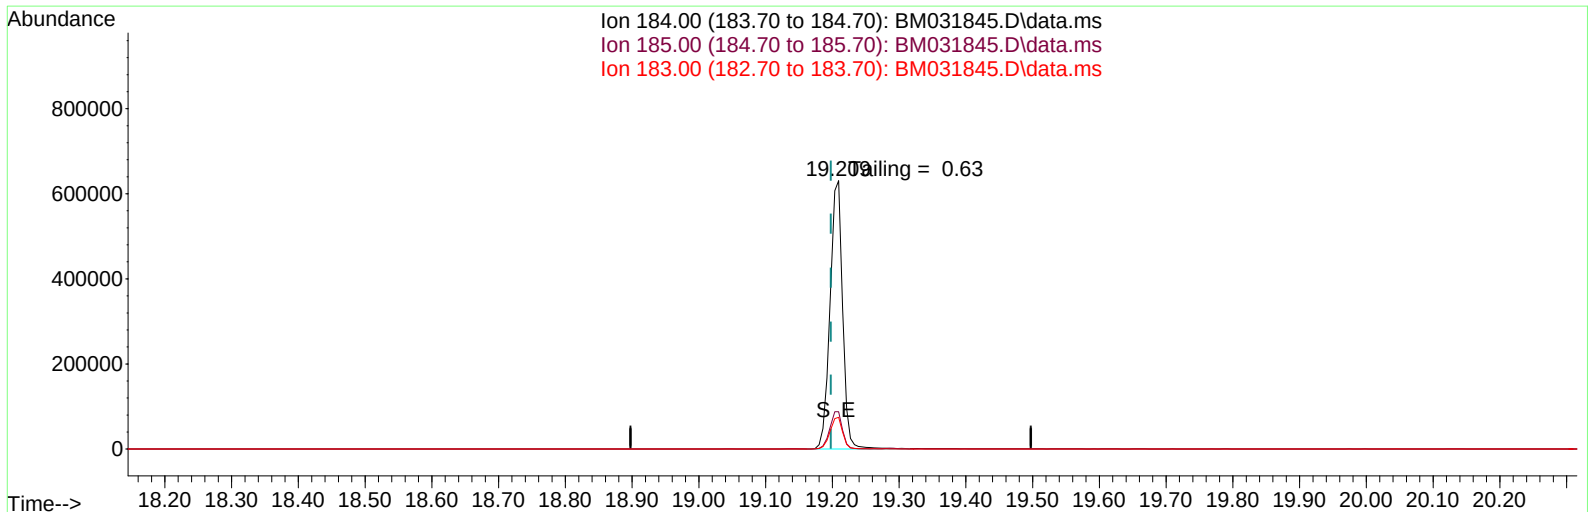

TIC: BM031845.D\data.ms

(77) Benzidine**19.209min (+ 0.012) 85280.31 ng****response 831245**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.91
183.00	12.30	11.81
0.00	0.00	0.00