

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031835.D
 Acq On : 20 Aug 2021 10:45
 Operator : CG/JU
 Sample : PB138504BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB138504BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031835.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.740	277	281	287	rVB	30357	40652	1.43%	0.290%
2	5.175	349	355	366	rBV	1168054	1653473	58.02%	11.781%
3	6.740	613	621	634	rBV	1105436	1730887	60.73%	12.332%
4	7.540	750	757	764	rVB	187882	290392	10.19%	2.069%
5	8.692	942	953	963	rBV	649666	1085103	38.07%	7.731%
6	10.298	1219	1226	1237	rBV	233723	391237	13.73%	2.788%
7	12.786	1642	1649	1663	rBV	1518396	2271886	79.72%	16.187%
8	14.174	1879	1885	1893	rBV	339104	499863	17.54%	3.561%
9	15.674	2134	2140	2159	rVB	1133525	1678654	58.90%	11.960%
10	16.933	2347	2354	2363	rBV	387648	552637	19.39%	3.937%
11	19.580	2798	2804	2809	rBV	2332024	2849954	100.00%	20.306%
12	21.133	3063	3068	3076	rBV	383691	500753	17.57%	3.568%
13	23.280	3427	3433	3444	rVB2	259101	489806	17.19%	3.490%




Sum of corrected areas: 14035297

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031835.D
Acq On : 20 Aug 2021 10:45
Operator : CG/JU
Sample : PB138504BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138504BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

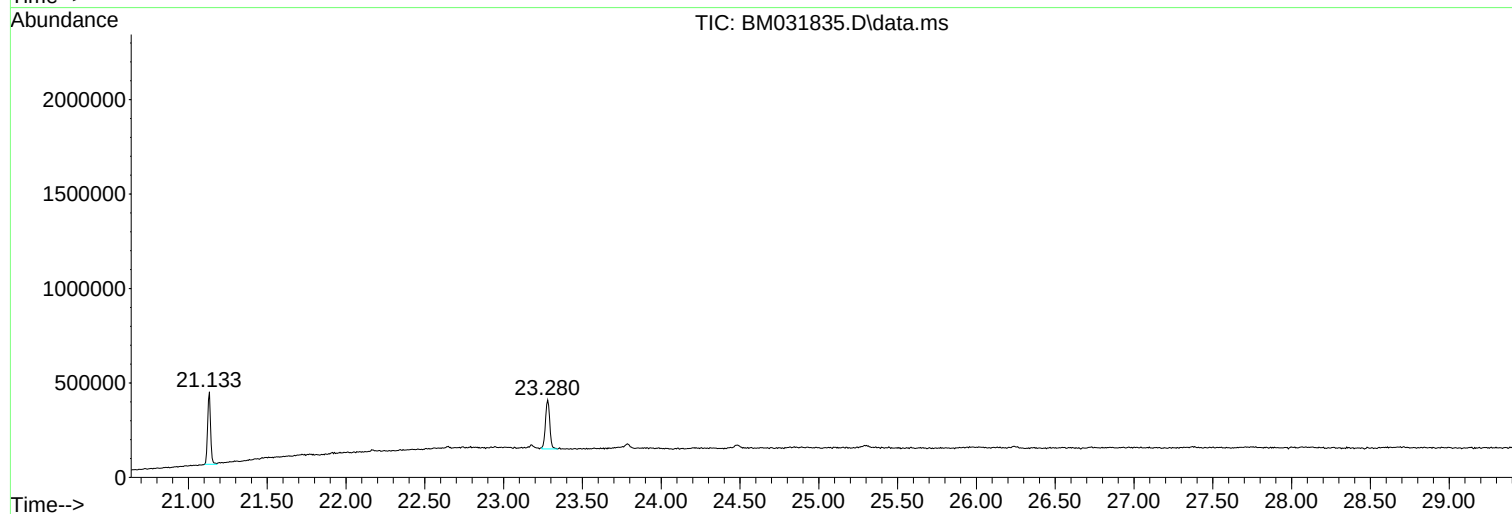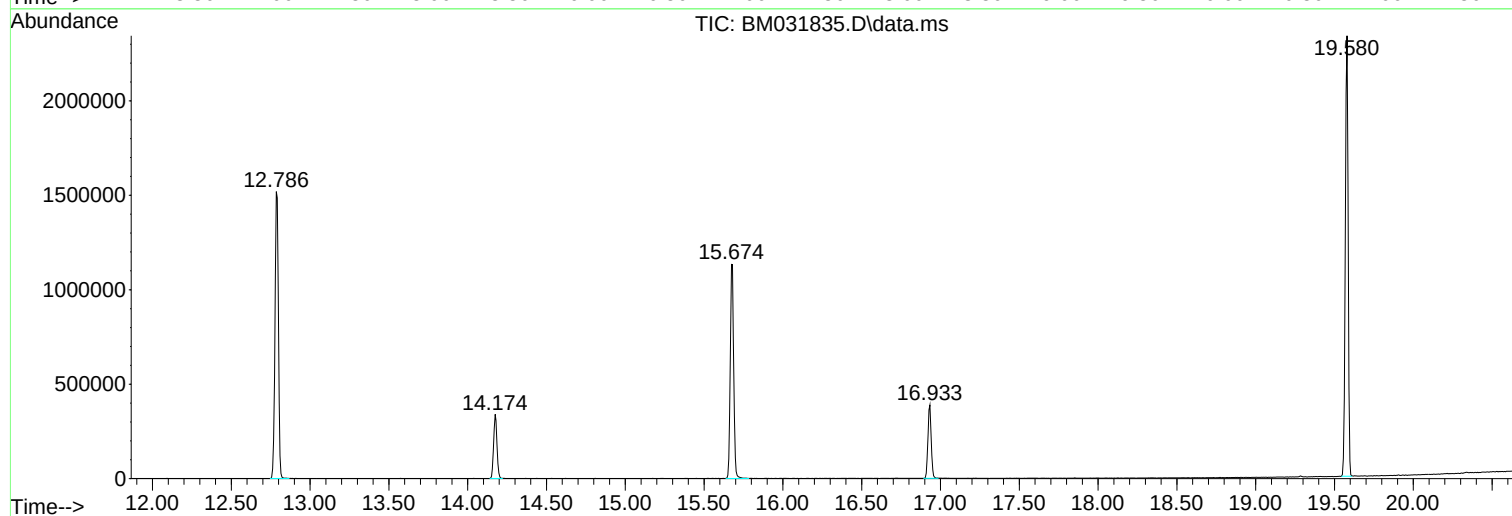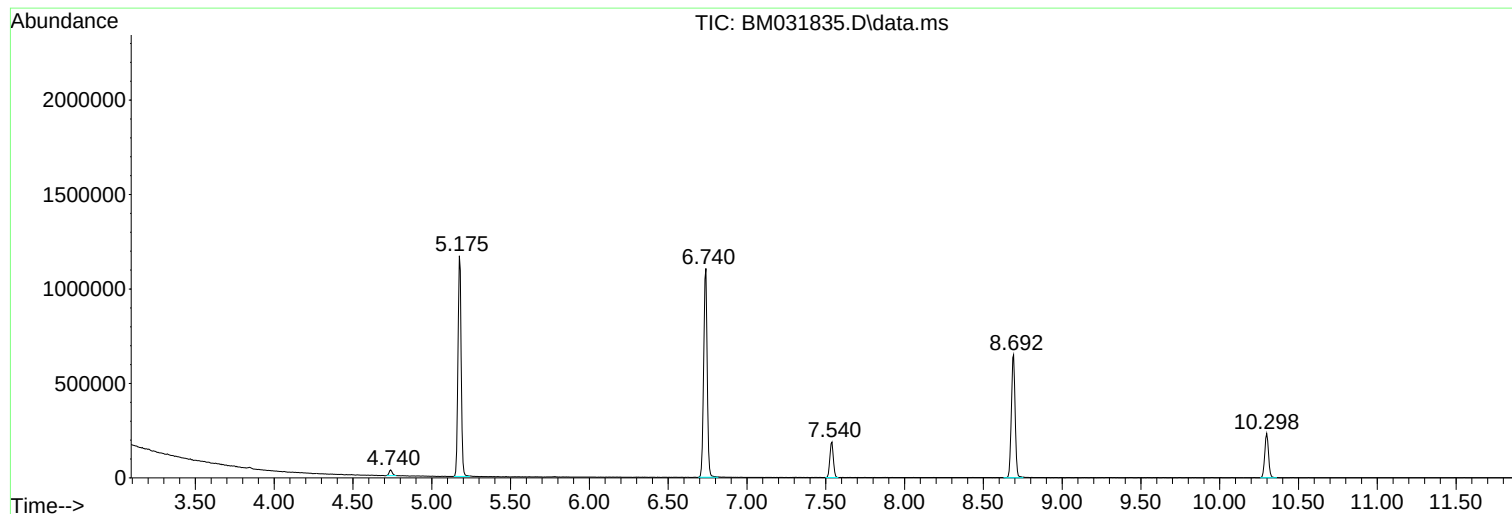

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031835.D
Acq On : 20 Aug 2021 10:45
Operator : CG/JU
Sample : PB138504BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138504BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031835.D
Acq On : 20 Aug 2021 10:45
Operator : CG/JU
Sample : PB138504BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138504BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------