

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM082021\  
 Data File : BM031836.D  
 Acq On : 20 Aug 2021 11:32  
 Operator : CG/JU  
 Sample : M3434-23  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SWCS-13-1015

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM081621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031836.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.734       | 275           | 280         | 285          | rVB      | 21502          | 31225         | 2.69%           | 0.264%        |
| 2         | 5.169       | 348           | 354         | 363          | rBV      | 574465         | 828491        | 71.29%          | 7.003%        |
| 3         | 6.728       | 613           | 619         | 630          | rBV      | 519897         | 831808        | 71.57%          | 7.031%        |
| 4         | 7.534       | 749           | 756         | 762          | rVB      | 170353         | 259687        | 22.34%          | 2.195%        |
| 5         | 7.846       | 802           | 809         | 816          | rVB      | 101065         | 153979        | 13.25%          | 1.302%        |
| 6         | 8.687       | 944           | 952         | 962          | rBV      | 393359         | 657653        | 56.59%          | 5.559%        |
| 7         | 10.104      | 1187          | 1193        | 1198         | rBV3     | 11685          | 22877         | 1.97%           | 0.193%        |
| 8         | 10.293      | 1218          | 1225        | 1232         | rBV      | 202136         | 325411        | 28.00%          | 2.751%        |
| 9         | 12.781      | 1642          | 1648        | 1660         | rVB      | 665043         | 1001639       | 86.19%          | 8.466%        |
| 10        | 14.169      | 1878          | 1884        | 1892         | rVB      | 261692         | 392627        | 33.78%          | 3.319%        |
| 11        | 14.622      | 1955          | 1961        | 1969         | rBV2     | 38588          | 65120         | 5.60%           | 0.550%        |
| 12        | 15.433      | 2094          | 2099        | 2110         | rBV4     | 6442           | 17192         | 1.48%           | 0.145%        |
| 13        | 15.675      | 2133          | 2140        | 2149         | rBV      | 479600         | 687658        | 59.17%          | 5.813%        |
| 14        | 16.351      | 2251          | 2255        | 2260         | rBV6     | 10437          | 16699         | 1.44%           | 0.141%        |
| 15        | 16.927      | 2347          | 2353        | 2358         | rBV      | 321732         | 468827        | 40.34%          | 3.963%        |
| 16        | 17.845      | 2501          | 2509        | 2531         | rBV      | 515283         | 898511        | 77.31%          | 7.595%        |
| 17        | 18.033      | 2538          | 2541        | 2546         | rVB5     | 16182          | 23129         | 1.99%           | 0.196%        |
| 18        | 18.127      | 2554          | 2557        | 2561         | rVB4     | 14483          | 18638         | 1.60%           | 0.158%        |
| 19        | 18.210      | 2567          | 2571        | 2576         | rVB5     | 29964          | 42824         | 3.68%           | 0.362%        |
| 20        | 18.398      | 2599          | 2603        | 2606         | rBV5     | 9486           | 11741         | 1.01%           | 0.099%        |
| 21        | 18.986      | 2699          | 2703        | 2705         | rBV3     | 20284          | 27512         | 2.37%           | 0.233%        |
| 22        | 19.010      | 2705          | 2707        | 2715         | rVB7     | 21266          | 38576         | 3.32%           | 0.326%        |
| 23        | 19.139      | 2722          | 2729        | 2745         | rVB      | 578262         | 875653        | 75.34%          | 7.402%        |
| 24        | 19.315      | 2750          | 2759        | 2761         | rBV2     | 98415          | 233527        | 20.09%          | 1.974%        |
| 25        | 19.574      | 2797          | 2803        | 2809         | rBV      | 980871         | 1162193       | 100.00%         | 9.824%        |
| 26        | 20.221      | 2910          | 2913        | 2916         | rBV5     | 14548          | 20600         | 1.77%           | 0.174%        |
| 27        | 20.333      | 2930          | 2932        | 2937         | rBV6     | 13836          | 20477         | 1.76%           | 0.173%        |
| 28        | 20.392      | 2939          | 2942        | 2946         | rVB2     | 28860          | 39970         | 3.44%           | 0.338%        |
| 29        | 20.486      | 2951          | 2958        | 2969         | rVB      | 174444         | 395832        | 34.06%          | 3.346%        |
| 30        | 20.862      | 3019          | 3022        | 3030         | rBV      | 80729          | 118621        | 10.21%          | 1.003%        |
| 31        | 21.127      | 3063          | 3067        | 3072         | rBV      | 408738         | 509882        | 43.87%          | 4.310%        |
| 32        | 21.345      | 3098          | 3104        | 3113         | rVB2     | 185983         | 383894        | 33.03%          | 3.245%        |
| 33        | 21.439      | 3115          | 3120        | 3130         | rVV3     | 98243          | 226840        | 19.52%          | 1.917%        |
| 34        | 21.545      | 3134          | 3138        | 3144         | rVB5     | 74542          | 138406        | 11.91%          | 1.170%        |
| 35        | 21.721      | 3165          | 3168        | 3170         | rBV      | 46062          | 52576         | 4.52%           | 0.444%        |
| 36        | 22.127      | 3232          | 3237        | 3241         | rBV      | 101152         | 193490        | 16.65%          | 1.635%        |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM082021\  
Data File : BM031836.D  
Acq On : 20 Aug 2021 11:32  
Operator : CG/JU  
Sample : M3434-23  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SWCS-13-1015

Integration Parameters: rteint.p  
Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM081621.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

|    |        |      |      |      |     |        |        |        |        |
|----|--------|------|------|------|-----|--------|--------|--------|--------|
| 37 | 22.645 | 3322 | 3325 | 3330 | rVB | 74886  | 95154  | 8.19%  | 0.804% |
| 38 | 23.274 | 3427 | 3432 | 3440 | rVB | 295084 | 541704 | 46.61% | 4.579% |




Sum of corrected areas: 11830643

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM082021\  
Data File : BM031836.D  
Acq On : 20 Aug 2021 11:32  
Operator : CG/JU  
Sample : M3434-23  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SWCS-13-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM081621.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

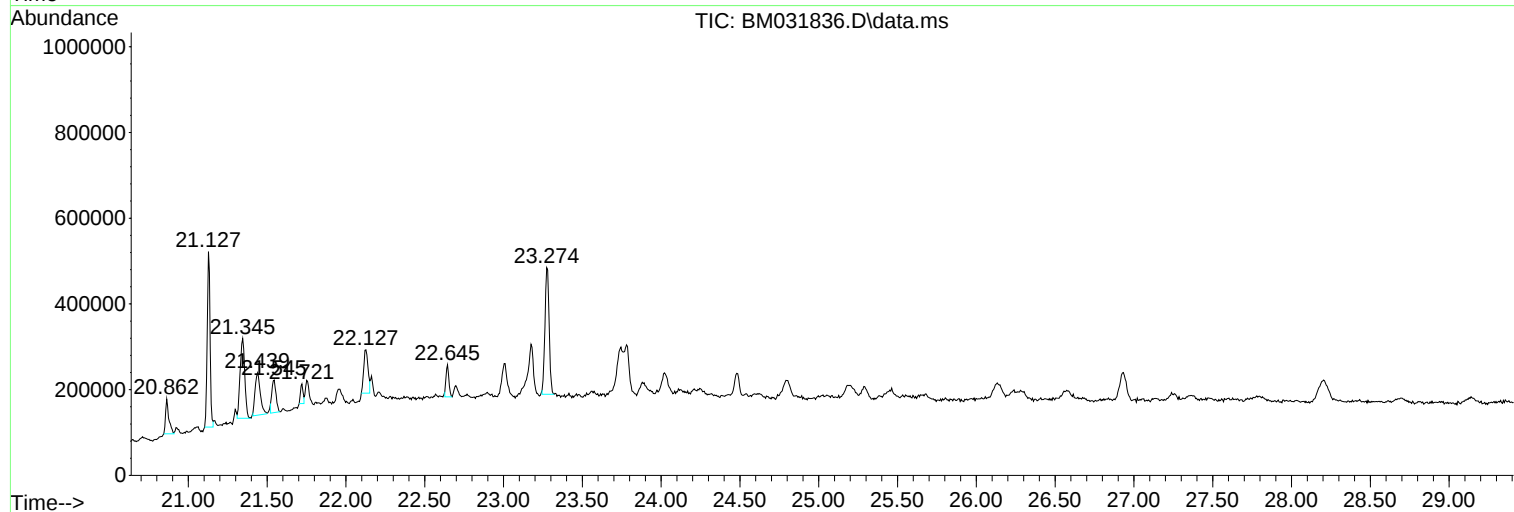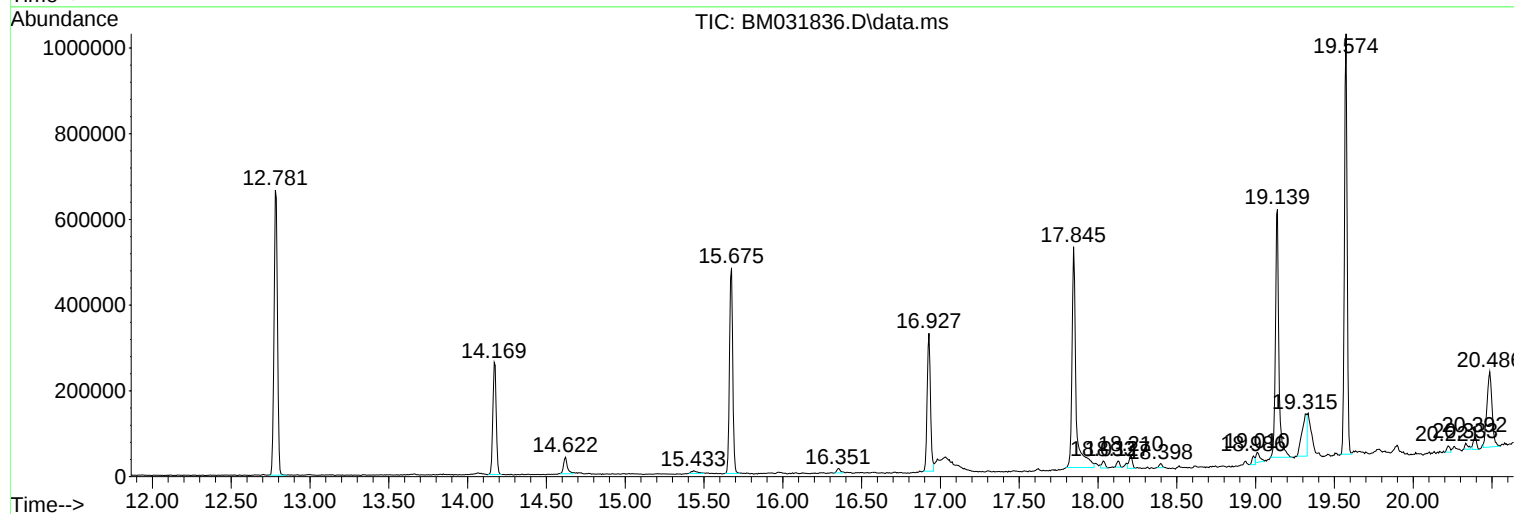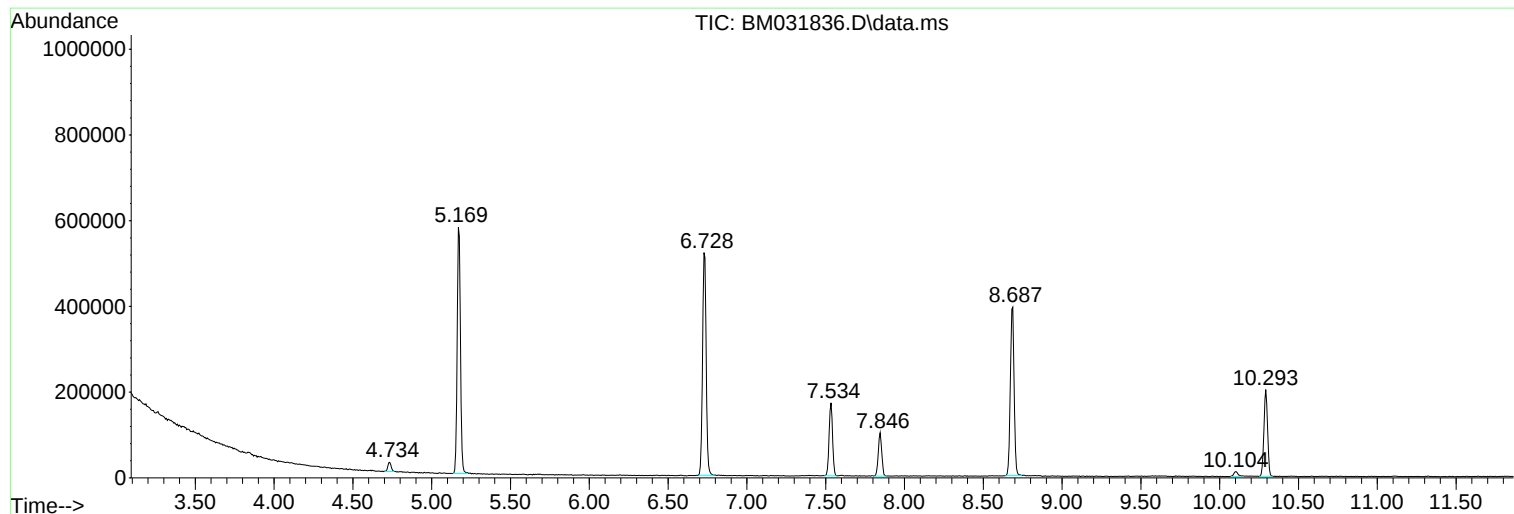

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM082021\  
Data File : BM031836.D  
Acq On : 20 Aug 2021 11:32  
Operator : CG/JU  
Sample : M3434-23  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SWCS-13-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM081621.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM082021\  
Data File : BM031836.D  
Acq On : 20 Aug 2021 11:32  
Operator : CG/JU  
Sample : M3434-23  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SWCS-13-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM081621.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|