

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031837.D
 Acq On : 20 Aug 2021 12:09
 Operator : CG/JU
 Sample : M3426-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-10-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031837.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.734	276	280	287	rVB	20532	30731	1.69%	0.232%
2	5.175	348	355	369	rVB	772231	1146782	63.10%	8.667%
3	6.734	612	620	630	rBV	725828	1165456	64.13%	8.808%
4	7.534	749	756	763	rBV	185122	288328	15.86%	2.179%
5	8.681	944	951	963	rBV	444297	745628	41.03%	5.635%
6	10.104	1187	1193	1208	rBV	13806	32495	1.79%	0.246%
7	10.292	1217	1225	1234	rBV	227990	372288	20.48%	2.813%
8	12.781	1642	1648	1657	rVB	898432	1330007	73.18%	10.051%
9	14.169	1878	1884	1891	rVB	301020	450555	24.79%	3.405%
10	14.622	1955	1961	1970	rBV3	14261	26536	1.46%	0.201%
11	15.674	2133	2140	2151	rBV	809831	1146448	63.08%	8.664%
12	16.927	2347	2353	2358	rBV	367203	530403	29.18%	4.008%
13	16.986	2358	2363	2366	rVB3	18706	28089	1.55%	0.212%
14	17.845	2503	2509	2519	rBV	254697	396659	21.83%	2.998%
15	18.715	2653	2657	2659	rBV3	15106	19989	1.10%	0.151%
16	18.992	2700	2704	2710	rBV	21231	46774	2.57%	0.353%
17	19.133	2724	2728	2736	rBV	190714	278484	15.32%	2.105%
18	19.574	2797	2803	2810	rVB	1522182	1817428	100.00%	13.735%
19	20.862	3018	3022	3031	rBV	240232	355940	19.58%	2.690%
20	21.127	3063	3067	3072	rBV	458568	577389	31.77%	4.363%
21	21.721	3164	3168	3169	rBV	139265	148912	8.19%	1.125%
22	21.751	3169	3173	3179	rVB2	377248	592108	32.58%	4.475%
23	22.209	3248	3251	3258	rVB2	82992	119985	6.60%	0.907%
24	22.645	3322	3325	3330	rVB2	106944	126753	6.97%	0.958%
25	22.698	3330	3334	3343	rVB	207768	362789	19.96%	2.742%
26	23.280	3427	3433	3439	rVB2	331991	595161	32.75%	4.498%
27	26.933	4049	4054	4073	rVB3	172227	500143	27.52%	3.780%




Sum of corrected areas: 13232260

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031837.D
Acq On : 20 Aug 2021 12:09
Operator : CG/JU
Sample : M3426-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-10-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

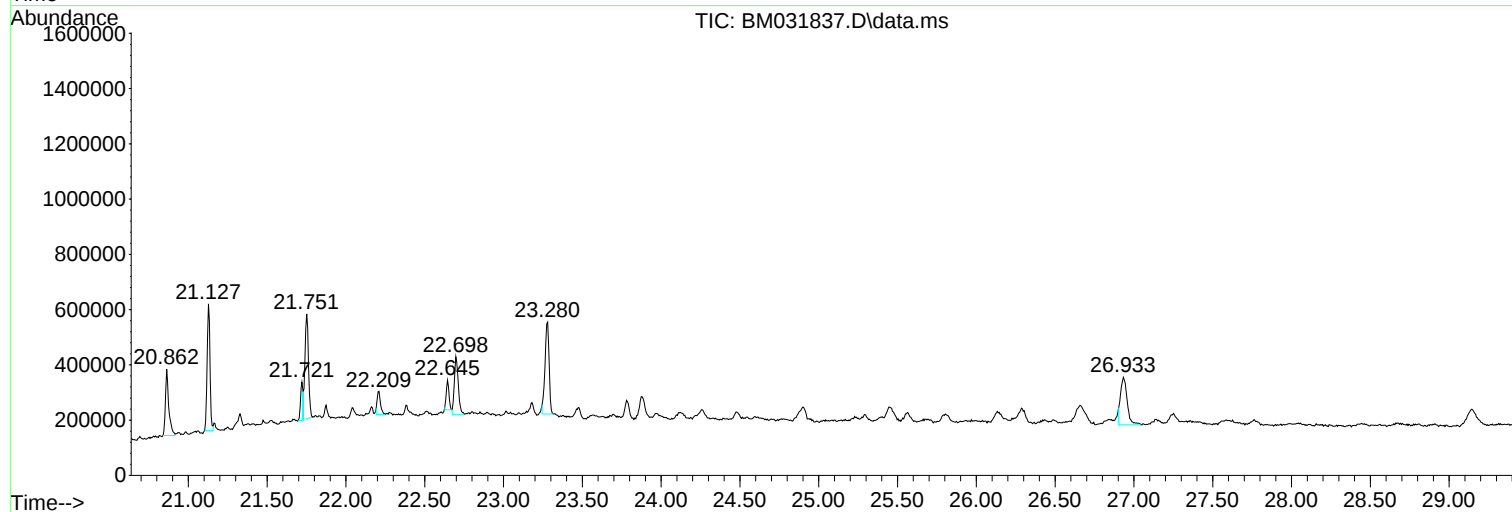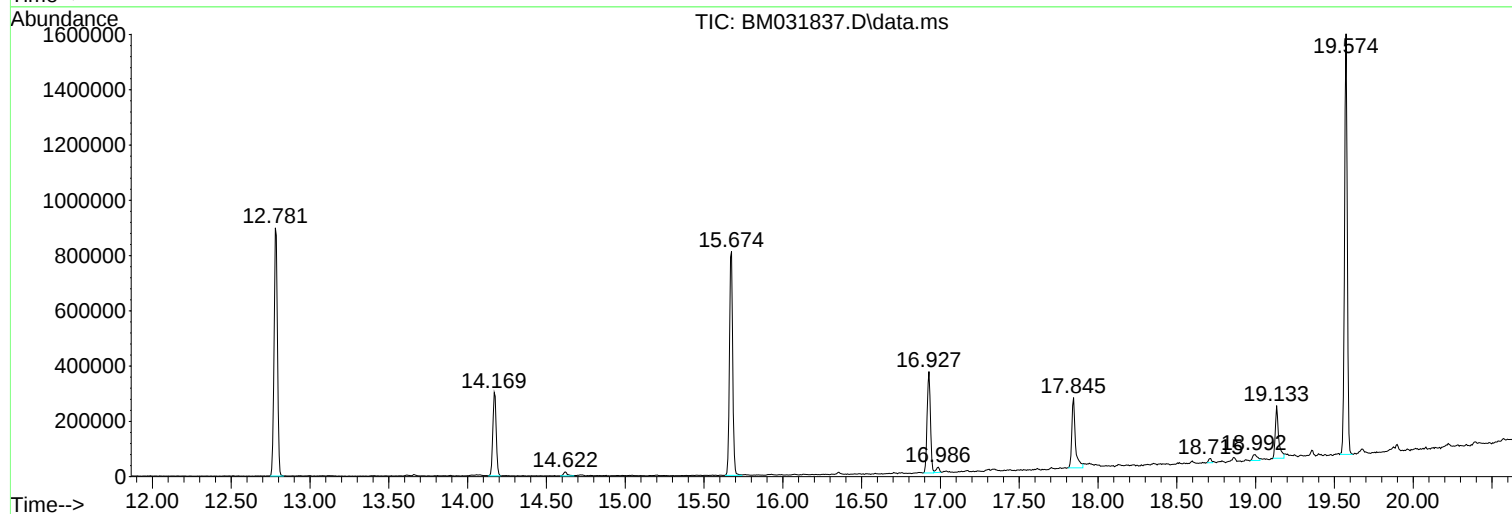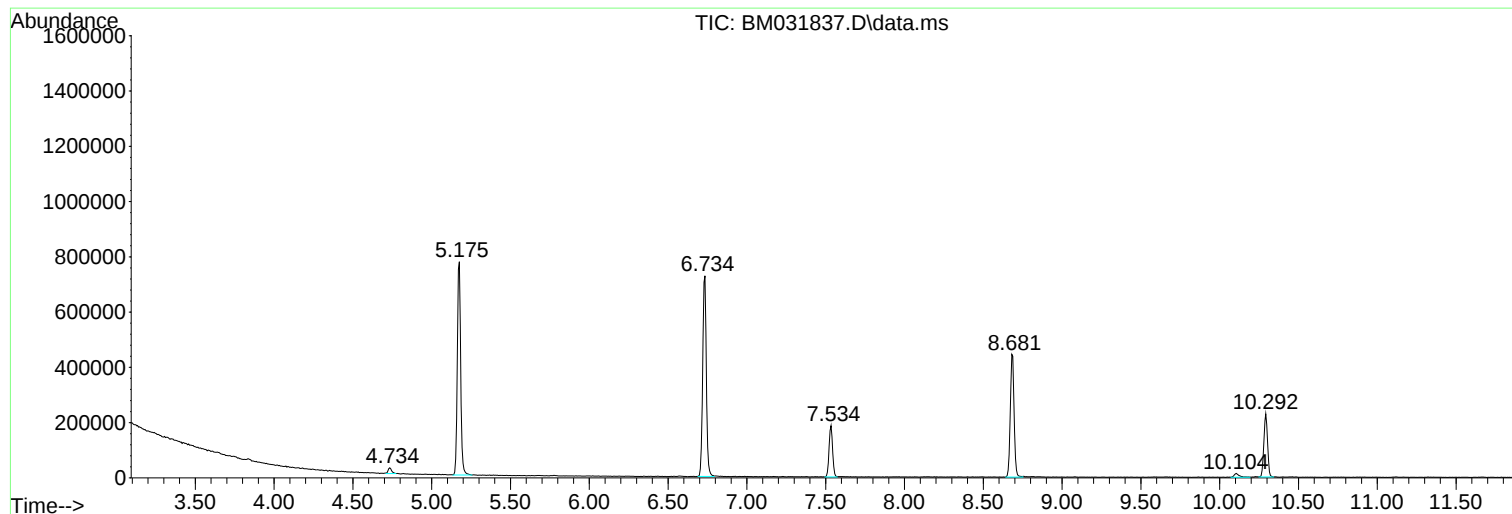

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031837.D
Acq On : 20 Aug 2021 12:09
Operator : CG/JU
Sample : M3426-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-10-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031837.D
Acq On : 20 Aug 2021 12:09
Operator : CG/JU
Sample : M3426-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-10-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------