

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031839.D
 Acq On : 20 Aug 2021 13:23
 Operator : CG/JU
 Sample : M3434-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-11-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031839.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.734	276	280	293	rVB2	26799	43415	2.39%	0.280%
2	5.175	348	355	362	rBV	772361	1114716	61.42%	7.188%
3	6.734	611	620	631	rBV	714892	1142204	62.94%	7.365%
4	7.534	749	756	763	rVB	197353	307152	16.92%	1.981%
5	8.687	944	952	964	rBV	436733	732507	40.36%	4.724%
6	10.104	1185	1193	1202	rBV2	14850	33180	1.83%	0.214%
7	10.292	1216	1225	1232	rBV	236799	399301	22.00%	2.575%
8	12.780	1642	1648	1658	rVB	895643	1353528	74.58%	8.728%
9	13.892	1831	1837	1841	rBV	19864	30502	1.68%	0.197%
10	14.169	1878	1884	1892	rVB	315616	461640	25.44%	2.977%
11	15.674	2132	2140	2150	rBV	783045	1067606	58.83%	6.884%
12	15.910	2175	2180	2188	rVB8	13494	32181	1.77%	0.208%
13	16.751	2319	2323	2332	rVB6	10732	20277	1.12%	0.131%
14	16.927	2347	2353	2357	rBV	370368	529732	29.19%	3.416%
15	16.968	2357	2360	2367	rVB	59553	87726	4.83%	0.566%
16	17.063	2373	2376	2382	rVB	17829	23755	1.31%	0.153%
17	17.804	2495	2502	2504	rBV5	16479	30553	1.68%	0.197%
18	17.845	2504	2509	2519	rVV3	156584	257768	14.20%	1.662%
19	17.992	2529	2534	2538	rBV2	23811	39577	2.18%	0.255%
20	18.357	2592	2596	2602	rVB8	12740	19302	1.06%	0.124%
21	18.727	2655	2659	2663	rVB2	24640	36140	1.99%	0.233%
22	18.786	2663	2669	2673	rBV7	14485	32632	1.80%	0.210%
23	18.992	2699	2704	2711	rBV	156979	227655	12.54%	1.468%
24	19.062	2711	2716	2719	rVV7	11977	20300	1.12%	0.131%
25	19.133	2724	2728	2734	rBV3	83402	141120	7.78%	0.910%
26	19.357	2758	2766	2770	rBV	142208	215048	11.85%	1.387%
27	19.574	2798	2803	2814	rVB	1523837	1814841	100.00%	11.703%
28	19.680	2819	2821	2828	rVB5	15040	28831	1.59%	0.186%
29	19.821	2841	2845	2846	rBV4	19478	24490	1.35%	0.158%
30	19.862	2849	2852	2856	rVV2	27712	48329	2.66%	0.312%
31	19.956	2866	2868	2872	rVB	18336	22004	1.21%	0.142%
32	20.015	2876	2878	2882	rVB	27624	30087	1.66%	0.194%
33	20.862	3018	3022	3028	rBV	308775	410922	22.64%	2.650%
34	21.127	3061	3067	3071	rBV2	505789	757726	41.75%	4.886%
35	21.162	3071	3073	3077	rVB	93433	115948	6.39%	0.748%
36	21.745	3168	3172	3181	rVB2	571928	871773	48.04%	5.622%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031839.D
Acq On : 20 Aug 2021 13:23
Operator : CG/JU
Sample : M3434-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-11-0205

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.874	3190	3194	3199	rVB	161629	233384	12.86%	1.505%
38	22.380	3277	3280	3290	rVB6	69083	103246	5.69%	0.666%
39	22.645	3320	3325	3329	rBV	380141	561214	30.92%	3.619%
40	22.697	3330	3334	3342	rVB3	179853	334449	18.43%	2.157%
41	23.180	3413	3416	3424	rVB2	95418	149379	8.23%	0.963%
42	23.274	3427	3432	3438	rVB2	325252	566110	31.19%	3.651%
43	23.474	3462	3466	3472	rVB	184673	293489	16.17%	1.893%
44	23.786	3514	3519	3524	rVB	184309	322683	17.78%	2.081%
45	23.880	3530	3535	3545	rVB	191131	419141	23.10%	2.703%




Sum of corrected areas: 15507563

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031839.D
Acq On : 20 Aug 2021 13:23
Operator : CG/JU
Sample : M3434-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-11-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

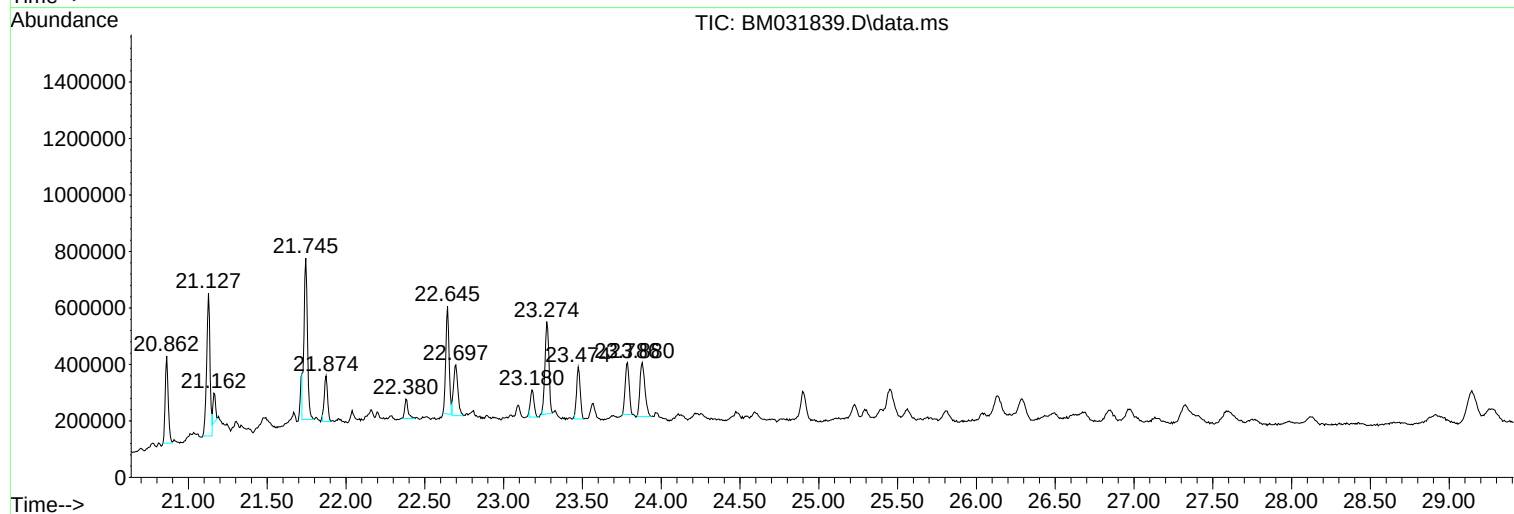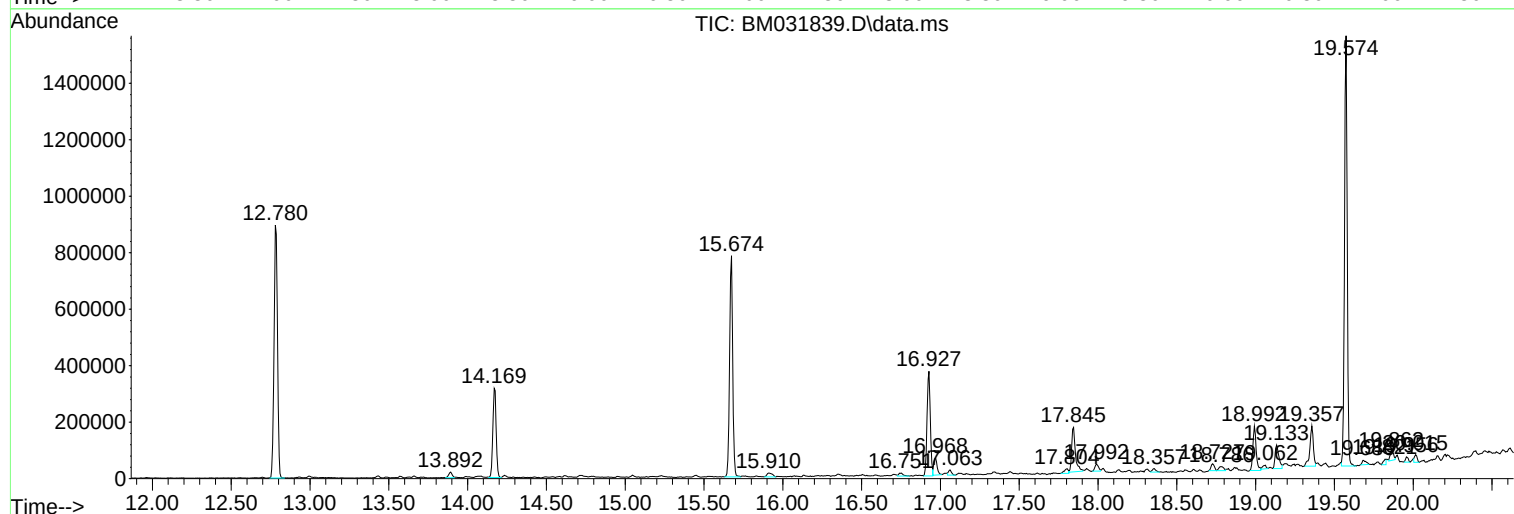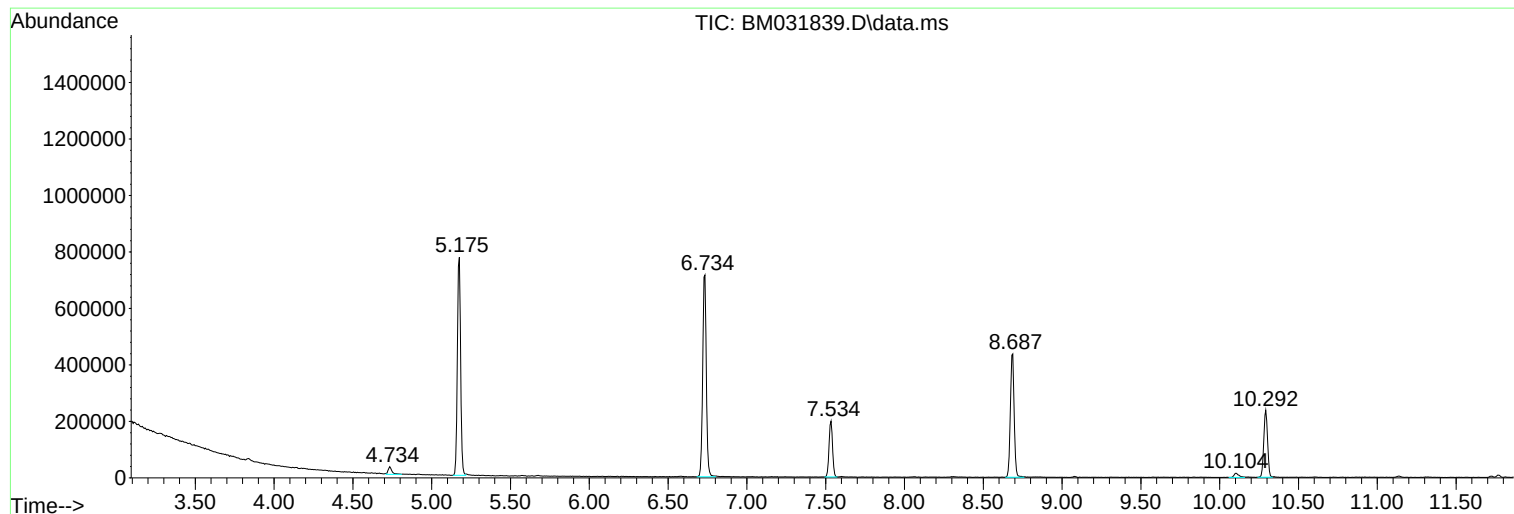

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031839.D
Acq On : 20 Aug 2021 13:23
Operator : CG/JU
Sample : M3434-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-11-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031839.D
Acq On : 20 Aug 2021 13:23
Operator : CG/JU
Sample : M3434-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-11-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------