

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031840.D
 Acq On : 20 Aug 2021 14:00
 Operator : CG/JU
 Sample : M3434-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-12-0002

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031840.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.734	276	280	288	rVB	19150	27756	1.43%	0.241%
2	5.175	348	355	372	rBV	754022	1151422	59.37%	10.002%
3	6.734	612	620	632	rBV	723402	1189557	61.34%	10.333%
4	7.534	749	756	764	rBV	208316	328579	16.94%	2.854%
5	8.681	944	951	961	rBV	444319	759773	39.18%	6.600%
6	10.099	1188	1192	1199	rBV3	14362	28960	1.49%	0.252%
7	10.293	1217	1225	1235	rBV	257444	432620	22.31%	3.758%
8	12.781	1642	1648	1660	rVB	993154	1496153	77.15%	12.997%
9	14.169	1878	1884	1891	rVB	355931	514224	26.52%	4.467%
10	15.675	2132	2140	2149	rBV	758833	1110506	57.26%	9.647%
11	15.910	2176	2180	2182	rBV4	15388	20973	1.08%	0.182%
12	16.704	2311	2315	2318	rBV6	12422	20326	1.05%	0.177%
13	16.751	2320	2323	2332	rVB6	16883	31185	1.61%	0.271%
14	16.928	2347	2353	2358	rBV	407984	575347	29.67%	4.998%
15	17.122	2382	2386	2391	rBV7	12100	21142	1.09%	0.184%
16	17.839	2503	2508	2520	rBV	171856	261245	13.47%	2.269%
17	18.133	2554	2558	2562	rBV2	17762	25160	1.30%	0.219%
18	18.774	2664	2667	2672	rVB3	24522	32533	1.68%	0.283%
19	18.992	2701	2704	2711	rBV	31829	60062	3.10%	0.522%
20	19.133	2724	2728	2734	rBV3	101437	163838	8.45%	1.423%
21	19.357	2763	2766	2770	rBV2	34158	40263	2.08%	0.350%
22	19.574	2798	2803	2812	rVB	1637352	1939343	100.00%	16.847%
23	20.863	3019	3022	3030	rVB	130589	164539	8.48%	1.429%
24	21.127	3063	3067	3072	rBV	466398	594528	30.66%	5.165%
25	23.280	3430	3433	3439	rVB2	324562	521675	26.90%	4.532%




Sum of corrected areas: 11511709

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031840.D
Acq On : 20 Aug 2021 14:00
Operator : CG/JU
Sample : M3434-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-12-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

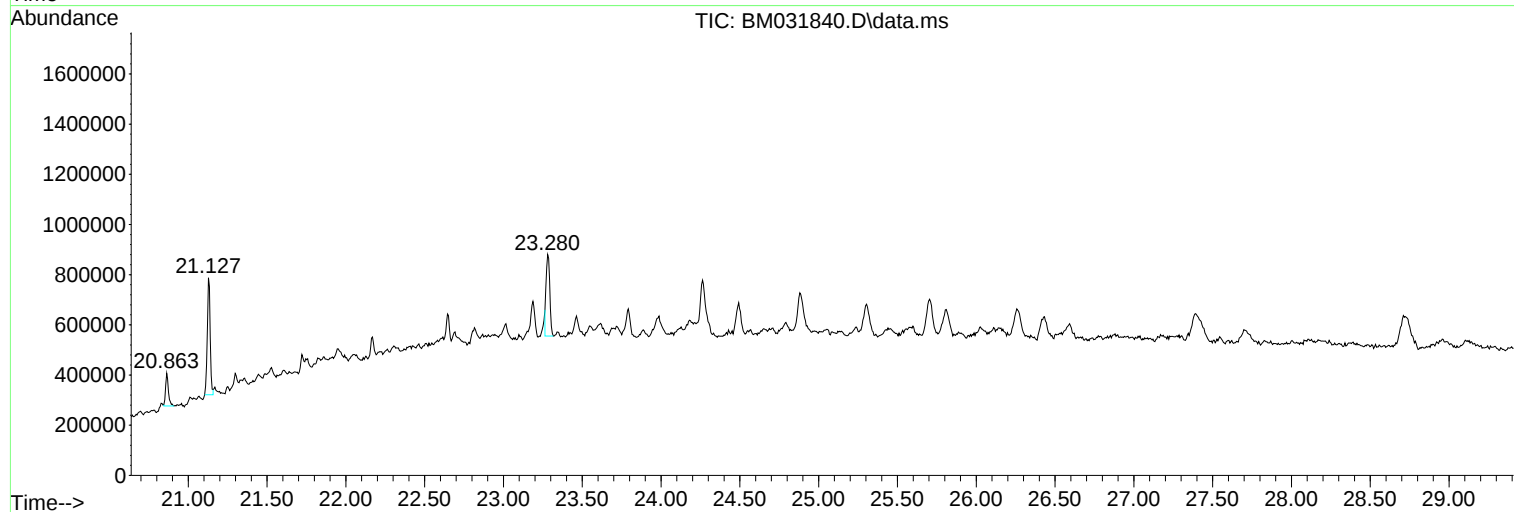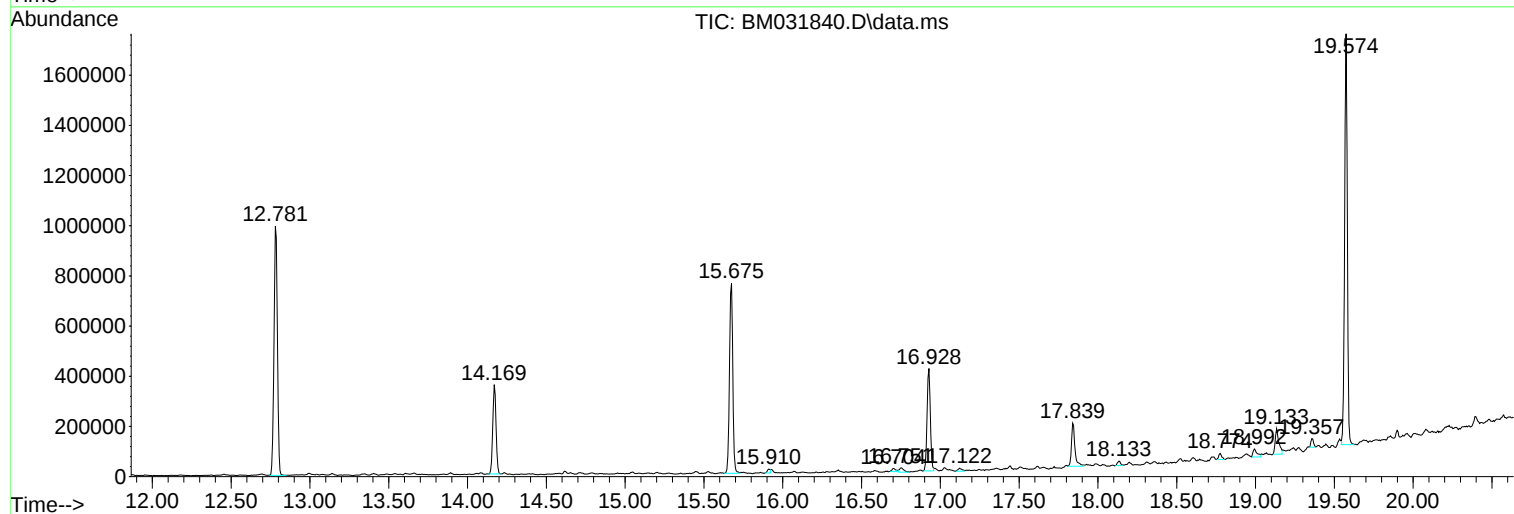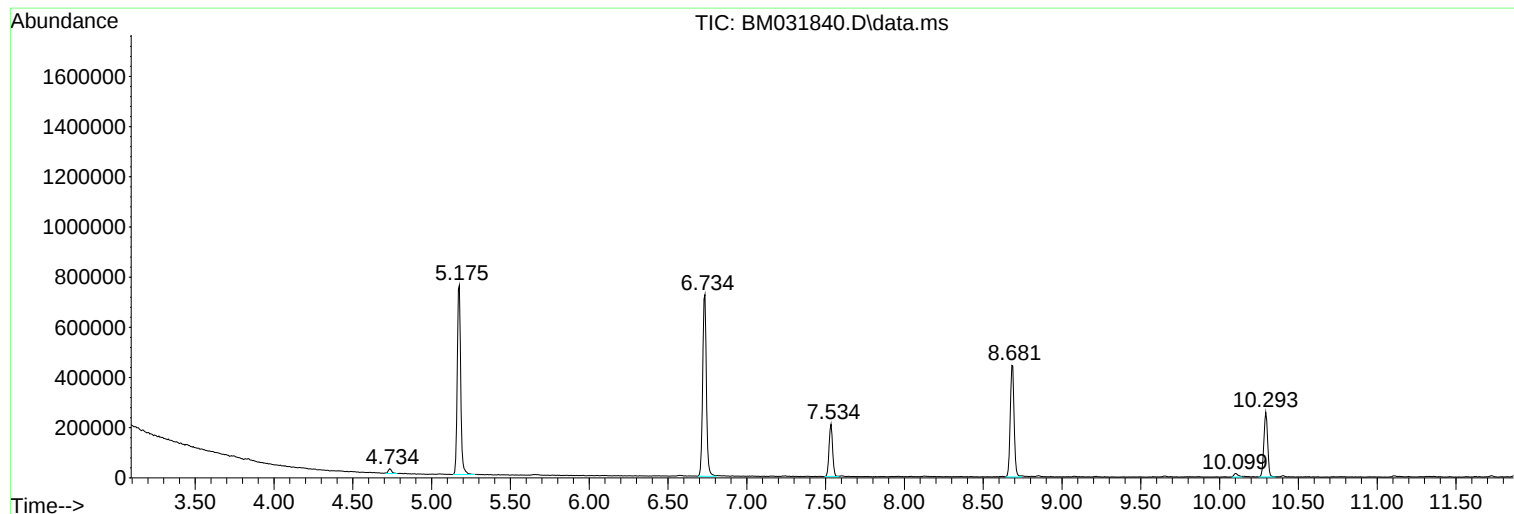

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031840.D
Acq On : 20 Aug 2021 14:00
Operator : CG/JU
Sample : M3434-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-12-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031840.D
Acq On : 20 Aug 2021 14:00
Operator : CG/JU
Sample : M3434-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-12-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------