

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031841.D
 Acq On : 20 Aug 2021 14:37
 Operator : CG/JU
 Sample : M3394-16
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-02-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031841.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.175	349	355	362	rBV	966209	1332267	11.97%	1.169%
2	6.734	611	620	636	rBV	880922	1404605	12.62%	1.232%
3	7.534	747	756	766	rBV	247510	385001	3.46%	0.338%
4	8.686	945	952	959	rBV	548218	885620	7.96%	0.777%
5	10.292	1216	1225	1230	rBV	292510	507889	4.56%	0.446%
6	10.345	1230	1234	1241	rVB	100822	169917	1.53%	0.149%
7	11.816	1477	1484	1500	rVB4	43918	133370	1.20%	0.117%
8	11.963	1503	1509	1517	rVB	111749	181847	1.63%	0.160%
9	12.186	1542	1547	1557	rVB	117285	192282	1.73%	0.169%
10	12.786	1642	1649	1656	rVB	1009921	1441947	12.96%	1.265%
11	13.345	1735	1744	1750	rBV2	79367	201476	1.81%	0.177%
12	13.492	1763	1769	1774	rBV	197332	337701	3.03%	0.296%
13	13.627	1787	1792	1797	rBV	174056	280543	2.52%	0.246%
14	13.727	1803	1809	1813	rBV	98970	150601	1.35%	0.132%
15	13.898	1830	1838	1851	rBV	916829	1515571	13.62%	1.330%
16	14.174	1875	1885	1891	rBV2	380402	616106	5.54%	0.540%
17	14.239	1891	1896	1900	rBV	101737	165711	1.49%	0.145%
18	14.392	1916	1922	1930	rBV3	62510	157692	1.42%	0.138%
19	14.580	1946	1954	1962	rVV	186873	385556	3.46%	0.338%
20	14.657	1962	1967	1972	rVB	144335	211220	1.90%	0.185%
21	14.798	1983	1991	1996	rBV3	161406	355569	3.20%	0.312%
22	15.051	2030	2034	2042	rVB2	179369	264356	2.38%	0.232%
23	15.174	2051	2055	2059	rVV2	114254	181379	1.63%	0.159%
24	15.233	2059	2065	2077	rVB3	334683	692886	6.23%	0.608%
25	15.445	2096	2101	2110	rVB5	92808	211771	1.90%	0.186%
26	15.527	2110	2115	2121	rBV2	123711	244176	2.19%	0.214%
27	15.680	2132	2141	2149	rVB2	880235	1350033	12.13%	1.184%
28	15.915	2175	2181	2190	rBV3	234044	407802	3.66%	0.358%
29	16.239	2229	2236	2241	rBV3	175856	396963	3.57%	0.348%
30	16.292	2241	2245	2250	rVB	145958	205373	1.85%	0.180%
31	16.386	2257	2261	2267	rVB2	108447	169079	1.52%	0.148%
32	16.509	2279	2282	2287	rVB2	106921	142064	1.28%	0.125%
33	16.592	2292	2296	2304	rVB3	206467	314828	2.83%	0.276%
34	16.662	2304	2308	2313	rBV2	76897	136003	1.22%	0.119%
35	16.751	2318	2323	2332	rVB	314804	500532	4.50%	0.439%
36	16.933	2349	2354	2357	rBV	363640	556480	5.00%	0.488%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031841.D
 Acq On : 20 Aug 2021 14:37
 Operator : CG/JU
 Sample : M3394-16
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-02-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	16.980	2357	2362	2370	rVV	4514630	6316478	56.76%	5.541%
38	17.068	2372	2377	2382	rVB	1066910	1402330	12.60%	1.230%
39	17.127	2382	2387	2392	rBV3	185449	338360	3.04%	0.297%
40	17.345	2420	2424	2432	rBV	219227	349900	3.14%	0.307%
41	17.456	2438	2443	2446	rVV2	152509	216652	1.95%	0.190%
42	17.509	2448	2452	2460	rVB2	285727	475665	4.27%	0.417%
43	17.656	2473	2477	2484	rVB	172425	314103	2.82%	0.276%
44	17.809	2498	2503	2507	rVV	1062380	1503746	13.51%	1.319%
45	17.856	2507	2511	2517	rVB	1396669	2000963	17.98%	1.755%
46	17.939	2520	2525	2530	rBV	342438	479717	4.31%	0.421%
47	18.003	2530	2536	2540	rVV2	1368243	2461539	22.12%	2.159%
48	18.039	2540	2542	2550	rVB	825500	1026904	9.23%	0.901%
49	18.133	2554	2558	2562	rBV5	84158	151724	1.36%	0.133%
50	18.209	2567	2571	2575	rVB2	174451	244239	2.19%	0.214%
51	18.315	2585	2589	2593	rBV	479899	647060	5.81%	0.568%
52	18.368	2593	2598	2606	rVB	765712	1053454	9.47%	0.924%
53	18.533	2622	2626	2628	rBV2	127739	185618	1.67%	0.163%
54	18.562	2628	2631	2636	rVV	232160	368273	3.31%	0.323%
55	18.615	2636	2640	2643	rVV	336773	444384	3.99%	0.390%
56	18.656	2643	2647	2651	rVB2	249989	351508	3.16%	0.308%
57	18.739	2655	2661	2665	rBV	849902	1375582	12.36%	1.207%
58	18.797	2665	2671	2675	rVV5	410083	997987	8.97%	0.875%
59	18.833	2675	2677	2681	rVB	287978	291862	2.62%	0.256%
60	18.886	2681	2686	2693	rBV3	490802	1008346	9.06%	0.885%
61	19.015	2700	2708	2713	rBV	7218506	10146052	91.18%	8.900%
62	19.074	2714	2718	2721	rBV	190584	275765	2.48%	0.242%
63	19.103	2721	2723	2727	rVV2	145264	171735	1.54%	0.151%
64	19.156	2727	2732	2736	rVB	537772	796115	7.15%	0.698%
65	19.221	2739	2743	2745	rBV2	187419	263124	2.36%	0.231%
66	19.250	2745	2748	2751	rVB2	156359	186256	1.67%	0.163%
67	19.380	2759	2770	2777	rBV	7222343	11127439	100.00%	9.761%
68	19.444	2777	2781	2787	rVB2	399648	657477	5.91%	0.577%
69	19.550	2795	2799	2800	rBV2	214590	287202	2.58%	0.252%
70	19.580	2800	2804	2807	rVB	1010722	1145219	10.29%	1.005%
71	19.697	2819	2824	2831	rBV2	563612	1292634	11.62%	1.134%
72	19.786	2836	2839	2842	rVV3	157460	198336	1.78%	0.174%
73	19.833	2842	2847	2850	rVV4	515997	985543	8.86%	0.865%
74	19.874	2850	2854	2858	rVB	1181415	1606540	14.44%	1.409%
75	19.974	2867	2871	2874	rBV	878187	1060512	9.53%	0.930%
76	20.033	2876	2881	2885	rVB2	902988	1234885	11.10%	1.083%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031841.D
 Acq On : 20 Aug 2021 14:37
 Operator : CG/JU
 Sample : M3394-16
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-02-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	20.127	2892	2897	2900	rBV2	240570	420607	3.78%	0.369%
78	20.168	2900	2904	2907	rVV2	709740	895268	8.05%	0.785%
79	20.215	2908	2912	2916	rVB	653759	877689	7.89%	0.770%
80	20.621	2978	2981	2987	rVB	572759	867819	7.80%	0.761%
81	20.786	3002	3009	3013	rBV3	828258	1478452	13.29%	1.297%
82	20.821	3013	3015	3019	rVV	655663	777957	6.99%	0.682%
83	20.862	3019	3022	3027	rVV2	596932	1005063	9.03%	0.882%
84	20.921	3029	3032	3037	rVB	536422	734092	6.60%	0.644%
85	21.133	3062	3068	3072	rBV2	3933930	6032189	54.21%	5.292%
86	21.186	3073	3077	3085	rVB	3949768	5062591	45.50%	4.441%
87	21.256	3087	3089	3092	rBV2	176339	171122	1.54%	0.150%
88	21.297	3093	3096	3101	rBV2	239619	403909	3.63%	0.354%
89	21.350	3101	3105	3112	rVV2	589328	836876	7.52%	0.734%
90	21.497	3127	3130	3133	rVB2	230402	268170	2.41%	0.235%
91	21.627	3149	3152	3155	rBV	293595	373484	3.36%	0.328%
92	21.680	3155	3161	3165	rVV	858142	1470021	13.21%	1.290%
93	21.727	3166	3169	3176	rVB2	500639	921449	8.28%	0.808%
94	21.868	3190	3193	3196	rBV2	451283	545952	4.91%	0.479%
95	22.674	3323	3330	3334	rBV	2566782	5828164	52.38%	5.113%
96	22.827	3351	3356	3361	rBV	601438	995146	8.94%	0.873%
97	23.127	3401	3407	3414	rVB	1686780	3037499	27.30%	2.665%
98	23.221	3416	3423	3428	rVB	2506287	4477524	40.24%	3.928%
99	23.350	3441	3445	3453	rVB2	628401	1219794	10.96%	1.070%
100	25.450	3794	3802	3810	rVB	1158213	3066577	27.56%	2.690%




Sum of corrected areas: 113994858

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031841.D
Acq On : 20 Aug 2021 14:37
Operator : CG/JU
Sample : M3394-16
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-02-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

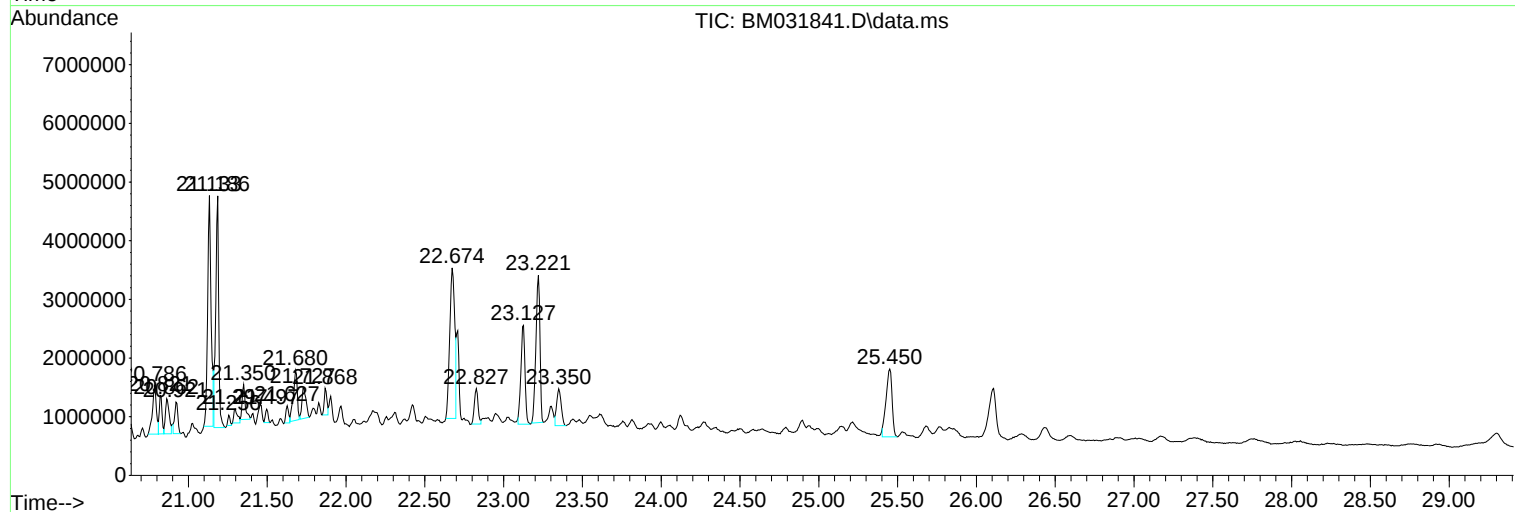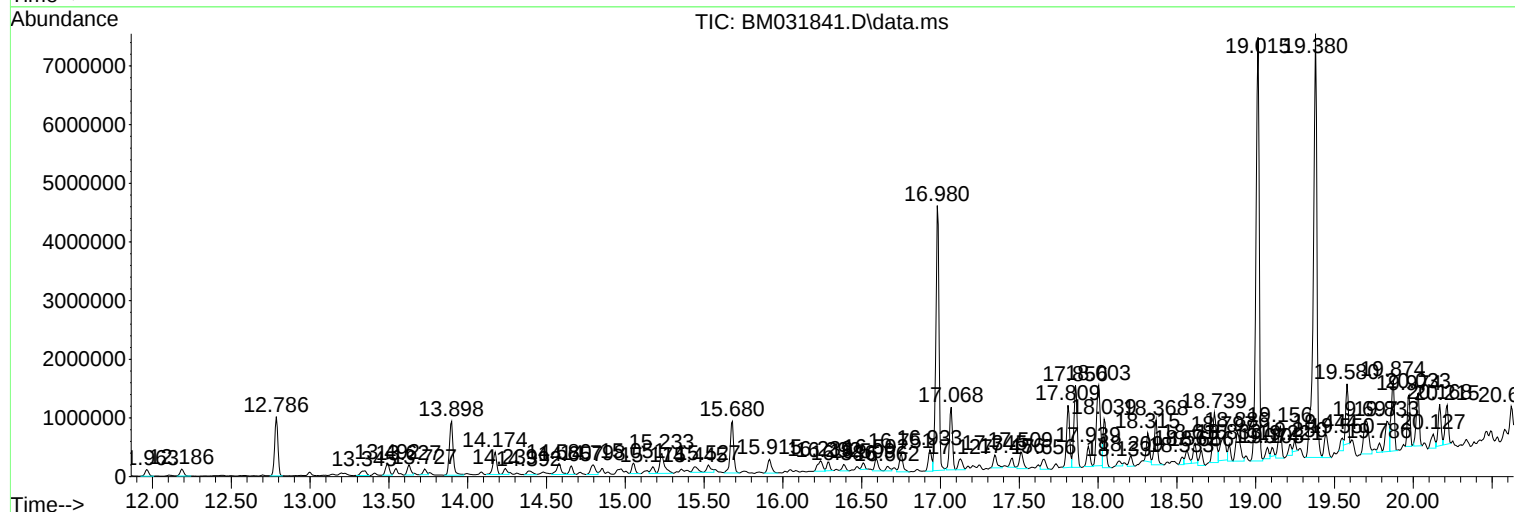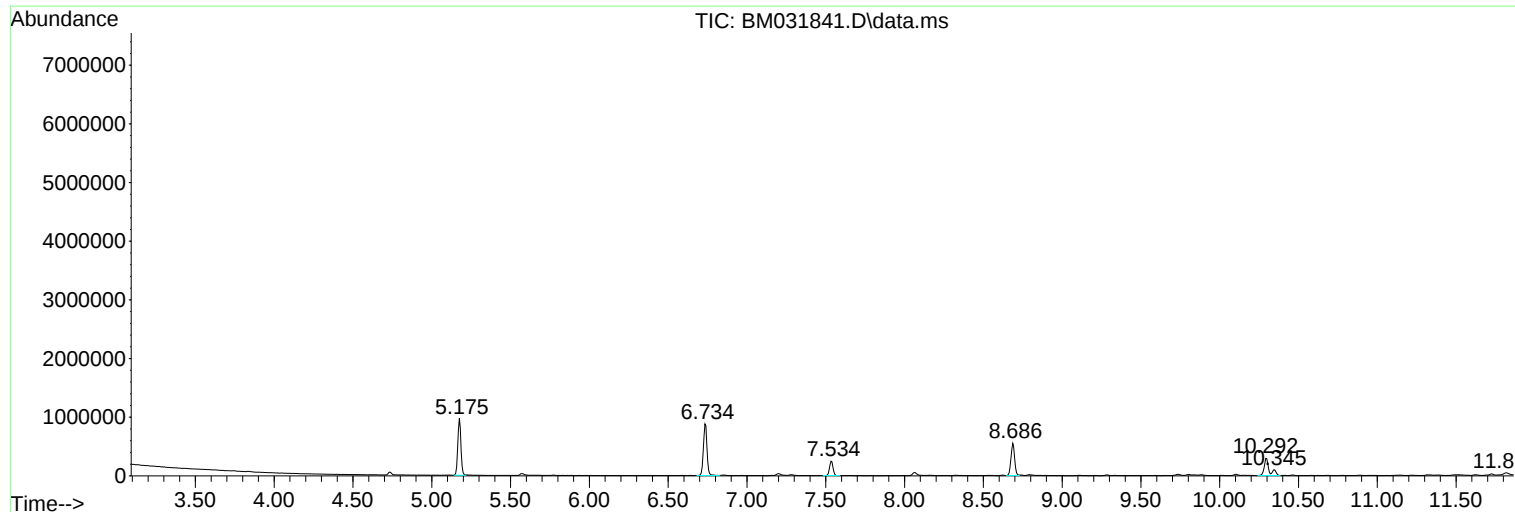

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031841.D
Acq On : 20 Aug 2021 14:37
Operator : CG/JU
Sample : M3394-16
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-02-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031841.D
Acq On : 20 Aug 2021 14:37
Operator : CG/JU
Sample : M3394-16
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-02-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------