

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031842.D
 Acq On : 20 Aug 2021 15:14
 Operator : CG/JU
 Sample : M3394-19
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-02-0510

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031842.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.734	276	280	287	rVB	64030	90502	4.63%	0.321%
2	5.175	349	355	362	rBV	958744	1355604	69.38%	4.805%
3	5.575	417	423	429	rBV5	17523	33845	1.73%	0.120%
4	6.740	613	621	631	rVB	871597	1373053	70.27%	4.867%
5	7.192	694	698	706	rVB3	15325	26432	1.35%	0.094%
6	7.534	746	756	764	rBV	223850	363755	18.62%	1.289%
7	8.063	840	846	852	rBV3	11926	21005	1.07%	0.074%
8	8.686	945	952	959	rBV	533513	877097	44.89%	3.109%
9	10.110	1187	1194	1201	rBV3	14668	33021	1.69%	0.117%
10	10.298	1219	1226	1232	rBV	262932	453797	23.22%	1.609%
11	11.963	1504	1509	1516	rVB	13677	23380	1.20%	0.083%
12	12.786	1642	1649	1655	rBV	972059	1401112	71.70%	4.967%
13	12.998	1681	1685	1695	rBV4	11800	20530	1.05%	0.073%
14	13.492	1763	1769	1774	rBV	29294	48830	2.50%	0.173%
15	13.545	1774	1778	1782	rBV2	14164	20396	1.04%	0.072%
16	13.627	1786	1792	1797	rBV	43027	64843	3.32%	0.230%
17	13.727	1803	1809	1813	rBV2	15839	24254	1.24%	0.086%
18	13.892	1829	1837	1849	rBV	189608	315937	16.17%	1.120%
19	14.174	1878	1885	1892	rBV	355845	518369	26.53%	1.838%
20	14.239	1892	1896	1899	rBV2	18688	29954	1.53%	0.106%
21	14.392	1916	1922	1925	rBV5	17047	30826	1.58%	0.109%
22	14.580	1947	1954	1959	rBV2	33447	63459	3.25%	0.225%
23	14.657	1963	1967	1972	rVB	44313	66431	3.40%	0.235%
24	14.721	1972	1978	1979	rBV6	13505	21127	1.08%	0.075%
25	14.792	1985	1990	1996	rVB5	43876	86210	4.41%	0.306%
26	14.851	1997	2000	2004	rVB	28774	36934	1.89%	0.131%
27	14.951	2012	2017	2018	rBV2	24635	28589	1.46%	0.101%
28	15.051	2030	2034	2042	rVB	41242	60685	3.11%	0.215%
29	15.139	2042	2049	2051	rBV5	17726	41660	2.13%	0.148%
30	15.174	2051	2055	2059	rVV4	31445	54452	2.79%	0.193%
31	15.227	2059	2064	2077	rVB3	55833	150691	7.71%	0.534%
32	15.357	2082	2086	2089	rBV6	15899	21959	1.12%	0.078%
33	15.445	2097	2101	2108	rVB8	30113	60779	3.11%	0.215%
34	15.527	2110	2115	2118	rBV	31565	53955	2.76%	0.191%
35	15.680	2131	2141	2149	rBV	788128	1161704	59.45%	4.118%
36	15.757	2149	2154	2160	rVB4	13768	28957	1.48%	0.103%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031842.D
 Acq On : 20 Aug 2021 15:14
 Operator : CG/JU
 Sample : M3394-19
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-02-0510

Integration Parameters: rteint.p

Integrator: RTE

Smoother: ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	15.915	2176	2181	2190	rBV7	54990	102578	5.25%	0.364%
38	16.015	2194	2198	2200	rBV3	15877	20125	1.03%	0.071%
39	16.239	2229	2236	2241	rBV2	60966	135689	6.94%	0.481%
40	16.286	2241	2244	2250	rVB	56643	78529	4.02%	0.278%
41	16.386	2258	2261	2267	rVB5	41707	67492	3.45%	0.239%
42	16.474	2267	2276	2278	rBV4	24971	53012	2.71%	0.188%
43	16.509	2278	2282	2286	rVB3	32195	46130	2.36%	0.164%
44	16.592	2292	2296	2301	rVB4	35558	55614	2.85%	0.197%
45	16.668	2304	2309	2313	rBV2	23138	46378	2.37%	0.164%
46	16.751	2319	2323	2332	rVB2	64752	111328	5.70%	0.395%
47	16.933	2348	2354	2357	rBV	380861	549101	28.10%	1.947%
48	16.974	2357	2361	2366	rVB	657094	875452	44.80%	3.103%
49	17.062	2372	2376	2382	rVB	224591	311755	15.95%	1.105%
50	17.127	2382	2387	2392	rBV2	60279	116139	5.94%	0.412%
51	17.174	2392	2395	2397	rBV	23044	21092	1.08%	0.075%
52	17.209	2397	2401	2405	rBV3	17147	29211	1.49%	0.104%
53	17.345	2420	2424	2428	rBV	33450	61953	3.17%	0.220%
54	17.456	2439	2443	2446	rBV2	33010	46216	2.37%	0.164%
55	17.509	2448	2452	2460	rVB	97792	159399	8.16%	0.565%
56	17.656	2473	2477	2483	rVB	51688	88448	4.53%	0.314%
57	17.733	2486	2490	2494	rBV3	24960	40862	2.09%	0.145%
58	17.809	2497	2503	2506	rVV	256964	401200	20.53%	1.422%
59	17.851	2506	2510	2518	rVB2	415979	657699	33.66%	2.331%
60	17.933	2520	2524	2529	rVV	121056	178065	9.11%	0.631%
61	17.998	2529	2535	2539	rVV2	387894	703878	36.02%	2.495%
62	18.039	2539	2542	2551	rVB	231673	324796	16.62%	1.151%
63	18.133	2554	2558	2562	rBV5	27303	52337	2.68%	0.186%
64	18.209	2567	2571	2575	rVB3	45256	63040	3.23%	0.223%
65	18.315	2585	2589	2593	rVV	119162	155004	7.93%	0.549%
66	18.362	2593	2597	2602	rVB2	90579	122081	6.25%	0.433%
67	18.533	2623	2626	2628	rBV2	32696	35474	1.82%	0.126%
68	18.562	2628	2631	2636	rVV2	59101	83597	4.28%	0.296%
69	18.615	2636	2640	2643	rVV	77308	98639	5.05%	0.350%
70	18.650	2643	2646	2651	rVB2	66278	89126	4.56%	0.316%
71	18.733	2655	2660	2665	rBV	242853	407165	20.84%	1.443%
72	18.798	2665	2671	2674	rVV3	128763	260416	13.33%	0.923%
73	18.827	2674	2676	2680	rVB	88290	100675	5.15%	0.357%
74	18.880	2680	2685	2692	rBV5	111335	257437	13.17%	0.913%
75	19.003	2700	2706	2711	rBV	1184086	1579296	80.82%	5.598%
76	19.068	2714	2717	2720	rVV	52763	64659	3.31%	0.229%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031842.D
 Acq On : 20 Aug 2021 15:14
 Operator : CG/JU
 Sample : M3394-19
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-02-0510

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	19.103	2720	2723	2726	rVV2	44950	59182	3.03%	0.210%
78	19.150	2726	2731	2736	rVV2	181990	315062	16.12%	1.117%
79	19.368	2759	2768	2777	rBV	1282908	1954003	100.00%	6.927%
80	19.445	2778	2781	2787	rVB3	81491	128505	6.58%	0.456%
81	19.580	2799	2804	2813	rVB	1197036	1519434	77.76%	5.386%
82	19.692	2819	2823	2830	rBV4	119199	260461	13.33%	0.923%
83	19.833	2843	2847	2849	rBV2	106406	169554	8.68%	0.601%
84	19.868	2850	2853	2857	rVB	249560	309608	15.84%	1.098%
85	19.968	2866	2870	2874	rBV	180591	216104	11.06%	0.766%
86	20.027	2876	2880	2883	rVB	159586	206544	10.57%	0.732%
87	20.162	2900	2903	2906	rVV	124091	131860	6.75%	0.467%
88	20.209	2908	2911	2916	rVB	134901	187361	9.59%	0.664%
89	20.868	3019	3023	3027	rBV3	170321	247340	12.66%	0.877%
90	21.127	3062	3067	3072	rBV2	842152	1695776	86.78%	6.011%
91	21.174	3072	3075	3081	rVB	569484	760680	38.93%	2.697%
92	22.656	3322	3327	3331	rBV	364628	758221	38.80%	2.688%
93	23.103	3400	3403	3410	rVB	242993	409921	20.98%	1.453%
94	23.197	3414	3419	3425	rVB	458824	784092	40.13%	2.780%
95	23.291	3431	3435	3439	rVB2	257706	380531	19.47%	1.349%




Sum of corrected areas: 28209460

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031842.D
Acq On : 20 Aug 2021 15:14
Operator : CG/JU
Sample : M3394-19
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-02-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

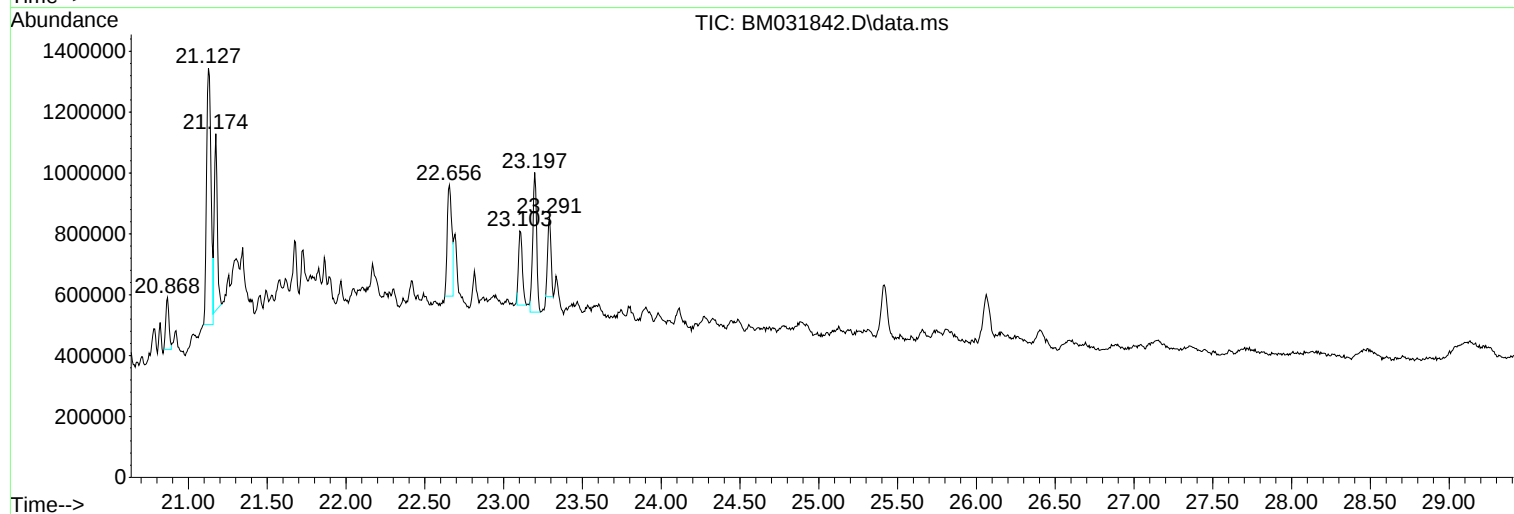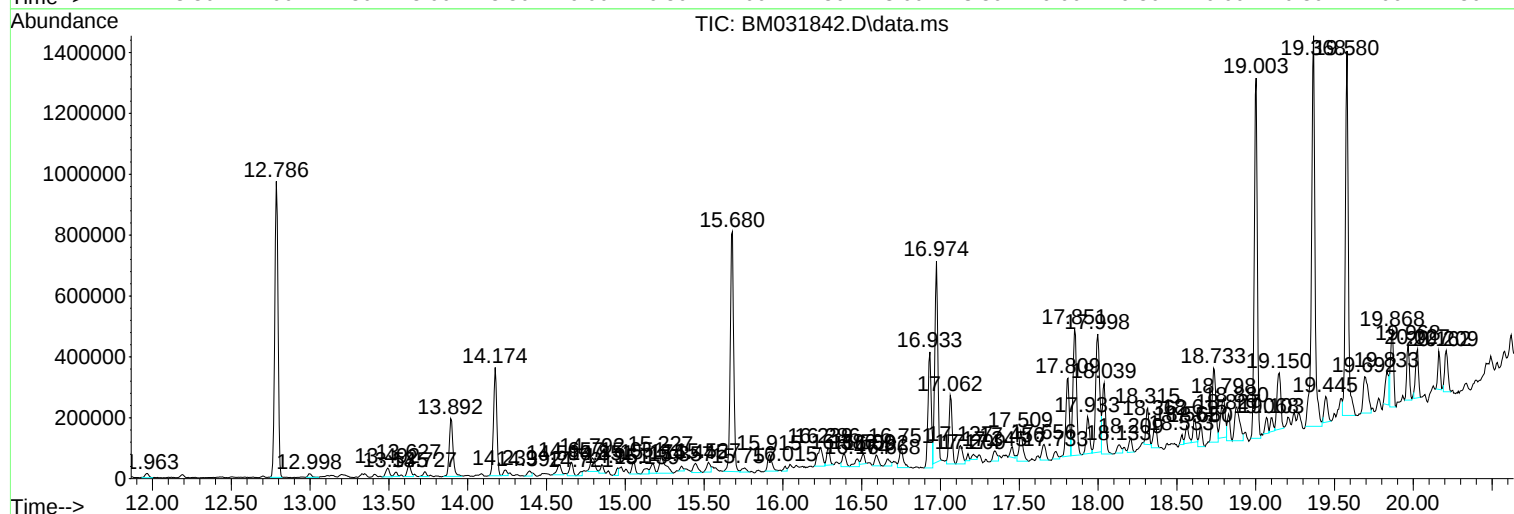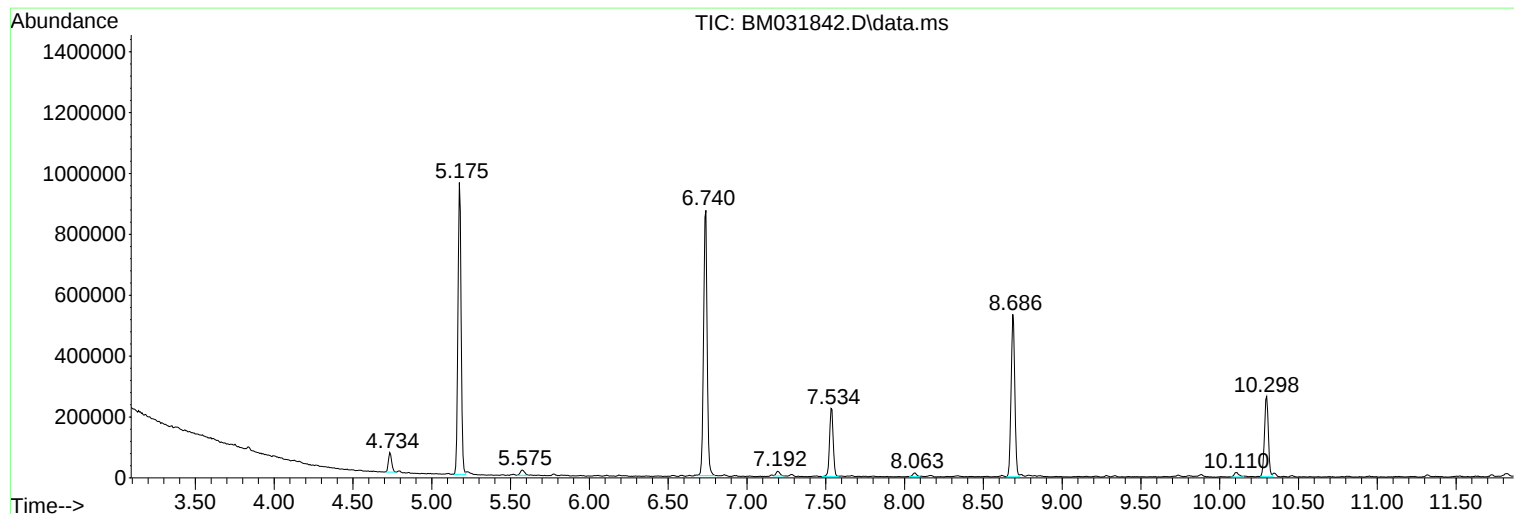

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031842.D
Acq On : 20 Aug 2021 15:14
Operator : CG/JU
Sample : M3394-19
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-02-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031842.D
Acq On : 20 Aug 2021 15:14
Operator : CG/JU
Sample : M3394-19
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-02-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------