

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031843.D
 Acq On : 20 Aug 2021 15:52
 Operator : CG/JU
 Sample : M3397-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-07-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031843.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.734	276	280	288	rVB	47236	69108	1.64%	0.173%
2	5.175	349	355	364	rBV	570602	804728	19.08%	2.012%
3	6.734	613	620	635	rVB	533316	843416	20.00%	2.108%
4	7.534	749	756	764	rBV	209961	331540	7.86%	0.829%
5	8.687	945	952	968	rBV	346147	572398	13.57%	1.431%
6	10.104	1185	1193	1205	rBV	30486	67142	1.59%	0.168%
7	10.298	1217	1226	1232	rBV	252291	416035	9.86%	1.040%
8	12.786	1642	1649	1658	rVB	740347	1069317	25.35%	2.673%
9	13.892	1830	1837	1847	rBV	102200	167699	3.98%	0.419%
10	14.174	1878	1885	1891	rBV	341642	496605	11.77%	1.241%
11	14.239	1891	1896	1904	rVB	54697	82490	1.96%	0.206%
12	14.580	1946	1954	1959	rBV	38207	59073	1.40%	0.148%
13	15.233	2059	2065	2077	rVB	79302	131512	3.12%	0.329%
14	15.527	2111	2115	2121	rBV2	30840	44316	1.05%	0.111%
15	15.674	2130	2140	2149	rBV	574646	849374	20.14%	2.123%
16	15.916	2176	2181	2189	rBV4	29607	54727	1.30%	0.137%
17	16.239	2225	2236	2241	rBV3	31166	75141	1.78%	0.188%
18	16.592	2291	2296	2303	rVB	56334	90421	2.14%	0.226%
19	16.663	2303	2308	2314	rBV3	31153	73301	1.74%	0.183%
20	16.751	2319	2323	2332	rVB	72071	118171	2.80%	0.295%
21	16.933	2348	2354	2357	rBV	382722	569108	13.49%	1.423%
22	16.974	2357	2361	2367	rVV	1459160	1926662	45.68%	4.816%
23	17.063	2368	2376	2382	rVV	375818	513955	12.19%	1.285%
24	17.121	2382	2386	2392	rVV3	29584	54066	1.28%	0.135%
25	17.345	2415	2424	2434	rBV	100000	211373	5.01%	0.528%
26	17.451	2438	2442	2449	rVV3	42110	76530	1.81%	0.191%
27	17.510	2449	2452	2460	rVB4	33048	68732	1.63%	0.172%
28	17.804	2497	2502	2506	rBV	163821	240906	5.71%	0.602%
29	17.851	2506	2510	2518	rVV2	319267	513650	12.18%	1.284%
30	17.933	2520	2524	2529	rVV	99559	149989	3.56%	0.375%
31	17.998	2529	2535	2539	rVV2	279814	494858	11.73%	1.237%
32	18.039	2539	2542	2549	rVB	110789	157590	3.74%	0.394%
33	18.315	2585	2589	2593	rVV	144882	182698	4.33%	0.457%
34	18.362	2593	2597	2602	rVB	124759	165953	3.93%	0.415%
35	18.562	2627	2631	2635	rVB2	39403	54814	1.30%	0.137%
36	18.609	2635	2639	2643	rVV	51822	70448	1.67%	0.176%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031843.D
 Acq On : 20 Aug 2021 15:52
 Operator : CG/JU
 Sample : M3397-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-07-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.651	2643	2646	2650	rVB2	45449	60063	1.42%	0.150%
38	18.733	2655	2660	2664	rBV	103409	176887	4.19%	0.442%
39	18.827	2674	2676	2680	rVB	44164	43403	1.03%	0.108%
40	18.880	2680	2685	2692	rBV2	123493	211006	5.00%	0.527%
41	19.004	2699	2706	2713	rBV	3203278	4217878	100.00%	10.544%
42	19.068	2714	2717	2720	rBV	34630	44988	1.07%	0.112%
43	19.104	2720	2723	2725	rVV2	44953	51926	1.23%	0.130%
44	19.145	2725	2730	2735	rVB2	111322	199952	4.74%	0.500%
45	19.245	2743	2747	2750	rVB	59334	71410	1.69%	0.179%
46	19.368	2758	2768	2776	rBV	2528647	4006892	95.00%	10.016%
47	19.439	2776	2780	2787	rVB2	114575	181497	4.30%	0.454%
48	19.545	2794	2798	2800	rBV	123412	175047	4.15%	0.438%
49	19.574	2800	2803	2808	rVB	986431	1216073	28.83%	3.040%
50	19.692	2818	2823	2830	rVB3	135772	323487	7.67%	0.809%
51	19.827	2842	2846	2849	rBV4	111128	209573	4.97%	0.524%
52	19.862	2849	2852	2857	rVB	295724	419096	9.94%	1.048%
53	19.968	2866	2870	2873	rBV	212949	260035	6.17%	0.650%
54	20.021	2873	2879	2883	rVV2	213708	371190	8.80%	0.928%
55	20.062	2883	2886	2890	rVB2	58332	80452	1.91%	0.201%
56	20.162	2900	2903	2907	rBV	88156	95051	2.25%	0.238%
57	20.209	2907	2911	2915	rBV2	104169	156346	3.71%	0.391%
58	20.615	2977	2980	2986	rVB	232203	292686	6.94%	0.732%
59	20.780	3004	3008	3011	rBV2	235612	321946	7.63%	0.805%
60	20.821	3011	3015	3018	rVV	201204	268048	6.36%	0.670%
61	20.862	3018	3022	3027	rVV3	236411	462534	10.97%	1.156%
62	20.915	3028	3031	3041	rVB	286112	393381	9.33%	0.983%
63	21.127	3061	3067	3072	rBV3	1763785	3048486	72.28%	7.621%
64	21.174	3072	3075	3084	rVB	1278178	1623170	38.48%	4.058%
65	21.286	3091	3094	3100	rBV	214465	294865	6.99%	0.737%
66	21.450	3117	3122	3126	rBV2	162355	309809	7.35%	0.774%
67	22.656	3321	3327	3332	rBV	1171826	2639615	62.58%	6.599%
68	22.815	3350	3354	3359	rVB	234680	349051	8.28%	0.873%
69	23.109	3399	3404	3412	rVB	676211	1202953	28.52%	3.007%
70	23.203	3414	3420	3426	rVV	1071608	1838637	43.59%	4.596%
71	23.286	3430	3434	3439	rVV2	324274	622293	14.75%	1.556%
72	23.333	3439	3442	3450	rVB2	297126	546770	12.96%	1.367%
73	25.421	3791	3797	3807	rVB	536064	1348853	31.98%	3.372%




Sum of corrected areas: 40003195

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031843.D
Acq On : 20 Aug 2021 15:52
Operator : CG/JU
Sample : M3397-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-07-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

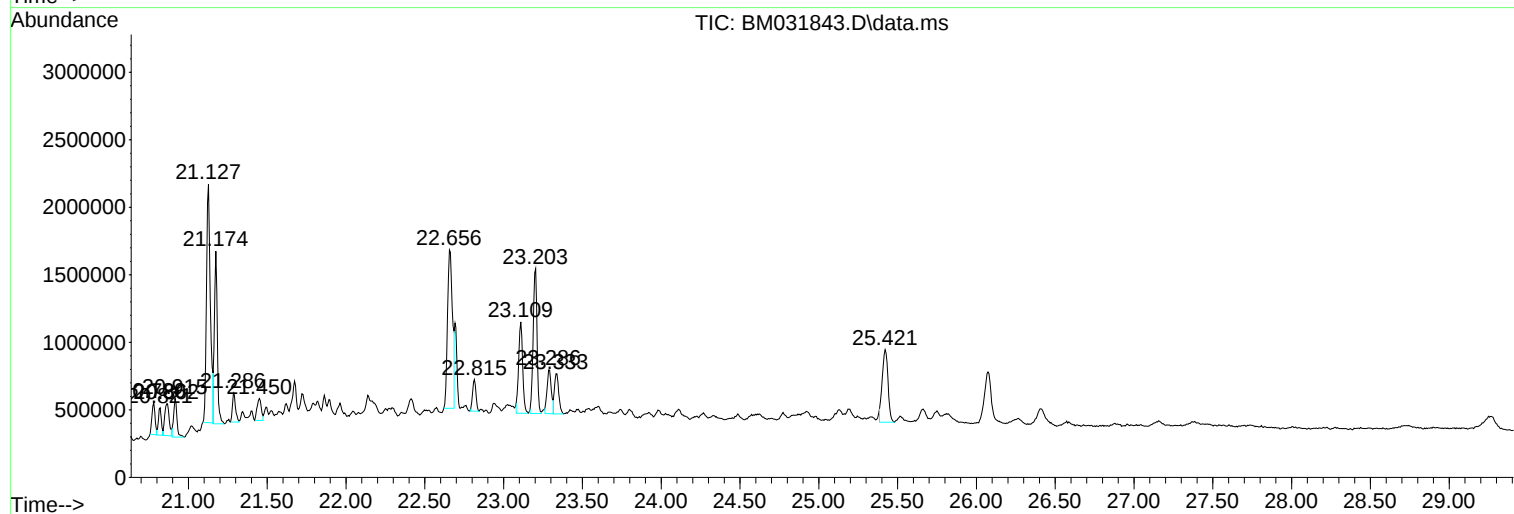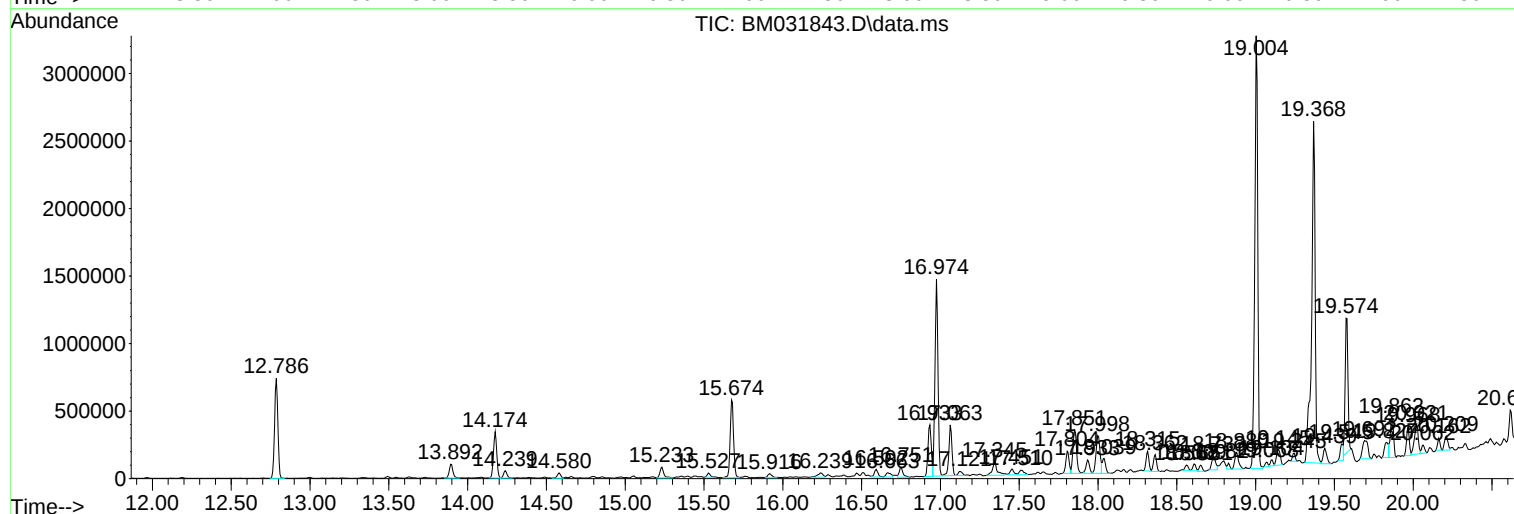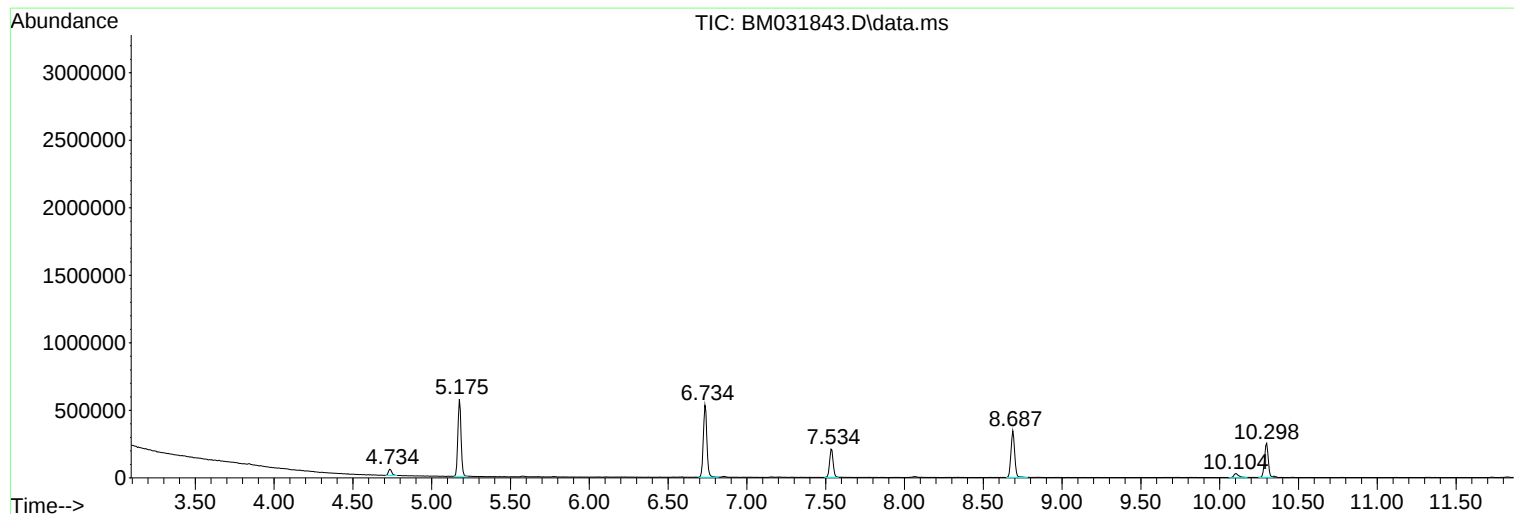

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031843.D
Acq On : 20 Aug 2021 15:52
Operator : CG/JU
Sample : M3397-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-07-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031843.D
Acq On : 20 Aug 2021 15:52
Operator : CG/JU
Sample : M3397-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-07-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------