

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031847.D
 Acq On : 20 Aug 2021 18:23
 Operator : CG/JU
 Sample : PB138447BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB138447BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031847.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.734	277	280	291	rVB2	30793	46417	1.28%	0.306%
2	5.175	349	355	366	rBV	1110628	1594532	44.06%	10.496%
3	6.740	613	621	634	rBV	1100576	1698963	46.95%	11.183%
4	7.540	750	757	764	rBV	173237	272619	7.53%	1.795%
5	8.692	945	953	964	rBV	631936	1050580	29.03%	6.915%
6	10.298	1219	1226	1237	rBV	227257	377755	10.44%	2.487%
7	12.786	1642	1649	1660	rBV	1493154	2214864	61.21%	14.579%
8	14.174	1879	1885	1899	rVB	329050	493702	13.64%	3.250%
9	15.680	2134	2141	2159	rVB	1302177	1790138	49.47%	11.784%
10	16.933	2348	2354	2368	rVB	410110	595982	16.47%	3.923%
11	17.845	2504	2509	2516	rBV3	22901	38560	1.07%	0.254%
12	19.580	2798	2804	2809	rBV	3129316	3618703	100.00%	23.820%
13	21.133	3063	3068	3075	rBV	537199	670823	18.54%	4.416%
14	23.286	3428	3434	3442	rVB2	391665	728106	20.12%	4.793%




Sum of corrected areas: 15191744

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031847.D
Acq On : 20 Aug 2021 18:23
Operator : CG/JU
Sample : PB138447BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138447BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

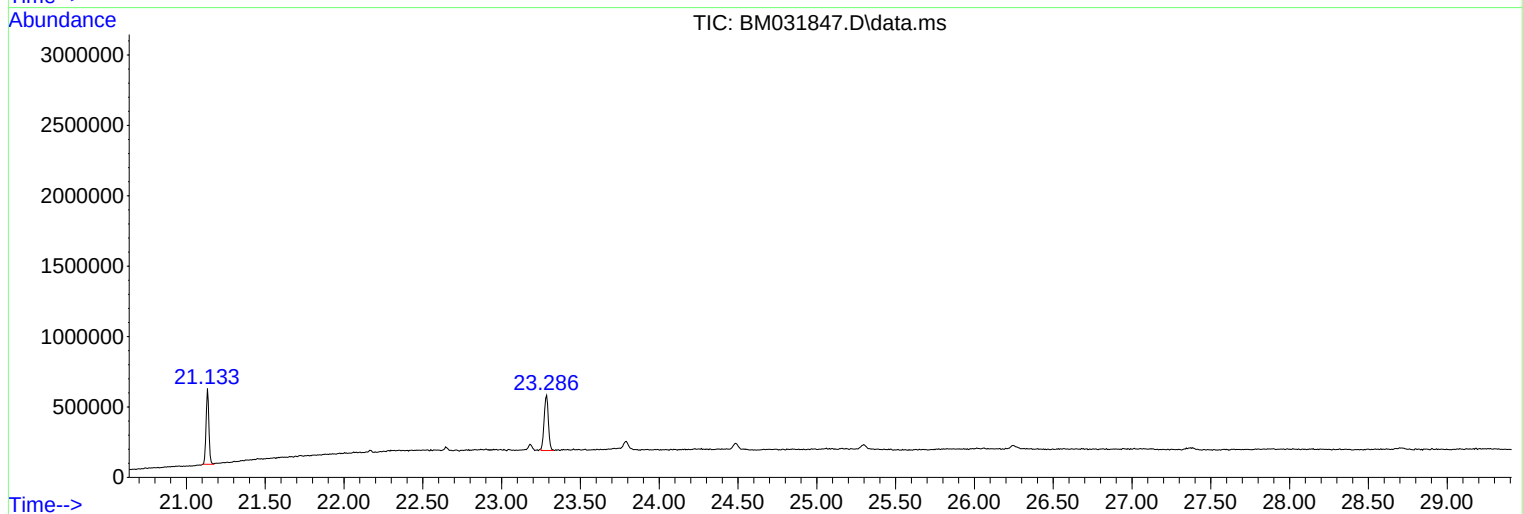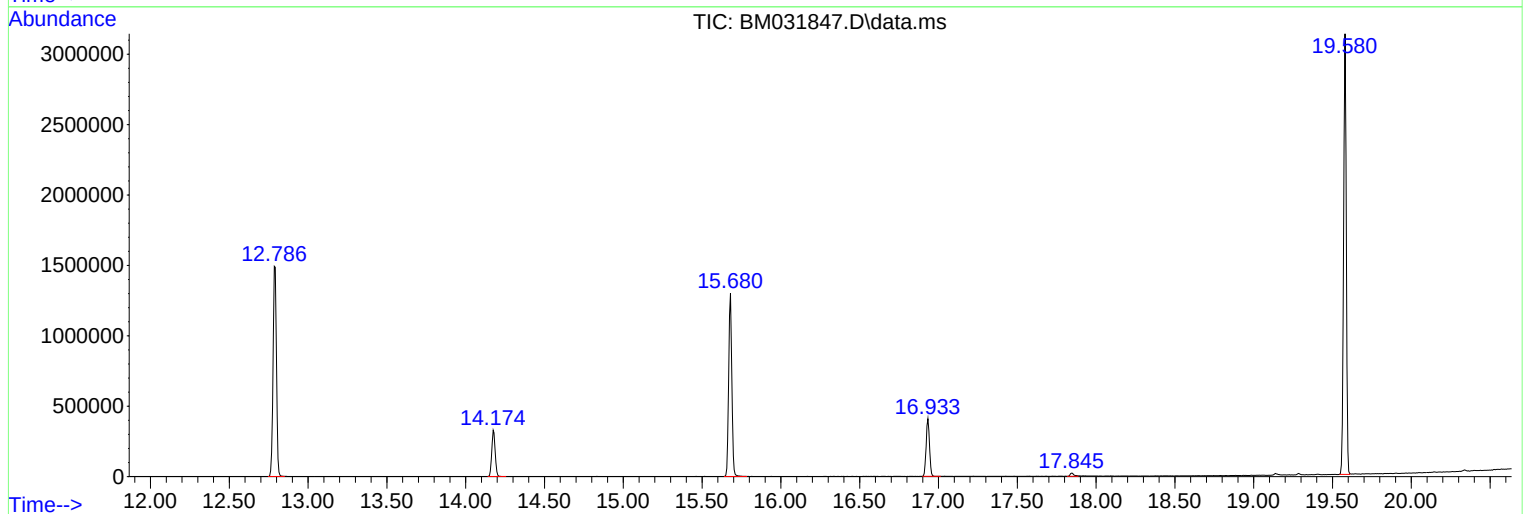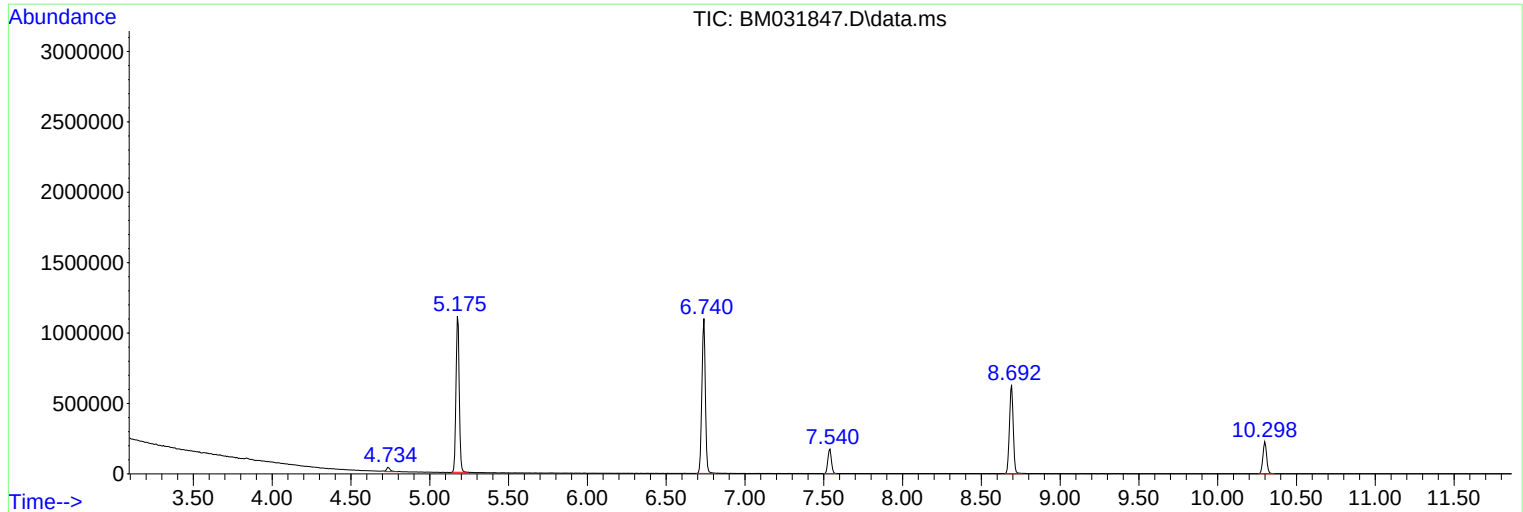

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031847.D
Acq On : 20 Aug 2021 18:23
Operator : CG/JU
Sample : PB138447BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138447BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.734	3.41 ng	46417	1,4-Dichlorobenzene-d4	7.540

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	53		
2	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39		
3	Propane, 1,1-dipropoxy-	160	C9H20O2	004744-11-0	33		
4	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	33		
5	3-Hydroxy-3-methyl-2-butanone	102	C5H10O2	000115-22-0	17		

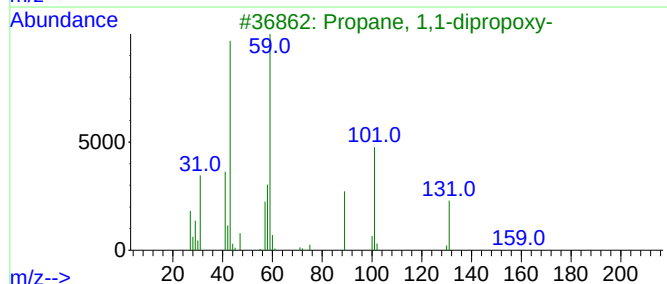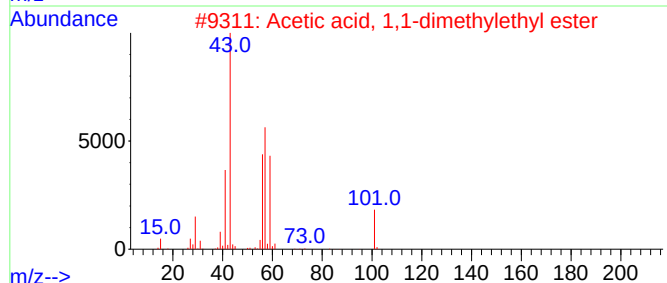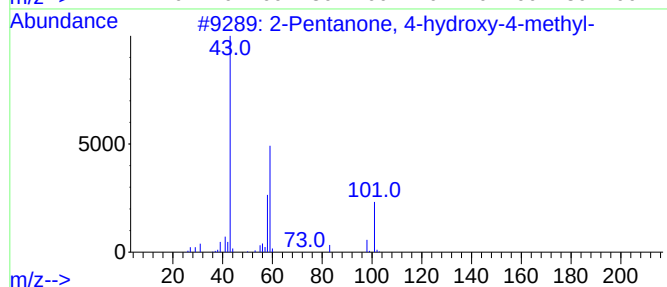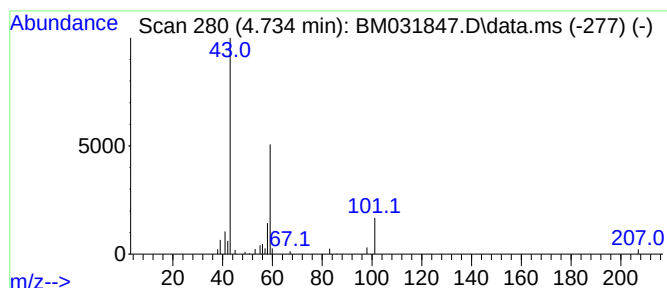

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031847.D
Acq On : 20 Aug 2021 18:23
Operator : CG/JU
Sample : PB138447BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138447BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.734	3.4	ng	46417	1	7.540	272619	20.0