

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031848.D
 Acq On : 20 Aug 2021 19:04
 Operator : CG/JU
 Sample : M3397-15
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-06-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031848.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.175	348	355	362	rBV	783191	1080768	5.29%	1.745%
2	6.734	612	620	633	rVB	734722	1129131	5.52%	1.823%
3	7.534	748	756	762	rBV	182093	281099	1.37%	0.454%
4	8.687	943	952	960	rBV	439550	717575	3.51%	1.159%
5	10.293	1217	1225	1231	rBV	236458	389918	1.91%	0.630%
6	12.787	1642	1649	1656	rBV	979410	1405658	6.87%	2.270%
7	14.175	1879	1885	1891	rBV	333362	507487	2.48%	0.819%
8	15.675	2134	2140	2148	rBV	870853	1231298	6.02%	1.988%
9	16.928	2348	2353	2357	rBV	458884	710708	3.48%	1.148%
10	16.969	2357	2360	2365	rVB	153513	217963	1.07%	0.352%
11	17.139	2384	2389	2402	rVB2	173287	613544	3.00%	0.991%
12	17.333	2412	2422	2439	rVB	479848	1664459	8.14%	2.688%
13	17.898	2498	2518	2531	rVB	6072268	17518378	85.67%	28.287%
14	18.939	2690	2695	2699	rBV	350284	501541	2.45%	0.810%
15	18.998	2700	2705	2708	rVV	973299	1601062	7.83%	2.585%
16	19.027	2708	2710	2717	rVV	712596	1316947	6.44%	2.126%
17	19.180	2721	2736	2758	rVB	8622960	20449578	100.00%	33.020%
18	19.363	2763	2767	2777	rVB	311049	477557	2.34%	0.771%
19	19.516	2788	2793	2799	rBV	212275	453258	2.22%	0.732%
20	19.580	2799	2804	2815	rVB	1571826	2025313	9.90%	3.270%
21	20.351	2929	2935	2948	rVB2	373805	809560	3.96%	1.307%
22	21.057	3049	3055	3061	rBV	646708	1091639	5.34%	1.763%
23	21.127	3062	3067	3071	rVV2	514204	857240	4.19%	1.384%
24	21.168	3071	3074	3084	rVB	169092	231378	1.13%	0.374%
25	21.686	3156	3162	3167	rBV	755939	1282215	6.27%	2.070%
26	22.345	3269	3274	3282	rVB	695309	1221639	5.97%	1.973%
27	22.645	3322	3325	3330	rBV2	151442	218884	1.07%	0.353%
28	23.098	3396	3402	3412	rBV	488163	1113962	5.45%	1.799%
29	23.186	3414	3417	3424	rVB2	181693	294066	1.44%	0.475%
30	23.280	3428	3433	3439	rVB2	320166	517153	2.53%	0.835%




Sum of corrected areas: 61930978

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031848.D
Acq On : 20 Aug 2021 19:04
Operator : CG/JU
Sample : M3397-15
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-06-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

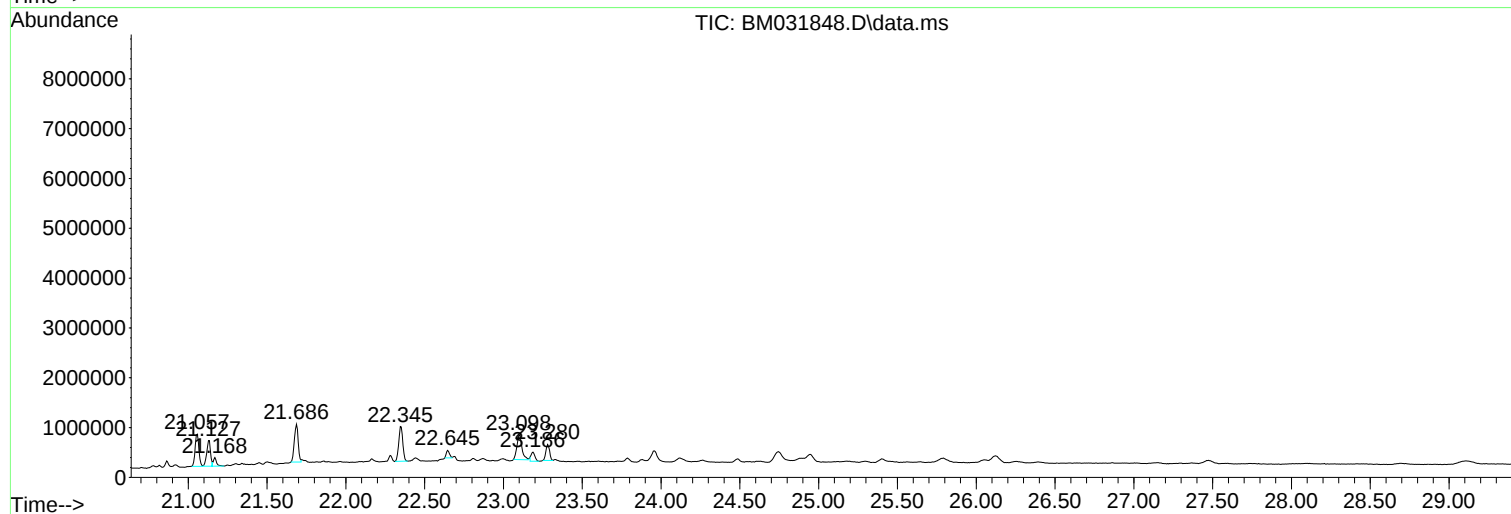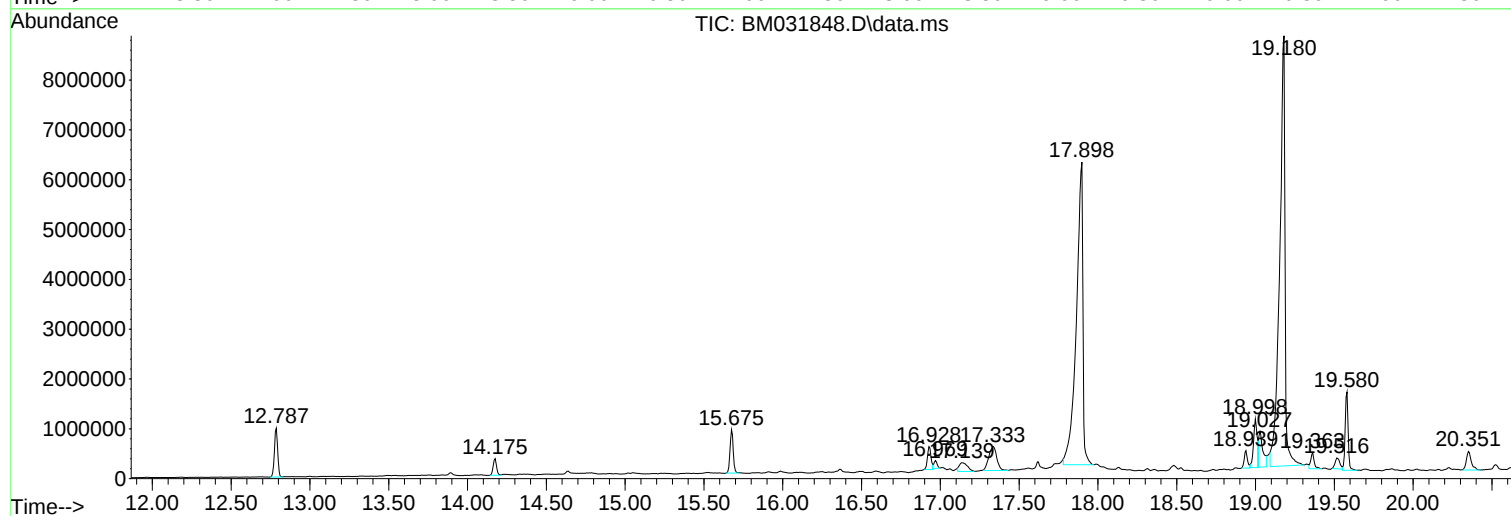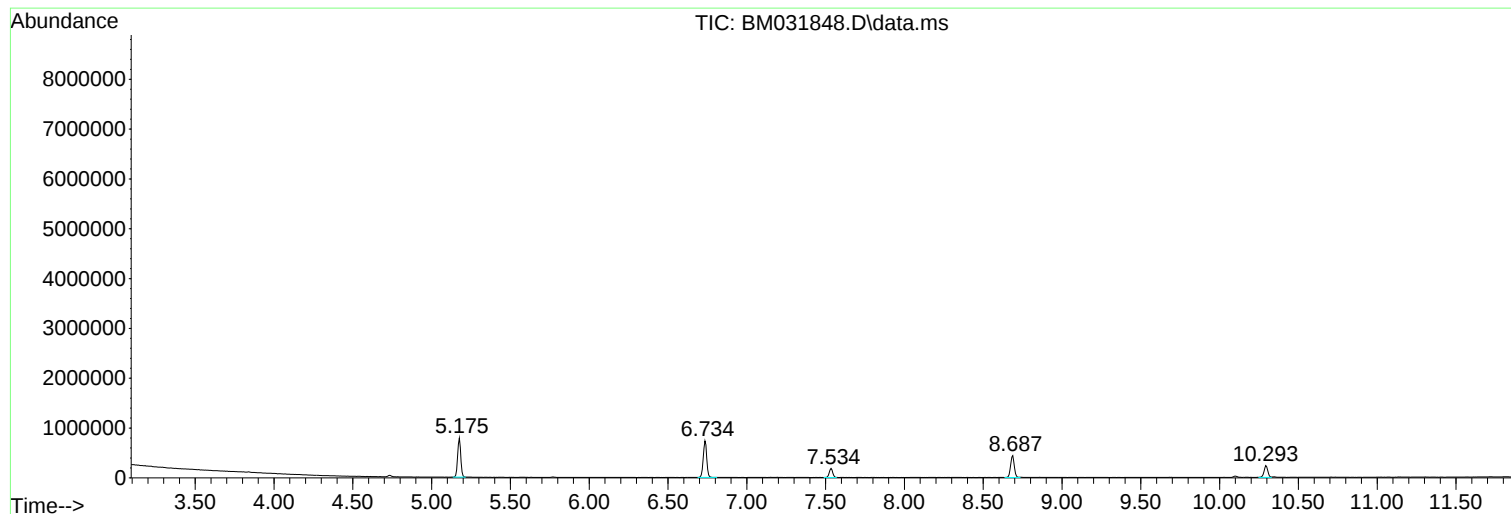

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031848.D
Acq On : 20 Aug 2021 19:04
Operator : CG/JU
Sample : M3397-15
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-06-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031848.D
Acq On : 20 Aug 2021 19:04
Operator : CG/JU
Sample : M3397-15
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-06-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------