

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031850.D
 Acq On : 20 Aug 2021 20:18
 Operator : CG/JU
 Sample : M3394-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-01-0510

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031850.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.734	276	280	288	rVB2	33013	49468	2.29%	0.341%
2	5.175	348	355	365	rVB	793019	1150406	53.31%	7.931%
3	6.734	612	620	630	rBV	797972	1234626	57.22%	8.511%
4	7.534	748	756	765	rBV	190088	291343	13.50%	2.008%
5	8.687	944	952	965	rBV	481364	780880	36.19%	5.383%
6	10.098	1186	1192	1204	rBV	26846	59607	2.76%	0.411%
7	10.292	1218	1225	1233	rBV	233192	383489	17.77%	2.644%
8	12.786	1642	1649	1661	rVB	1071386	1553455	71.99%	10.709%
9	14.174	1878	1885	1893	rVB	325368	479722	22.23%	3.307%
10	15.674	2134	2140	2150	rVB	964761	1314191	60.90%	9.060%
11	16.927	2347	2353	2357	rBV	413207	569413	26.39%	3.925%
12	16.968	2357	2360	2367	rVB	52788	72721	3.37%	0.501%
13	17.845	2503	2509	2523	rBV	452641	759473	35.20%	5.236%
14	18.933	2691	2694	2699	rBV2	16390	22199	1.03%	0.153%
15	18.992	2699	2704	2718	rBV	149504	303698	14.07%	2.094%
16	19.139	2723	2729	2749	rBV	978066	1668861	77.34%	11.505%
17	19.356	2763	2766	2771	rVB	102077	129825	6.02%	0.895%
18	19.574	2798	2803	2813	rVB	1793651	2157790	100.00%	14.876%
19	20.862	3018	3022	3027	rBV4	86636	122397	5.67%	0.844%
20	21.127	3062	3067	3071	rBV2	477604	655565	30.38%	4.519%
21	21.162	3071	3073	3079	rVB	52340	68117	3.16%	0.470%
22	22.156	3239	3242	3253	rVB2	95338	139208	6.45%	0.960%
23	23.280	3427	3433	3438	rVB2	304006	539093	24.98%	3.716%




Sum of corrected areas: 14505547

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031850.D
Acq On : 20 Aug 2021 20:18
Operator : CG/JU
Sample : M3394-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-01-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

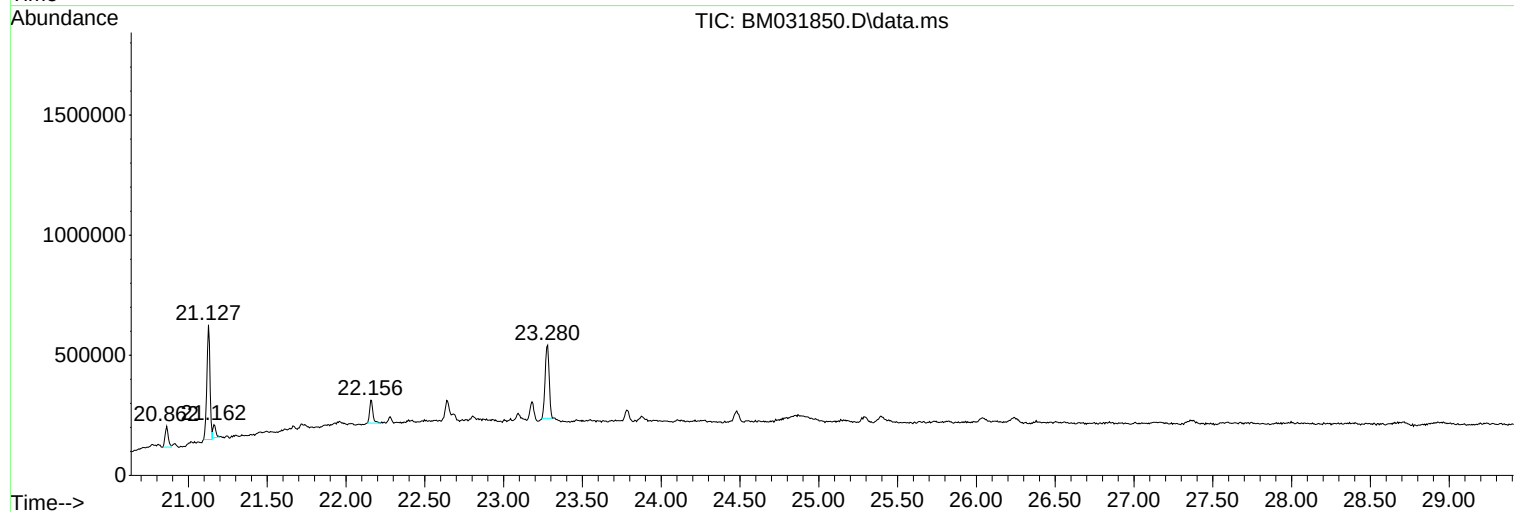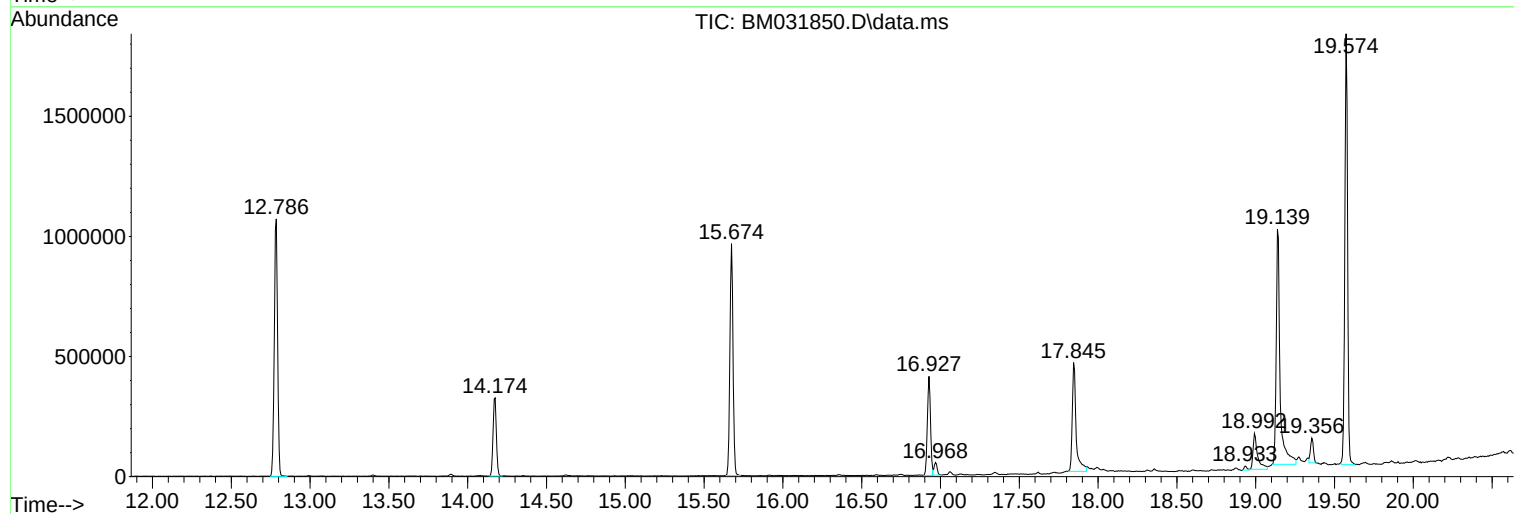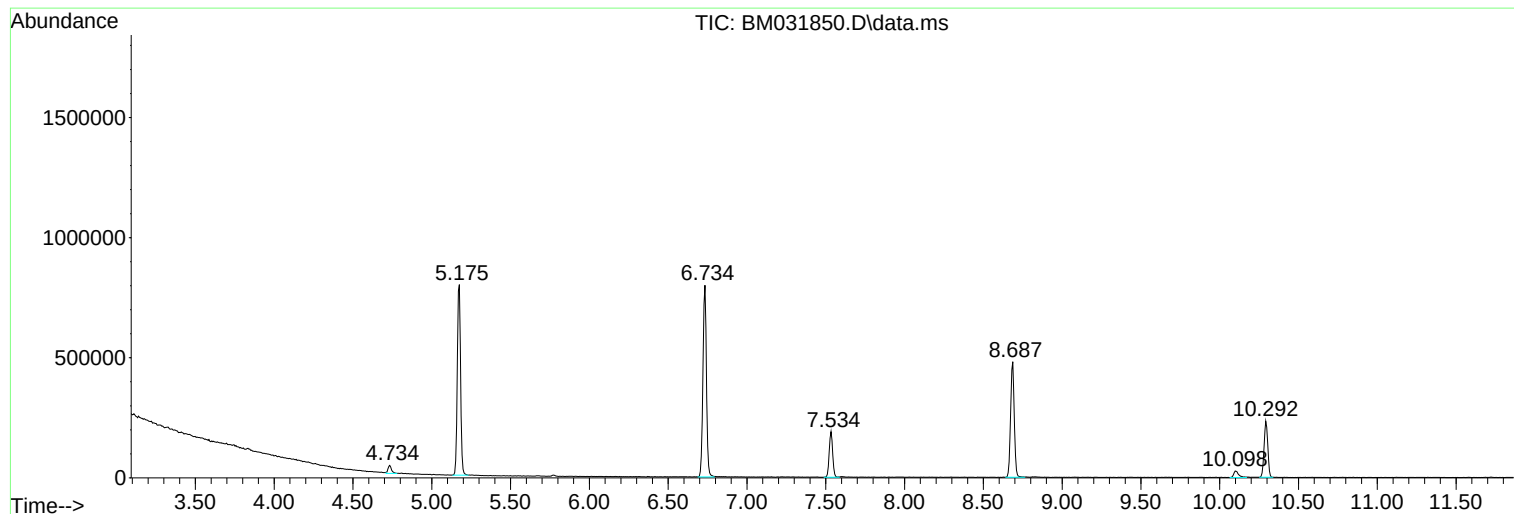

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031850.D
Acq On : 20 Aug 2021 20:18
Operator : CG/JU
Sample : M3394-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-01-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031850.D
Acq On : 20 Aug 2021 20:18
Operator : CG/JU
Sample : M3394-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-01-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------