

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031851.D
 Acq On : 20 Aug 2021 20:55
 Operator : CG/JU
 Sample : M3419-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-03-1015

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031851.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.734	276	280	287	rVB	31865	48045	2.04%	0.309%
2	5.175	348	355	365	rBV	942366	1364957	57.95%	8.771%
3	6.734	613	620	633	rBV	954043	1459277	61.95%	9.377%
4	7.534	749	756	765	rVB	184561	290131	12.32%	1.864%
5	8.687	944	952	962	rBV	565887	929388	39.45%	5.972%
6	10.098	1185	1192	1202	rBV2	32153	67037	2.85%	0.431%
7	10.293	1217	1225	1238	rVB	240391	397366	16.87%	2.553%
8	12.787	1642	1649	1658	rBV	1166630	1750027	74.29%	11.245%
9	14.175	1878	1885	1893	rVB	326865	488442	20.74%	3.139%
10	14.728	1970	1979	1994	rBV2	8489	29114	1.24%	0.187%
11	15.675	2131	2140	2149	rBV	1142992	1569931	66.65%	10.088%
12	15.904	2175	2179	2188	rVB	18053	27350	1.16%	0.176%
13	16.927	2347	2353	2358	rBV	404385	570984	24.24%	3.669%
14	16.969	2358	2360	2367	rVB	22396	28711	1.22%	0.184%
15	17.851	2500	2510	2518	rBV	509661	779434	33.09%	5.009%
16	18.551	2626	2629	2634	rVB	41805	53607	2.28%	0.344%
17	18.998	2700	2705	2711	rBV3	53456	141854	6.02%	0.912%
18	19.145	2723	2730	2750	rBV	1155753	1837243	78.00%	11.806%
19	19.357	2763	2766	2771	rVB	33102	41505	1.76%	0.267%
20	19.574	2798	2803	2813	rVB	2017775	2355577	100.00%	15.137%
21	20.862	3018	3022	3028	rBV2	118342	152681	6.48%	0.981%
22	21.127	3063	3067	3071	rBV	463383	560184	23.78%	3.600%
23	22.162	3240	3243	3247	rBV3	75451	86202	3.66%	0.554%
24	23.280	3428	3433	3439	rVB2	314078	533024	22.63%	3.425%




Sum of corrected areas: 15562071

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031851.D
Acq On : 20 Aug 2021 20:55
Operator : CG/JU
Sample : M3419-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-03-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

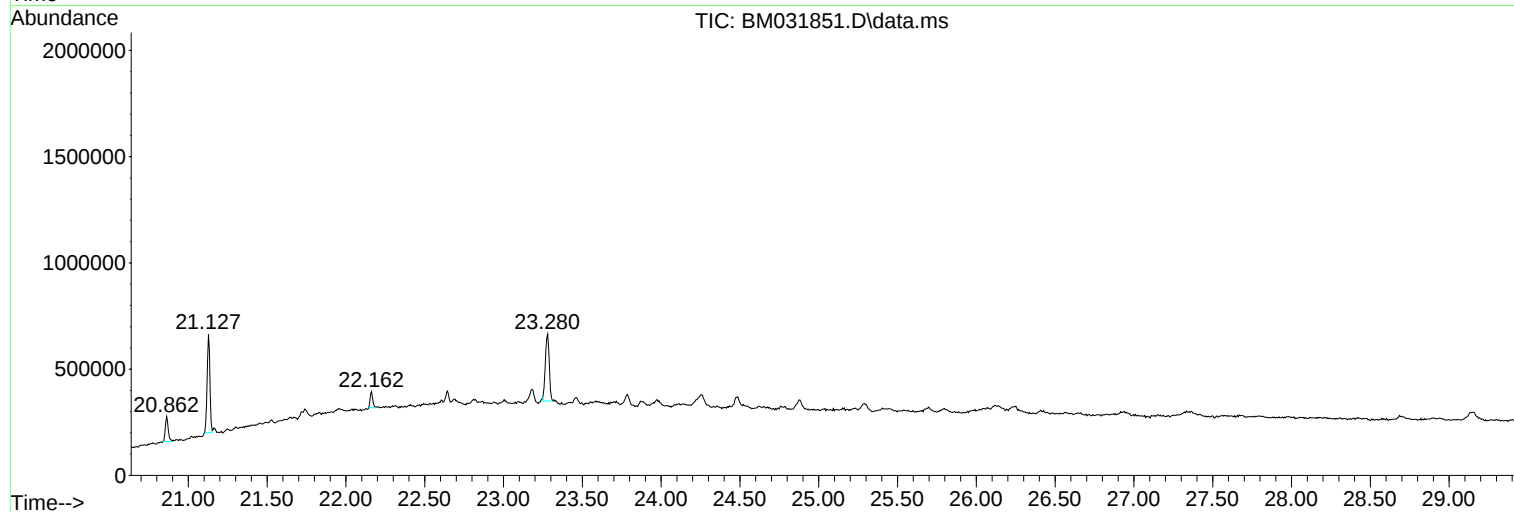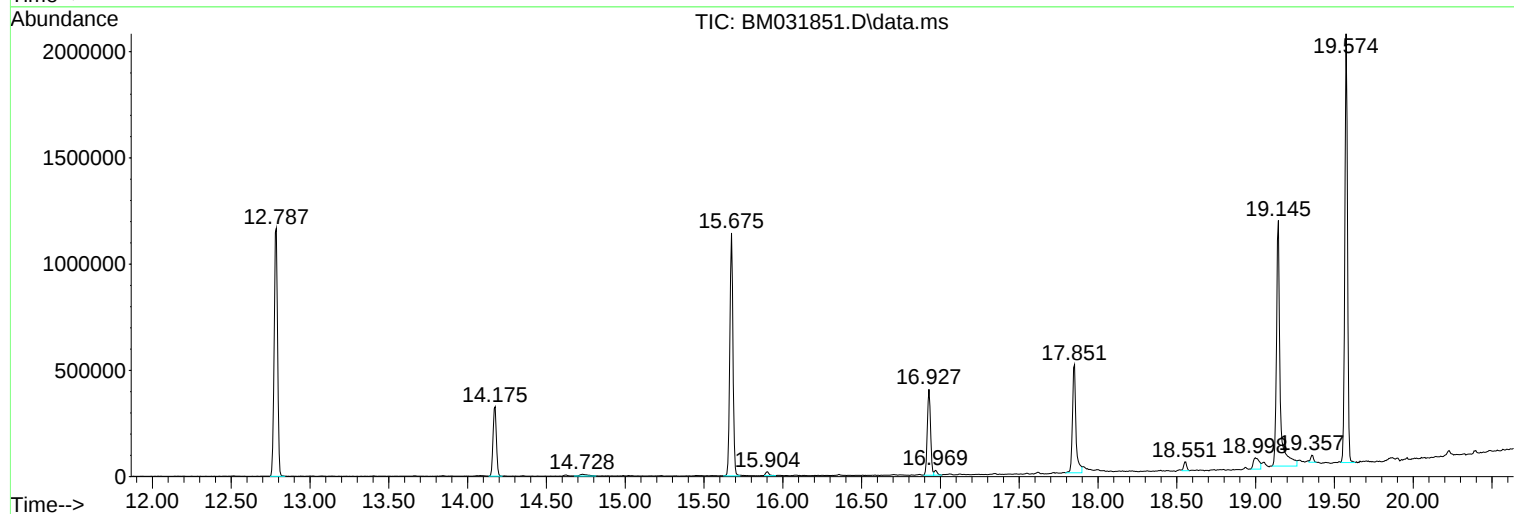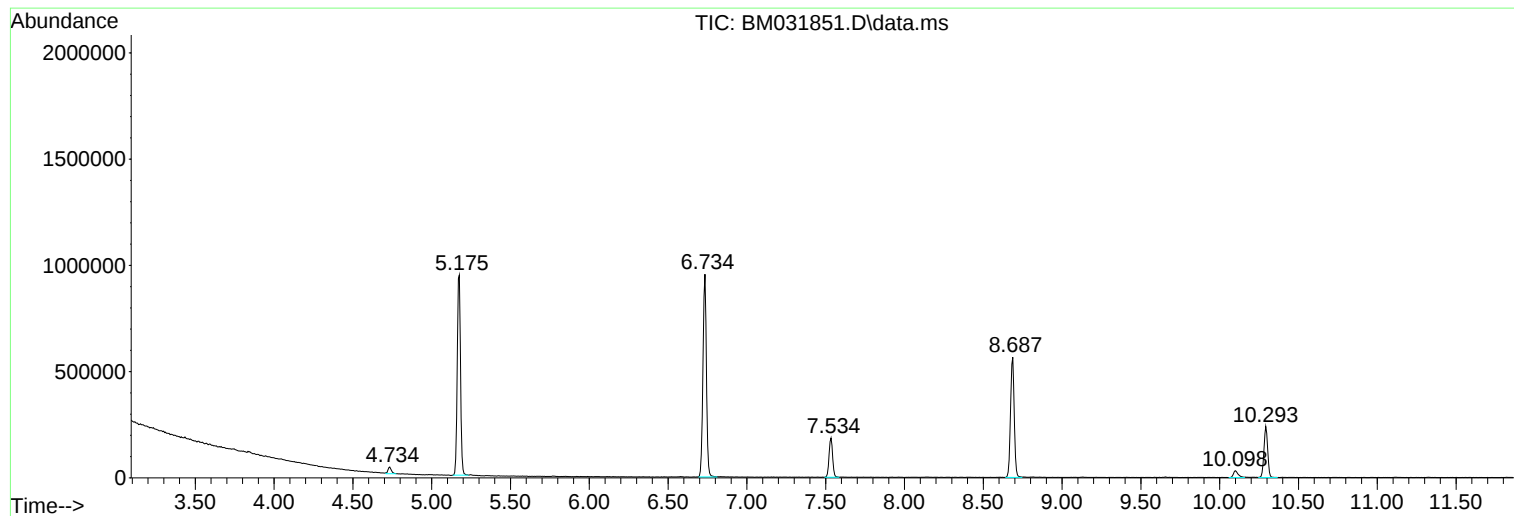

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031851.D
Acq On : 20 Aug 2021 20:55
Operator : CG/JU
Sample : M3419-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-03-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031851.D
Acq On : 20 Aug 2021 20:55
Operator : CG/JU
Sample : M3419-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-03-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------