

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031855.D
 Acq On : 20 Aug 2021 23:24
 Operator : CG/JU
 Sample : M3435-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-17-0306

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031855.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.834	124	127	135	rVB2	70568	110050	2.13%	0.201%
2	4.334	207	212	221	rVB	209204	313343	6.06%	0.571%
3	5.175	348	355	360	rVV	796043	1169068	22.60%	2.132%
4	5.228	360	364	380	rVB	42990	110907	2.14%	0.202%
5	5.581	418	424	430	rVB	95214	139653	2.70%	0.255%
6	5.828	459	466	474	rBV7	25909	65835	1.27%	0.120%
7	6.034	494	501	509	rBV5	36744	72899	1.41%	0.133%
8	6.104	509	513	518	rBV	47821	65416	1.26%	0.119%
9	6.534	582	586	591	rVB2	43403	64400	1.25%	0.117%
10	6.734	614	620	631	rVB	780335	1294723	25.03%	2.361%
11	7.157	686	692	694	rBV	106077	155278	3.00%	0.283%
12	7.181	694	696	703	rVB	75187	99720	1.93%	0.182%
13	7.440	729	740	745	rBV6	22693	67404	1.30%	0.123%
14	7.534	745	756	761	rBV2	177360	326560	6.31%	0.595%
15	8.069	841	847	851	rVB4	38216	69792	1.35%	0.127%
16	8.687	945	952	958	rBV	491216	818046	15.82%	1.492%
17	8.740	958	961	970	rVB	49375	73151	1.41%	0.133%
18	10.092	1182	1191	1199	rBV	105851	197568	3.82%	0.360%
19	10.292	1210	1225	1229	rBV	246170	496586	9.60%	0.905%
20	10.339	1229	1233	1240	rVB	166222	280101	5.42%	0.511%
21	11.722	1460	1468	1479	rBV2	51229	93057	1.80%	0.170%
22	11.963	1499	1509	1515	rBV	140647	231896	4.48%	0.423%
23	12.110	1526	1534	1541	rBV3	27361	91439	1.77%	0.167%
24	12.186	1541	1547	1556	rVB	70978	136197	2.63%	0.248%
25	12.786	1642	1649	1656	rVB	891609	1314100	25.41%	2.396%
26	12.992	1679	1684	1690	rVB2	86387	123210	2.38%	0.225%
27	13.104	1695	1703	1707	rBV3	40548	73269	1.42%	0.134%
28	13.322	1735	1740	1743	rBV2	39509	72729	1.41%	0.133%
29	13.486	1762	1768	1773	rBV2	67023	127817	2.47%	0.233%
30	13.539	1773	1777	1781	rVV	43393	69038	1.33%	0.126%
31	13.892	1831	1837	1847	rVB	149688	239503	4.63%	0.437%
32	14.086	1861	1870	1875	rVB2	71510	117575	2.27%	0.214%
33	14.169	1877	1884	1890	rBV	316518	507335	9.81%	0.925%
34	14.386	1917	1921	1930	rVB6	24281	64318	1.24%	0.117%
35	14.574	1948	1953	1958	rVB	72425	103981	2.01%	0.190%
36	14.733	1972	1980	1984	rBV2	44647	136527	2.64%	0.249%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031855.D
 Acq On : 20 Aug 2021 23:24
 Operator : CG/JU
 Sample : M3435-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-17-0306

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	14.798	1986	1991	1996	rVV7	42334	107632	2.08%	0.196%
38	15.045	2029	2033	2038	rVB2	86885	107593	2.08%	0.196%
39	15.227	2059	2064	2069	rBV3	102631	135465	2.62%	0.247%
40	15.451	2096	2102	2107	rVV4	54262	103559	2.00%	0.189%
41	15.527	2111	2115	2124	rVB6	37404	71846	1.39%	0.131%
42	15.674	2131	2140	2148	rVB	846298	1278899	24.73%	2.332%
43	15.910	2173	2180	2189	rBV4	153714	349118	6.75%	0.637%
44	16.133	2214	2218	2225	rBV4	73136	117944	2.28%	0.215%
45	16.239	2230	2236	2240	rVV5	38864	88427	1.71%	0.161%
46	16.351	2250	2255	2264	rVV6	72712	144426	2.79%	0.263%
47	16.504	2278	2281	2285	rVB2	49277	61549	1.19%	0.112%
48	16.586	2291	2295	2303	rVB2	54450	80496	1.56%	0.147%
49	16.704	2311	2315	2318	rBV	65412	79929	1.55%	0.146%
50	16.751	2318	2323	2331	rVB2	98633	176081	3.40%	0.321%
51	16.927	2348	2353	2356	rBV	376761	530414	10.26%	0.967%
52	16.968	2356	2360	2366	rVV	648520	924994	17.88%	1.686%
53	17.057	2368	2375	2381	rVB	187987	335625	6.49%	0.612%
54	17.127	2382	2387	2391	rBV4	73900	125425	2.43%	0.229%
55	17.339	2419	2423	2431	rVB	76315	120580	2.33%	0.220%
56	17.439	2437	2440	2444	rVB2	70545	87837	1.70%	0.160%
57	17.804	2498	2502	2505	rBV	121100	160222	3.10%	0.292%
58	17.851	2505	2510	2517	rVB	576460	805723	15.58%	1.469%
59	17.992	2529	2534	2538	rBV2	203138	359231	6.95%	0.655%
60	18.033	2539	2541	2548	rVB	113203	136948	2.65%	0.250%
61	18.133	2555	2558	2564	rBV3	55251	66766	1.29%	0.122%
62	18.204	2567	2570	2575	rVB4	59310	73239	1.42%	0.134%
63	18.310	2585	2588	2592	rBV	96958	133639	2.58%	0.244%
64	18.357	2593	2596	2599	rVV	121575	156317	3.02%	0.285%
65	18.398	2599	2603	2608	rVB	249831	317264	6.13%	0.578%
66	18.609	2636	2639	2643	rBV2	87439	117905	2.28%	0.215%
67	18.733	2653	2660	2664	rBV2	202541	489158	9.46%	0.892%
68	18.780	2665	2668	2673	rVV4	122182	216584	4.19%	0.395%
69	18.827	2673	2676	2679	rVB2	71130	76688	1.48%	0.140%
70	18.998	2700	2705	2710	rBV	1208497	1605060	31.03%	2.926%
71	19.062	2712	2716	2720	rVB3	120680	185377	3.58%	0.338%
72	19.139	2725	2729	2735	rBV2	540296	761111	14.72%	1.388%
73	19.333	2758	2762	2763	rBV	130473	168403	3.26%	0.307%
74	19.362	2763	2767	2771	rVB	1006584	1219837	23.59%	2.224%
75	19.574	2799	2803	2814	rVB	1190772	1542720	29.83%	2.813%
76	19.786	2835	2839	2843	rBV	441906	548275	10.60%	1.000%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031855.D
 Acq On : 20 Aug 2021 23:24
 Operator : CG/JU
 Sample : M3435-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-17-0306

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	19.868	2849	2853	2857	rBV2	362368	484378	9.37%	0.883%
78	19.962	2866	2869	2873	rVB	179801	210593	4.07%	0.384%
79	20.133	2895	2898	2901	rBV	143409	184914	3.58%	0.337%
80	20.862	3018	3022	3029	rBV3	1074175	1393720	26.95%	2.541%
81	20.986	3040	3043	3046	rBV	160866	183189	3.54%	0.334%
82	21.062	3054	3056	3061	rVB	376443	351393	6.79%	0.641%
83	21.127	3062	3067	3071	rVV2	731989	1421354	27.48%	2.591%
84	21.168	3071	3074	3083	rVB	881323	1159113	22.41%	2.113%
85	21.750	3165	3173	3180	rBV3	946007	1924542	37.21%	3.509%
86	22.209	3248	3251	3255	rVB	213167	269220	5.21%	0.491%
87	22.650	3321	3326	3330	rBV	827640	1398722	27.04%	2.550%
88	22.697	3330	3334	3342	rVB2	954002	1674723	32.38%	3.053%
89	22.774	3343	3347	3351	rBV	800386	1088246	21.04%	1.984%
90	23.103	3400	3403	3410	rVB	312355	480182	9.28%	0.875%
91	23.192	3414	3418	3424	rVB	486562	821141	15.88%	1.497%
92	23.692	3500	3503	3514	rVB	319652	661077	12.78%	1.205%
93	23.791	3516	3520	3528	rVB2	318912	552144	10.68%	1.007%
94	23.880	3531	3535	3544	rVB	377006	763302	14.76%	1.392%
95	23.974	3546	3551	3557	rBV	558836	1007016	19.47%	1.836%
96	24.239	3589	3596	3609	rVB5	788674	2487487	48.10%	4.535%
97	25.827	3857	3866	3876	rVB3	1115452	3179270	61.47%	5.797%
98	26.150	3915	3921	3932	rVB2	480003	1351549	26.13%	2.464%
99	26.321	3940	3950	3960	rVB3	1766758	5171976	100.00%	9.430%
100	26.674	4002	4010	4026	rVB5	840669	2967100	57.37%	5.410%




Sum of corrected areas: 54847148

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031855.D
Acq On : 20 Aug 2021 23:24
Operator : CG/JU
Sample : M3435-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-17-0306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

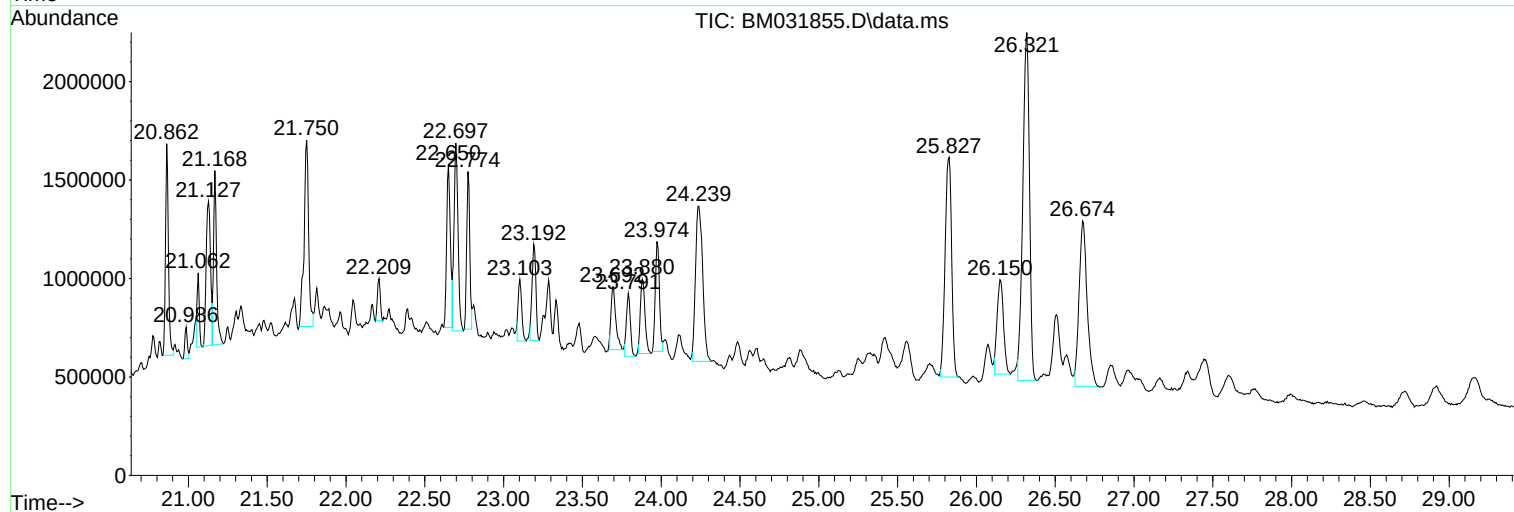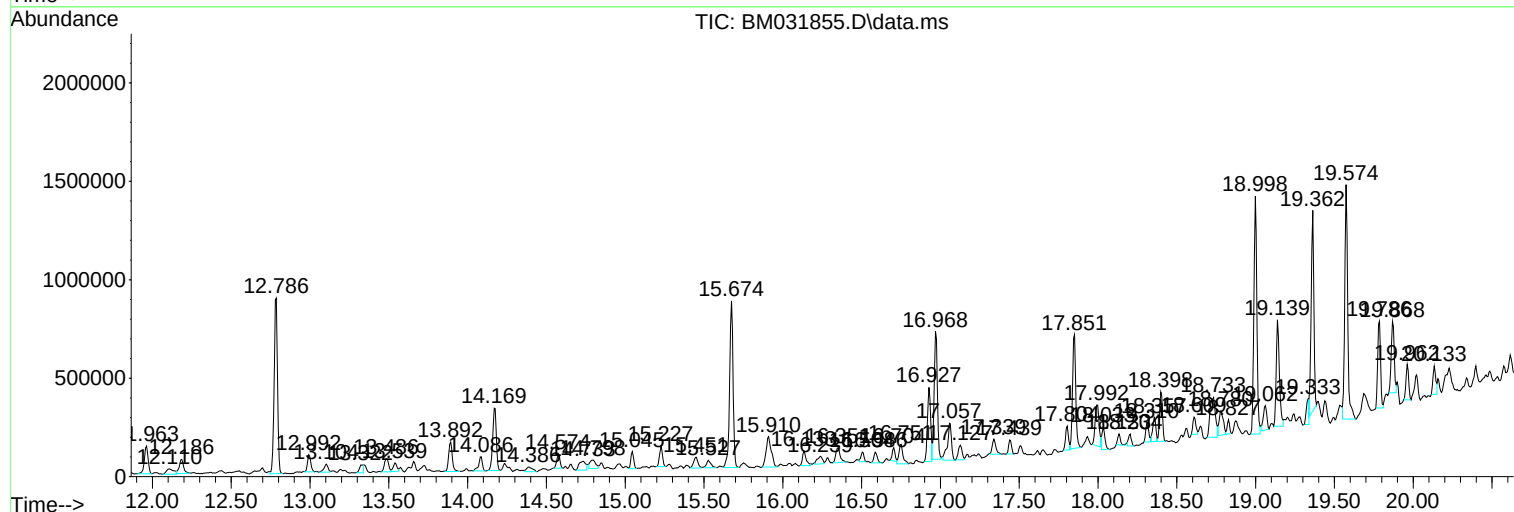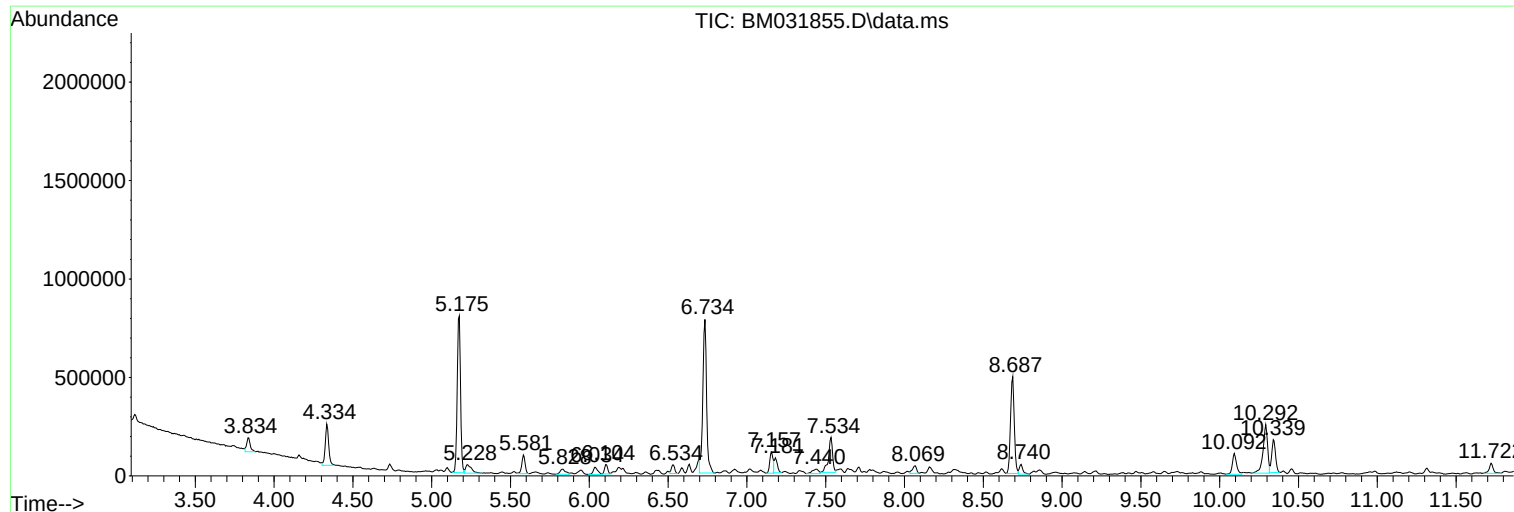

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031855.D
Acq On : 20 Aug 2021 23:24
Operator : CG/JU
Sample : M3435-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-17-0306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031855.D
Acq On : 20 Aug 2021 23:24
Operator : CG/JU
Sample : M3435-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-17-0306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------