

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031856.D
 Acq On : 21 Aug 2021 00:02
 Operator : CG/JU
 Sample : M3435-29
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-22-0003

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031856.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.175	349	355	367	rVB	734511	1057732	9.58%	2.185%
2	6.734	612	620	632	rBV	701168	1111907	10.07%	2.296%
3	7.534	749	756	765	rBV	184623	281244	2.55%	0.581%
4	8.686	944	952	960	rBV	427281	710405	6.43%	1.467%
5	10.292	1218	1225	1233	rVB	224492	372159	3.37%	0.769%
6	12.786	1642	1649	1657	rVB	732953	1114538	10.09%	2.302%
7	14.174	1878	1885	1892	rBV	301002	456261	4.13%	0.942%
8	15.674	2132	2140	2150	rBV	748326	1039948	9.42%	2.148%
9	16.927	2346	2353	2358	rBV	385356	536590	4.86%	1.108%
10	17.845	2504	2509	2520	rBV	183171	297228	2.69%	0.614%
11	17.980	2527	2532	2541	rVB	247052	322721	2.92%	0.667%
12	18.603	2634	2638	2650	rVB2	71305	125172	1.13%	0.259%
13	18.709	2652	2656	2664	rBV	229141	360296	3.26%	0.744%
14	18.992	2700	2704	2712	rBV	67689	143081	1.30%	0.296%
15	19.133	2724	2728	2736	rBV	134706	196945	1.78%	0.407%
16	19.574	2798	2803	2809	rVB	905664	1102512	9.98%	2.277%
17	19.868	2849	2853	2856	rBV	212075	284473	2.58%	0.588%
18	19.898	2856	2858	2862	rVB	109935	111850	1.01%	0.231%
19	20.774	3003	3007	3012	rVB2	98770	120039	1.09%	0.248%
20	20.862	3017	3022	3032	rBV	845031	1211888	10.97%	2.503%
21	20.980	3039	3042	3048	rBV3	121084	154465	1.40%	0.319%
22	21.127	3063	3067	3071	rBV	399406	502891	4.55%	1.039%
23	21.162	3071	3073	3081	rVB2	125926	164226	1.49%	0.339%
24	21.327	3098	3101	3107	rVB2	146188	220282	1.99%	0.455%
25	21.550	3136	3139	3143	rVB	133349	144478	1.31%	0.298%
26	21.750	3164	3173	3180	rBV2	1163271	2235708	20.24%	4.617%
27	21.809	3180	3183	3188	rVB	148403	165140	1.50%	0.341%
28	22.039	3219	3222	3228	rBV2	128495	187358	1.70%	0.387%
29	22.203	3246	3250	3255	rVB	276029	376806	3.41%	0.778%
30	22.380	3277	3280	3289	rVB3	136446	181662	1.64%	0.375%
31	22.644	3321	3325	3329	rBV	428853	607979	5.50%	1.256%
32	22.697	3329	3334	3341	rVV	1245176	1984269	17.97%	4.098%
33	22.774	3342	3347	3358	rVB	1006438	1509600	13.67%	3.118%
34	23.250	3424	3428	3429	rBV	150563	196340	1.78%	0.406%
35	23.280	3430	3433	3438	rVV	293452	470803	4.26%	0.972%
36	23.333	3438	3442	3449	rVB2	171742	277044	2.51%	0.572%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031856.D
Acq On : 21 Aug 2021 00:02
Operator : CG/JU
Sample : M3435-29
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-22-0003

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	23.691	3498	3503	3512	rVB	412342	798911	7.23%	1.650%
38	23.785	3515	3519	3527	rVB	300872	553710	5.01%	1.144%
39	23.880	3529	3535	3544	rVV	628767	1369403	12.40%	2.828%
40	23.974	3545	3551	3555	rVV	807468	1532668	13.88%	3.165%
41	24.021	3555	3559	3567	rVB	573872	1069596	9.68%	2.209%
42	24.227	3588	3594	3608	rBV	435903	1055035	9.55%	2.179%
43	26.150	3914	3921	3936	rBV3	384749	1169300	10.59%	2.415%
44	26.315	3939	3949	3960	rVB2	2544652	7185985	65.06%	14.841%
45	26.503	3974	3981	3992	rVB2	466432	1344005	12.17%	2.776%
46	26.685	3999	4012	4030	rVB2	3299104	11044632	100.00%	22.811%
47	26.850	4034	4040	4050	rVB3	325648	959760	8.69%	1.982%




Sum of corrected areas: 48419045

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031856.D
Acq On : 21 Aug 2021 00:02
Operator : CG/JU
Sample : M3435-29
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-22-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

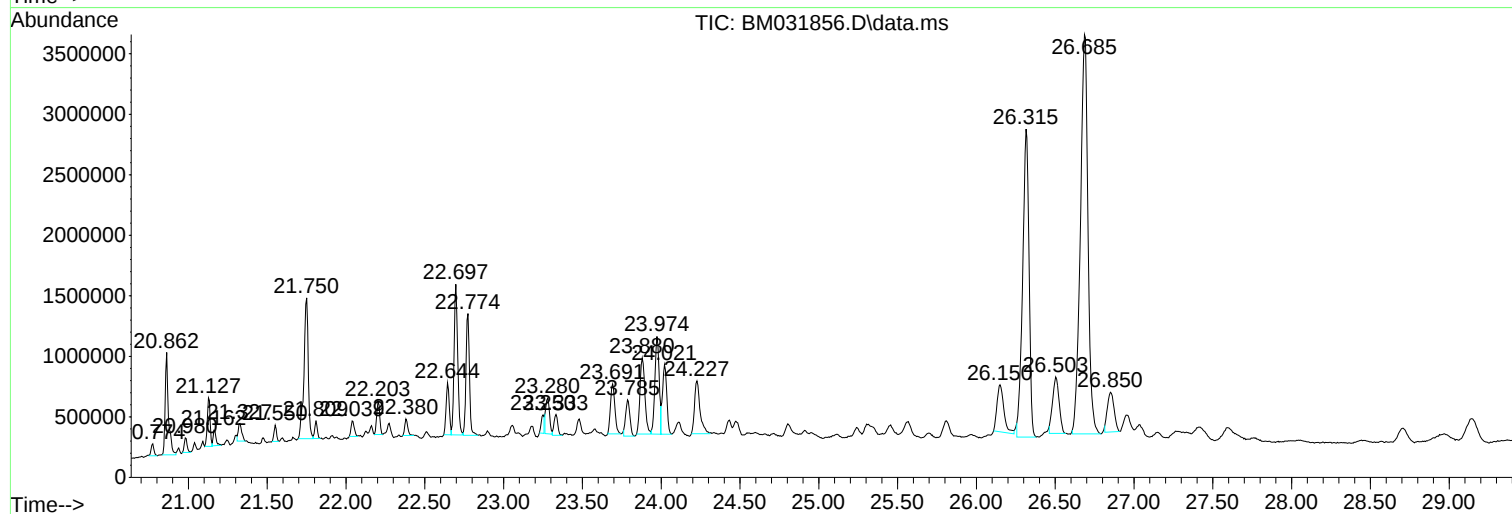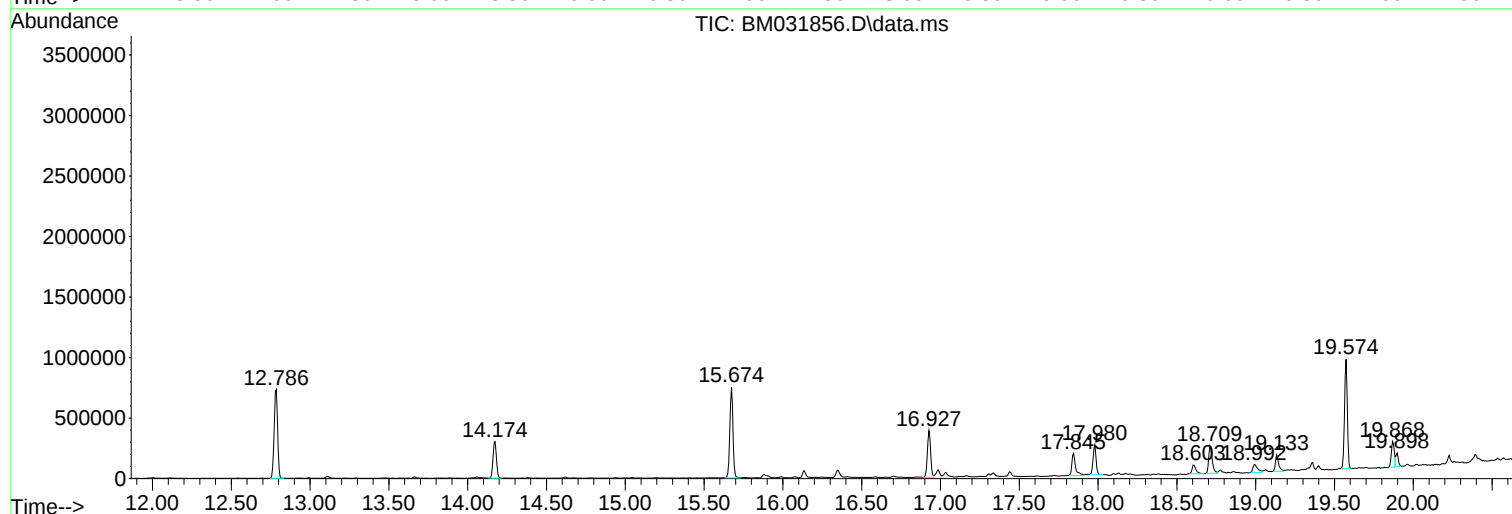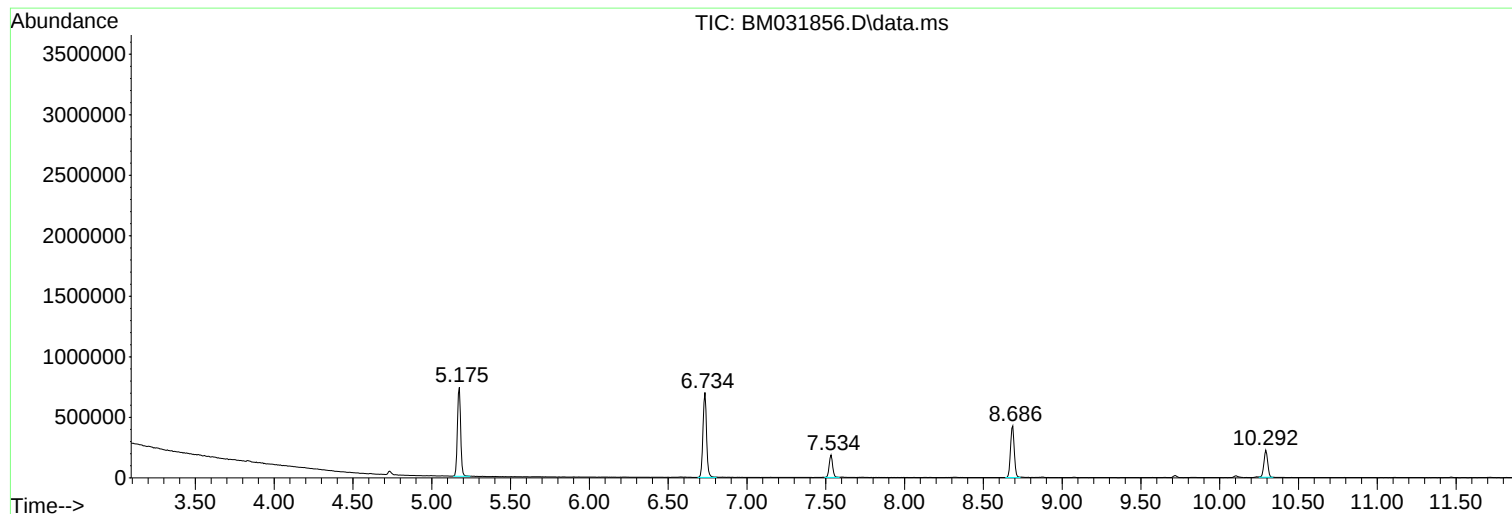

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031856.D
Acq On : 21 Aug 2021 00:02
Operator : CG/JU
Sample : M3435-29
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-22-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031856.D
Acq On : 21 Aug 2021 00:02
Operator : CG/JU
Sample : M3435-29
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-22-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
