

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031857.D
 Acq On : 21 Aug 2021 00:38
 Operator : CG/JU
 Sample : M3434-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-11-0510

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031857.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.734	277	280	290	rVB	22723	36285	1.81%	0.309%
2	5.175	348	355	365	rVB	881776	1250086	62.24%	10.653%
3	6.734	612	620	635	rBV	847827	1303476	64.90%	11.108%
4	7.534	750	756	764	rBV	178819	277258	13.80%	2.363%
5	8.686	944	952	964	rBV	500407	820872	40.87%	6.995%
6	10.104	1186	1193	1205	rBV2	18283	40709	2.03%	0.347%
7	10.292	1218	1225	1234	rBV	223824	369388	18.39%	3.148%
8	12.786	1641	1649	1656	rBV	1042194	1572791	78.31%	13.403%
9	14.174	1878	1885	1895	rVB	305946	453607	22.58%	3.866%
10	15.674	2132	2140	2150	rBV	954698	1317093	65.58%	11.224%
11	16.927	2347	2353	2361	rBV	380678	520912	25.94%	4.439%
12	17.845	2503	2509	2519	rBV	183492	272314	13.56%	2.321%
13	18.709	2652	2656	2664	rBV	33456	55770	2.78%	0.475%
14	19.133	2724	2728	2736	rBV	104759	157630	7.85%	1.343%
15	19.574	2797	2803	2812	rBV	1727107	2008518	100.00%	17.116%
16	19.868	2850	2853	2857	rBV4	27793	42210	2.10%	0.360%
17	20.862	3018	3022	3028	rBV	116197	153298	7.63%	1.306%
18	21.127	3063	3067	3072	rBV	441227	539586	26.86%	4.598%
19	23.274	3427	3432	3439	rVB2	313128	542647	27.02%	4.624%




Sum of corrected areas: 11734450

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031857.D
Acq On : 21 Aug 2021 00:38
Operator : CG/JU
Sample : M3434-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-11-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

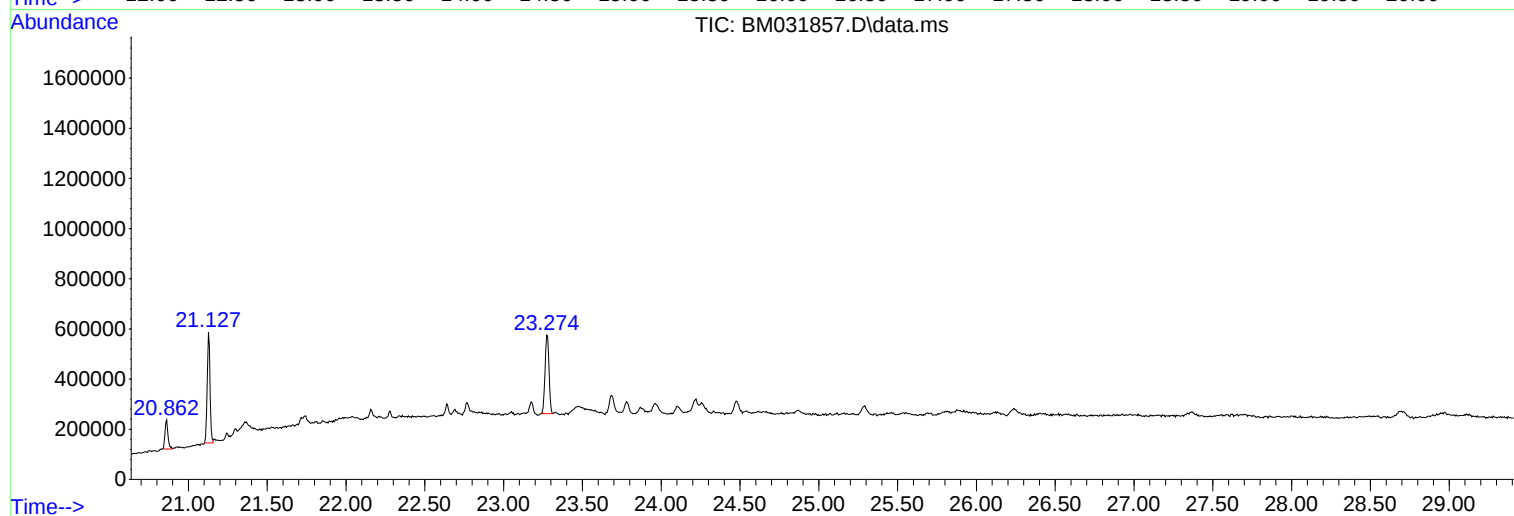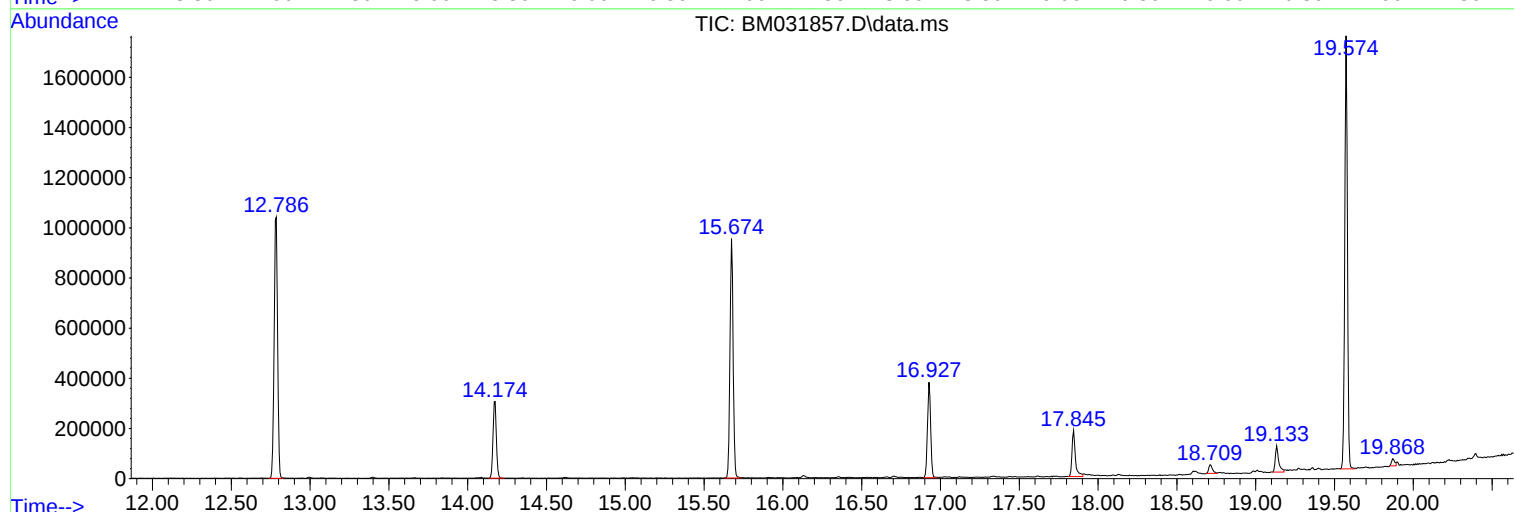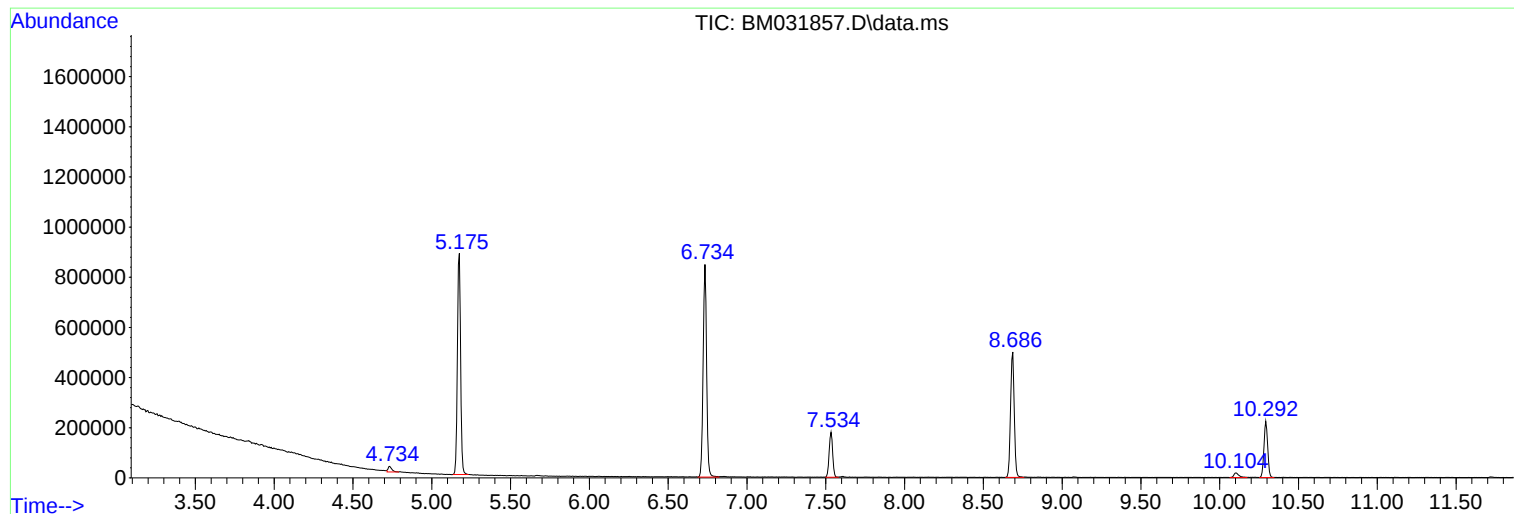

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031857.D
Acq On : 21 Aug 2021 00:38
Operator : CG/JU
Sample : M3434-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-11-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031857.D
Acq On : 21 Aug 2021 00:38
Operator : CG/JU
Sample : M3434-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-11-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc