

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031858.D
 Acq On : 21 Aug 2021 01:16
 Operator : CG/JU
 Sample : M3434-27
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-14-0205

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.734	276	280	288	rVB2	34900	53579	2.57%	0.431%
2	5.175	348	355	370	rVB	1007477	1428160	68.60%	11.499%
3	6.734	612	620	629	rBV	949241	1454549	69.87%	11.711%
4	7.534	749	756	762	rVB	169449	260748	12.53%	2.099%
5	8.687	943	952	966	rBV	566503	932492	44.79%	7.508%
6	10.098	1186	1192	1205	rBV3	16739	38974	1.87%	0.314%
7	10.293	1218	1225	1234	rBV	207693	336321	16.16%	2.708%
8	12.787	1642	1649	1659	rVB	1089773	1617359	77.69%	13.022%
9	14.169	1878	1884	1891	rBV	275694	413060	19.84%	3.326%
10	15.675	2133	2140	2156	rBV	1043059	1448351	69.57%	11.661%
11	16.927	2347	2353	2358	rBV	346052	491592	23.61%	3.958%
12	16.969	2358	2360	2365	rVB	23801	30950	1.49%	0.249%
13	17.845	2504	2509	2518	rVB2	92986	144239	6.93%	1.161%
14	17.992	2530	2534	2538	rBV5	15332	24617	1.18%	0.198%
15	18.716	2653	2657	2664	rBV6	29370	65111	3.13%	0.524%
16	18.992	2699	2704	2710	rBV	78592	131983	6.34%	1.063%
17	19.133	2724	2728	2734	rBV3	59684	99297	4.77%	0.799%
18	19.357	2763	2766	2770	rVB	69288	82791	3.98%	0.667%
19	19.574	2798	2803	2813	rVB	1792107	2081771	100.00%	16.761%
20	20.862	3018	3022	3027	rBV	149136	185969	8.93%	1.497%
21	21.127	3062	3067	3071	rBV	443585	591048	28.39%	4.759%
22	23.280	3427	3433	3439	rVB	293193	507050	24.36%	4.083%




Sum of corrected areas: 12420011

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031858.D
Acq On : 21 Aug 2021 01:16
Operator : CG/JU
Sample : M3434-27
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-14-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

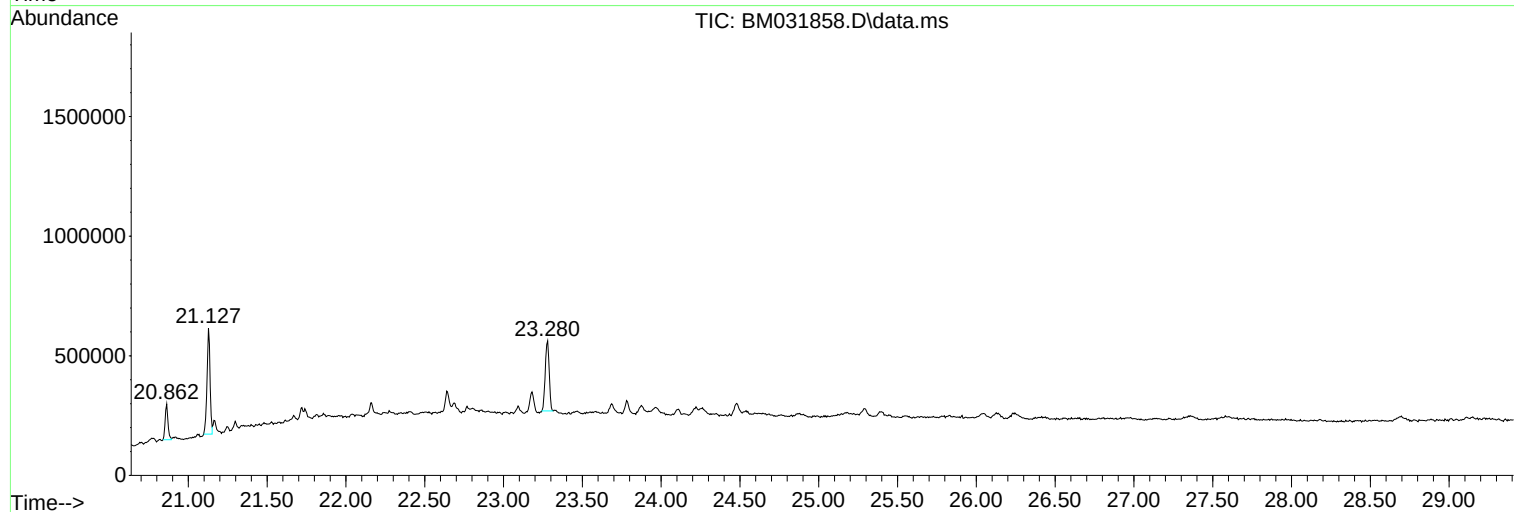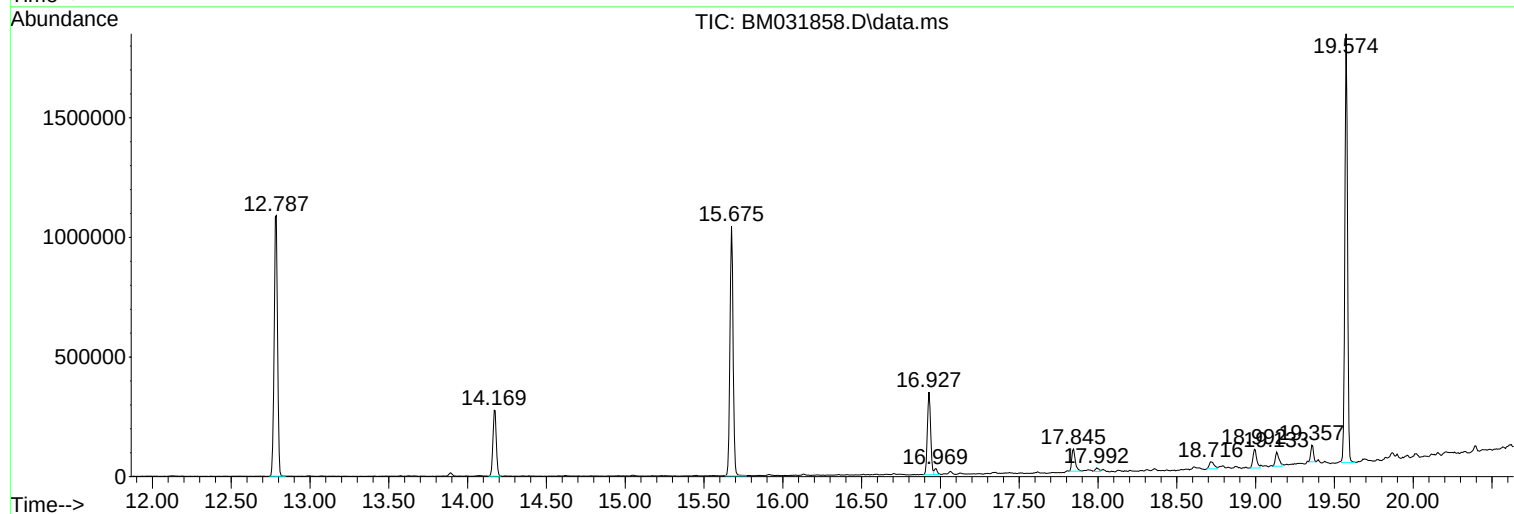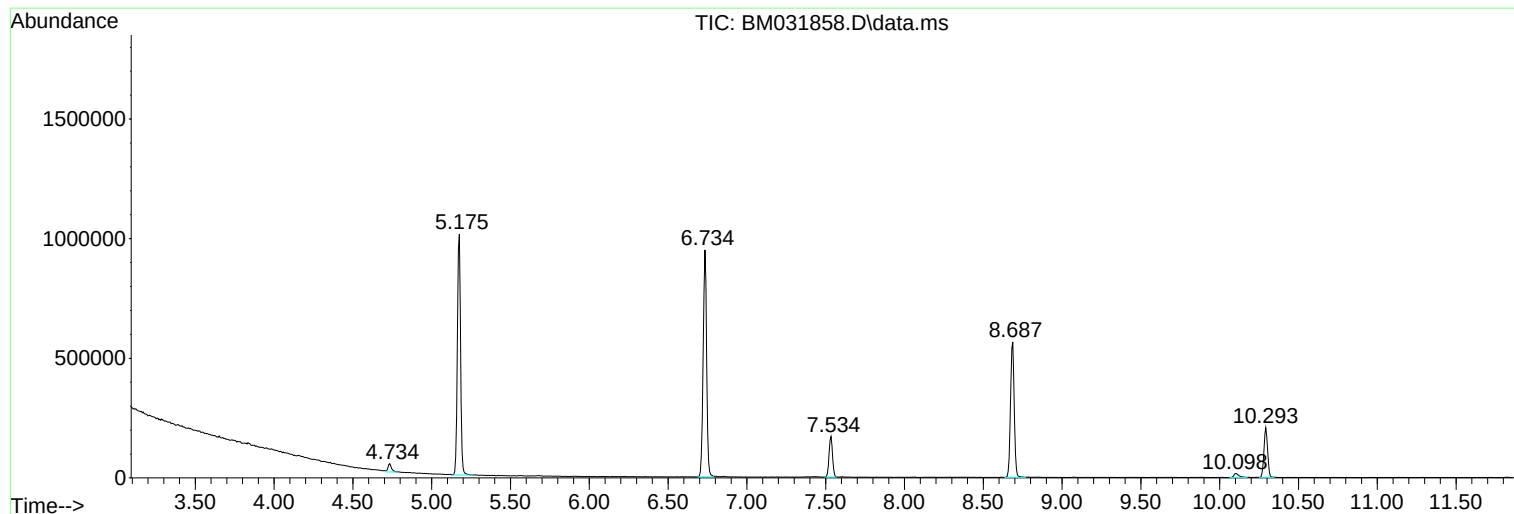

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031858.D
Acq On : 21 Aug 2021 01:16
Operator : CG/JU
Sample : M3434-27
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-14-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031858.D
Acq On : 21 Aug 2021 01:16
Operator : CG/JU
Sample : M3434-27
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-14-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
