

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031860.D
 Acq On : 21 Aug 2021 02:30
 Operator : CG/JU
 Sample : M3435-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-17-0003

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031860.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.834	124	127	137	rVB2	104716	161151	2.10%	0.213%
2	4.334	207	212	220	rVB	217383	314161	4.09%	0.415%
3	5.175	348	355	360	rBV	886711	1286448	16.74%	1.700%
4	5.228	360	364	380	rVB	72720	195341	2.54%	0.258%
5	5.581	417	424	431	rVB	246109	352108	4.58%	0.465%
6	5.828	458	466	474	rBV4	68586	166298	2.16%	0.220%
7	5.946	479	486	493	rVB2	62468	122230	1.59%	0.162%
8	6.034	496	501	509	rBV4	95303	185285	2.41%	0.245%
9	6.104	509	513	518	rBV	135128	190745	2.48%	0.252%
10	6.187	523	527	530	rBV3	64730	103275	1.34%	0.137%
11	6.534	582	586	591	rVB2	113388	164610	2.14%	0.218%
12	6.587	591	595	599	rBV	67608	90289	1.17%	0.119%
13	6.634	599	603	606	rVV	113822	156401	2.04%	0.207%
14	6.693	606	613	616	rVV4	140107	292337	3.80%	0.386%
15	6.734	616	620	631	rVB	836622	1409556	18.34%	1.863%
16	6.922	646	652	660	rBV5	47458	111352	1.45%	0.147%
17	7.157	686	692	694	rBV	253953	382283	4.97%	0.505%
18	7.181	694	696	703	rVB	179192	234244	3.05%	0.310%
19	7.440	729	740	745	rBV6	49315	167148	2.17%	0.221%
20	7.504	745	751	752	rVV2	80540	125062	1.63%	0.165%
21	7.534	752	756	760	rVV	181520	285458	3.71%	0.377%
22	7.587	760	765	770	rVB5	43320	107368	1.40%	0.142%
23	7.640	770	774	781	rBV3	51737	111740	1.45%	0.148%
24	7.710	781	786	789	rVB2	70396	97813	1.27%	0.129%
25	8.063	840	846	851	rVB3	102949	193513	2.52%	0.256%
26	8.157	857	862	868	rBV3	84543	152243	1.98%	0.201%
27	8.316	884	889	897	rVB4	49391	114173	1.49%	0.151%
28	8.616	929	940	945	rBV3	81227	177583	2.31%	0.235%
29	8.687	945	952	957	rVV	550985	929874	12.10%	1.229%
30	8.740	957	961	970	rVB	130747	221685	2.88%	0.293%
31	8.857	977	981	987	rVB5	62912	131809	1.72%	0.174%
32	8.963	987	999	1002	rBV10	30081	97065	1.26%	0.128%
33	9.210	1035	1041	1047	rVB3	43642	93096	1.21%	0.123%
34	10.092	1183	1191	1198	rBV	151426	276379	3.60%	0.365%
35	10.292	1214	1225	1229	rBV2	258090	556078	7.24%	0.735%
36	10.345	1229	1234	1240	rVB	277572	482589	6.28%	0.638%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031860.D
 Acq On : 21 Aug 2021 02:30
 Operator : CG/JU
 Sample : M3435-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-17-0003

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	11.316	1393	1399	1410	rBV	97377	206622	2.69%	0.273%
38	11.722	1459	1468	1477	rBV2	97055	207117	2.69%	0.274%
39	11.963	1503	1509	1514	rVB	249939	415212	5.40%	0.549%
40	12.104	1527	1533	1541	rBV3	70325	229829	2.99%	0.304%

41	12.186	1542	1547	1556	rVB	137269	261327	3.40%	0.345%
42	12.698	1630	1634	1638	rVB	100614	133762	1.74%	0.177%
43	12.786	1643	1649	1656	rVB	1101077	1619734	21.08%	2.141%
44	12.992	1680	1684	1692	rVB2	150822	240267	3.13%	0.318%
45	13.328	1735	1741	1742	rBV	83162	117433	1.53%	0.155%

46	13.486	1763	1768	1773	rBV	107917	190623	2.48%	0.252%
47	13.539	1773	1777	1780	rVV	76070	115710	1.51%	0.153%
48	13.628	1787	1792	1794	rBV2	55634	87595	1.14%	0.116%
49	13.657	1794	1797	1802	rVB2	134261	174730	2.27%	0.231%
50	13.892	1831	1837	1847	rBV	366108	566941	7.38%	0.749%

51	14.080	1865	1869	1874	rVB	118957	160037	2.08%	0.212%
52	14.169	1878	1884	1891	rVV2	349098	606478	7.89%	0.802%
53	14.233	1891	1895	1904	rVB	303400	505732	6.58%	0.668%
54	14.392	1917	1922	1930	rVB3	46709	132382	1.72%	0.175%
55	14.486	1933	1938	1943	rBV7	40395	86883	1.13%	0.115%

56	14.580	1948	1954	1959	rVV	252340	396218	5.16%	0.524%
57	14.710	1972	1976	1978	rBV2	71360	106084	1.38%	0.140%
58	14.957	2014	2018	2024	rVB5	50708	96193	1.25%	0.127%
59	15.045	2029	2033	2038	rVB2	143199	181399	2.36%	0.240%
60	15.227	2059	2064	2070	rBV	451135	649016	8.44%	0.858%

61	15.451	2096	2102	2110	rVV5	125526	259668	3.38%	0.343%
62	15.527	2111	2115	2124	rVB2	107561	187812	2.44%	0.248%
63	15.674	2132	2140	2147	rVV	1095712	1615052	21.01%	2.135%
64	15.745	2149	2152	2162	rVB8	46652	108412	1.41%	0.143%
65	15.910	2176	2180	2189	rVB4	240178	511702	6.66%	0.676%

66	16.239	2230	2236	2240	rBV2	85926	154821	2.01%	0.205%
67	16.592	2292	2296	2302	rVB2	124891	197058	2.56%	0.260%
68	16.663	2305	2308	2312	rVV3	66645	137424	1.79%	0.182%
69	16.704	2312	2315	2318	rVV	142072	198941	2.59%	0.263%
70	16.751	2318	2323	2332	rVB2	309100	524663	6.83%	0.694%

71	16.933	2349	2354	2357	rBV	364980	588559	7.66%	0.778%
72	16.980	2357	2362	2367	rVB	3626321	4830250	62.85%	6.385%
73	17.063	2372	2376	2382	rVB	1002668	1416727	18.43%	1.873%
74	17.127	2382	2387	2392	rBV	175054	297740	3.87%	0.394%
75	17.345	2420	2424	2432	rVB	329612	481730	6.27%	0.637%

76	17.445	2438	2441	2446	rVV2	137380	177028	2.30%	0.234%
----	--------	------	------	------	------	--------	--------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031860.D
 Acq On : 21 Aug 2021 02:30
 Operator : CG/JU
 Sample : M3435-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SWCS-17-0003

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	17.510	2449	2452	2461	rVB3	132018	229125	2.98%	0.303%
78	17.804	2498	2502	2506	rBV	382578	562116	7.31%	0.743%
79	17.857	2506	2511	2518	rVV	1095266	1513780	19.70%	2.001%
80	17.939	2522	2525	2530	rVV	200672	342665	4.46%	0.453%
81	17.998	2530	2535	2539	rVV2	776713	1375923	17.90%	1.819%
82	18.039	2539	2542	2548	rVB	314619	433899	5.65%	0.574%
83	18.315	2585	2589	2593	rBV	335821	440701	5.73%	0.583%
84	18.363	2593	2597	2601	rVB	328202	442228	5.75%	0.585%
85	18.739	2658	2661	2666	rBV	255177	376815	4.90%	0.498%
86	19.015	2702	2708	2712	rBV	5578673	7391643	96.18%	9.771%
87	19.145	2727	2730	2736	rBV2	452828	693903	9.03%	0.917%
88	19.374	2759	2769	2777	rBV	4433476	7685425	100.00%	10.159%
89	19.445	2778	2781	2787	rVB3	300727	476291	6.20%	0.630%
90	19.580	2800	2804	2808	rVB	1599458	1840962	23.95%	2.433%
91	19.868	2850	2853	2857	rVB	863869	1150965	14.98%	1.521%
92	19.968	2867	2870	2874	rVB	706018	803851	10.46%	1.063%
93	20.627	2979	2982	2987	rVB2	630121	758164	9.86%	1.002%
94	20.868	3020	3023	3029	rVB4	1151175	1387086	18.05%	1.833%
95	21.068	3054	3057	3060	rVB	612506	598384	7.79%	0.791%
96	21.127	3063	3067	3072	rVV2	2799875	4897613	63.73%	6.474%
97	21.180	3073	3076	3084	rVB	2887116	3602736	46.88%	4.762%
98	22.668	3324	3329	3333	rBV2	1821172	4125252	53.68%	5.453%
99	23.127	3402	3407	3412	rVB	1074296	1830809	23.82%	2.420%
100	23.215	3417	3422	3427	rVB	1902069	3278524	42.66%	4.334%




Sum of corrected areas: 75652561

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031860.D
Acq On : 21 Aug 2021 02:30
Operator : CG/JU
Sample : M3435-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-17-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

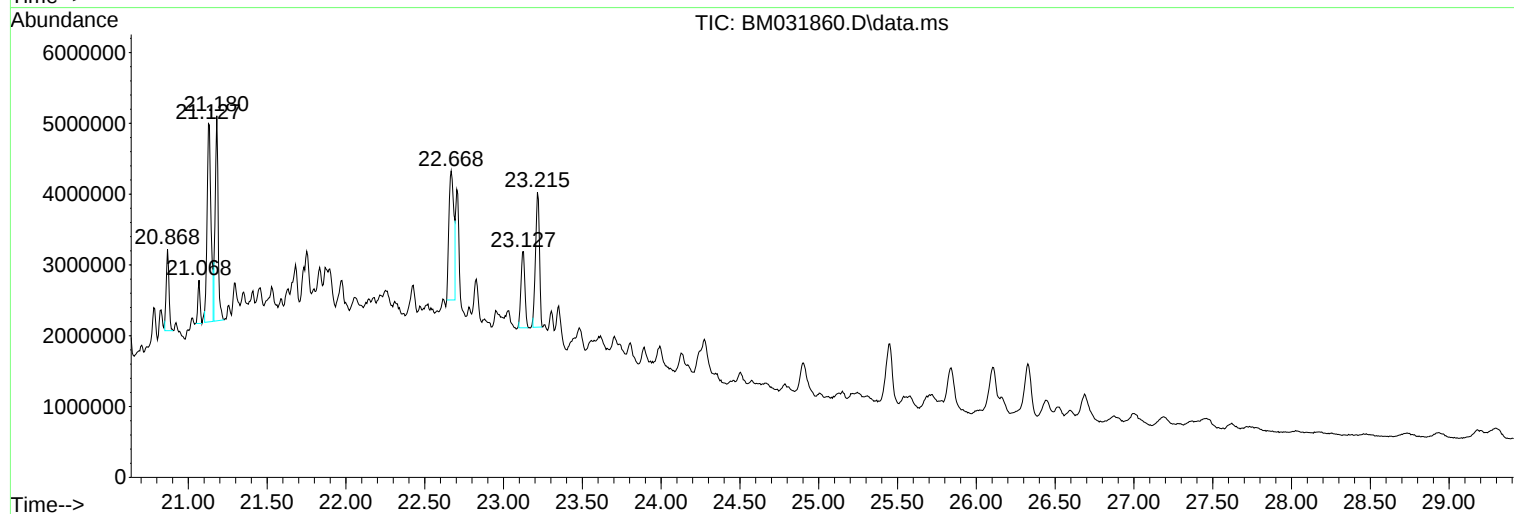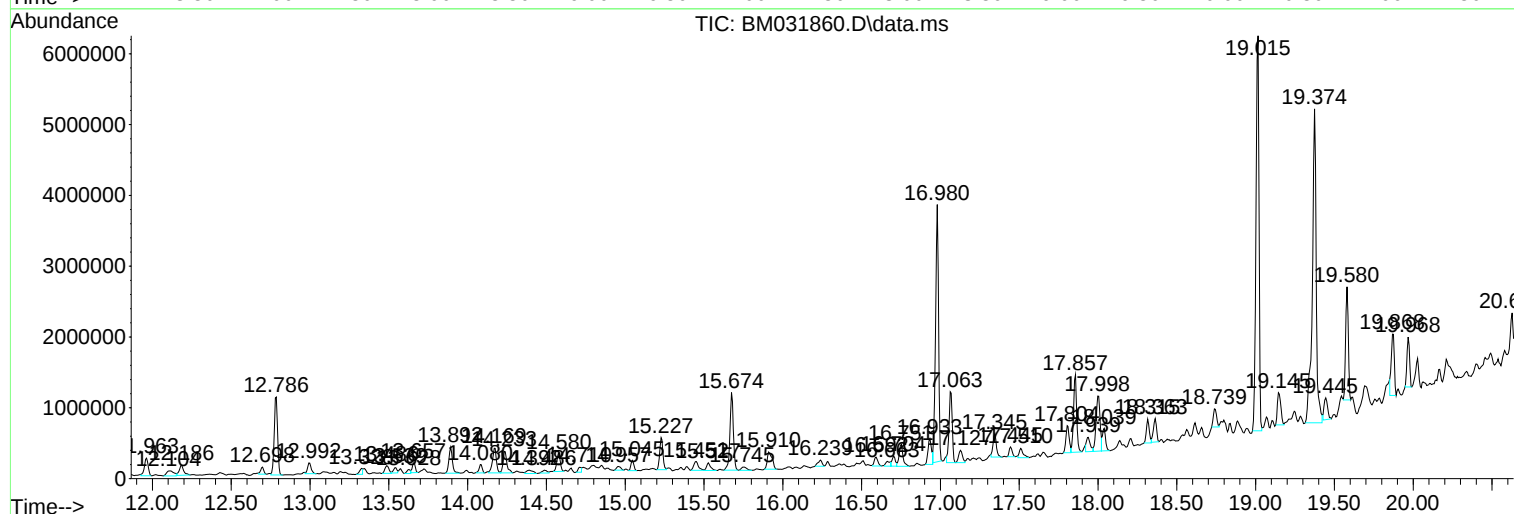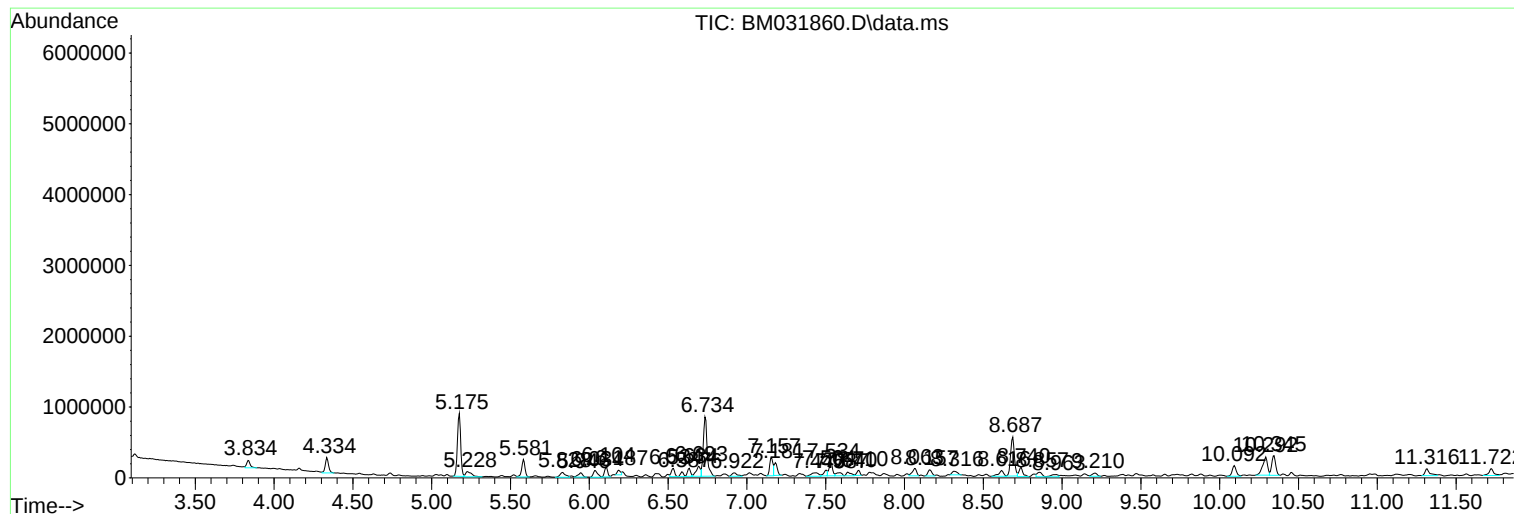

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031860.D
Acq On : 21 Aug 2021 02:30
Operator : CG/JU
Sample : M3435-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-17-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031860.D
Acq On : 21 Aug 2021 02:30
Operator : CG/JU
Sample : M3435-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SWCS-17-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------