


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031833.D
 Acq On : 20 Aug 2021 08:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 18 14:13:35 2021

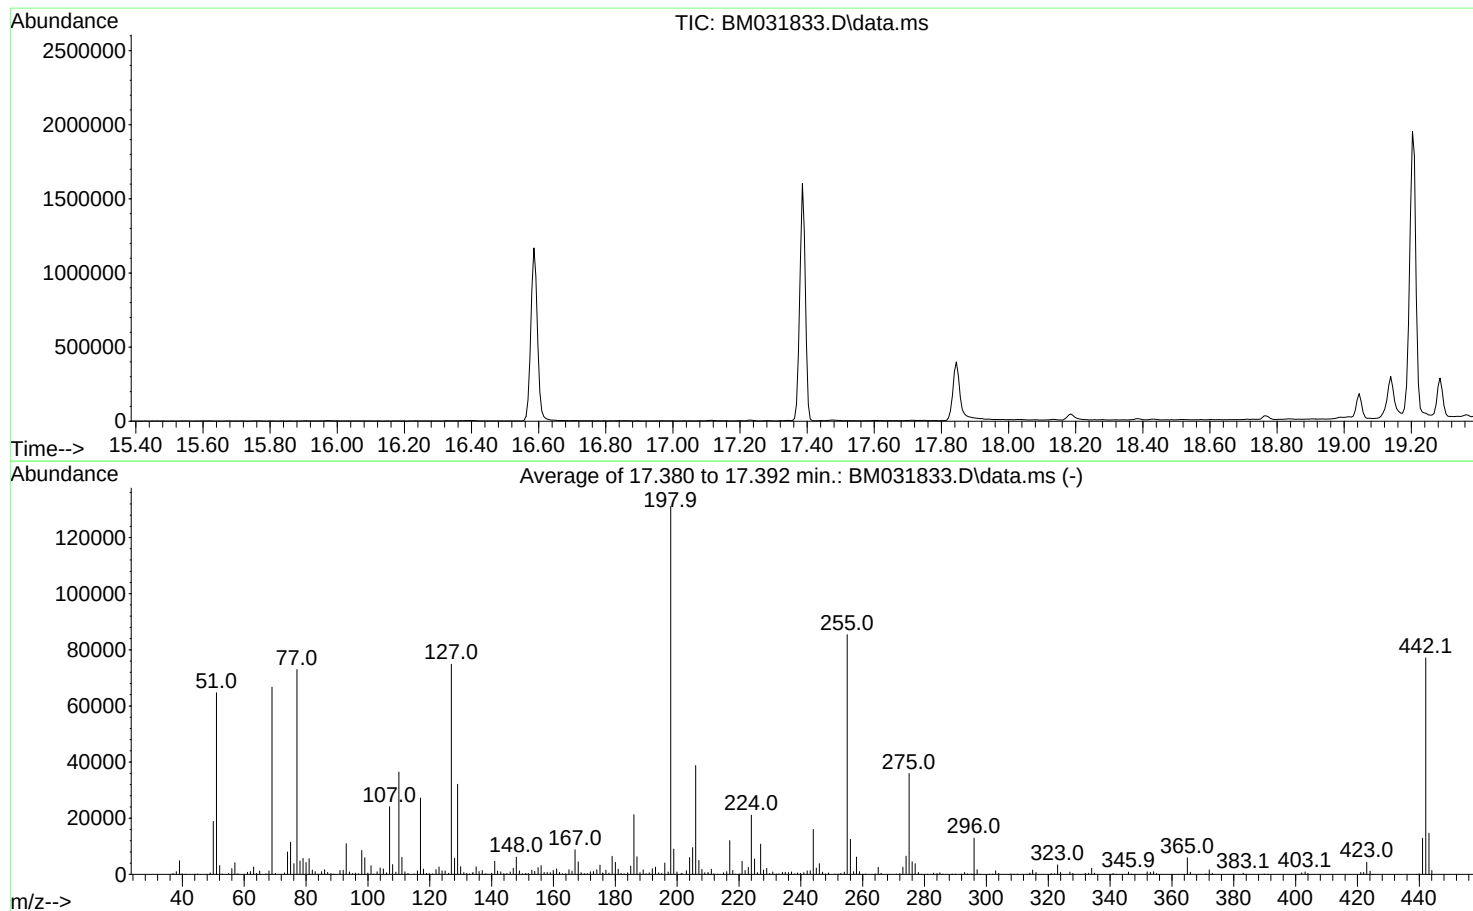




AutoFind: Scans 2430, 2431, 2432; Background Corrected with Scan 2423

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.4	64731	PASS
68	69	0.00	2	1.8	1218	PASS
69	198	0.00	100	50.9	66707	PASS
70	69	0.00	2	0.5	325	PASS
127	198	10	80	57.1	74843	PASS
197	198	0.00	2	0.7	864	PASS
198	198	100	100	100.0	131064	PASS
199	198	5	9	6.9	8989	PASS
275	198	10	60	27.4	35901	PASS
365	198	1	100	4.5	5948	PASS
441	198	0.01	100	9.8	12895	PASS
442	442	50	100	100.0	77131	PASS
443	442	15	24	19.0	14645	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\  
Data File : BM031833.D  
Acq On    : 20 Aug 2021   08:52  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 20 11:05:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 18 14:13:35 2021
Response via : Initial Calibration

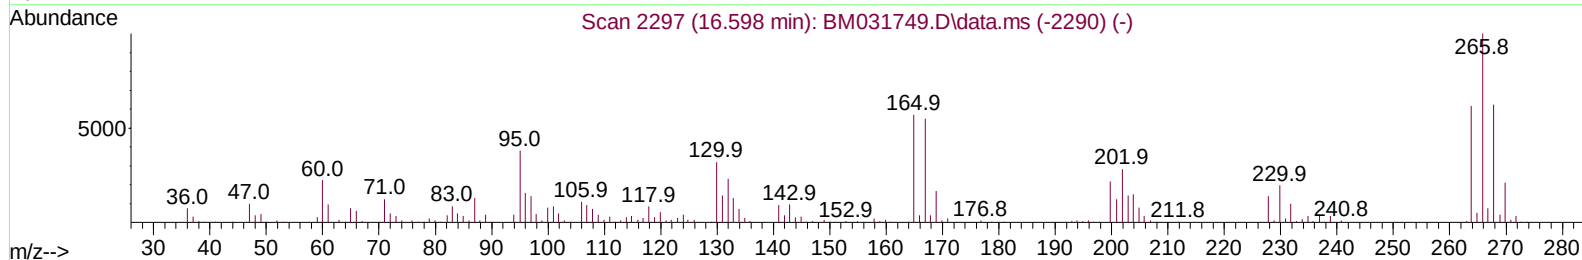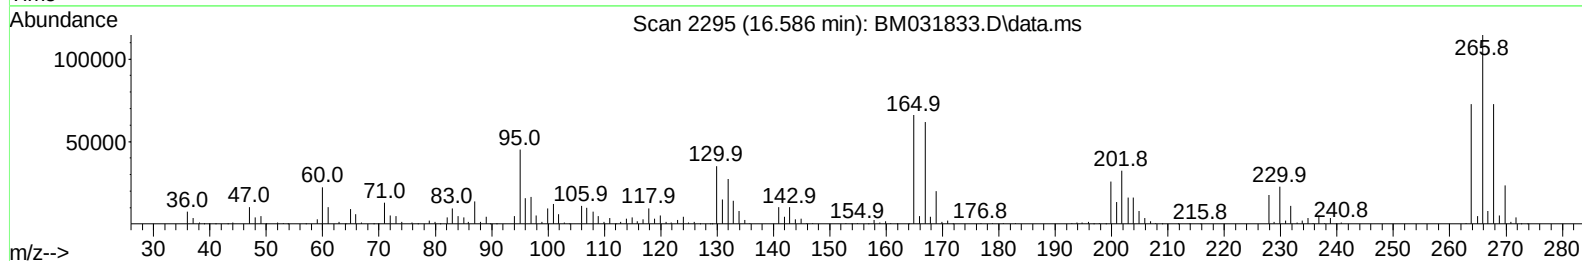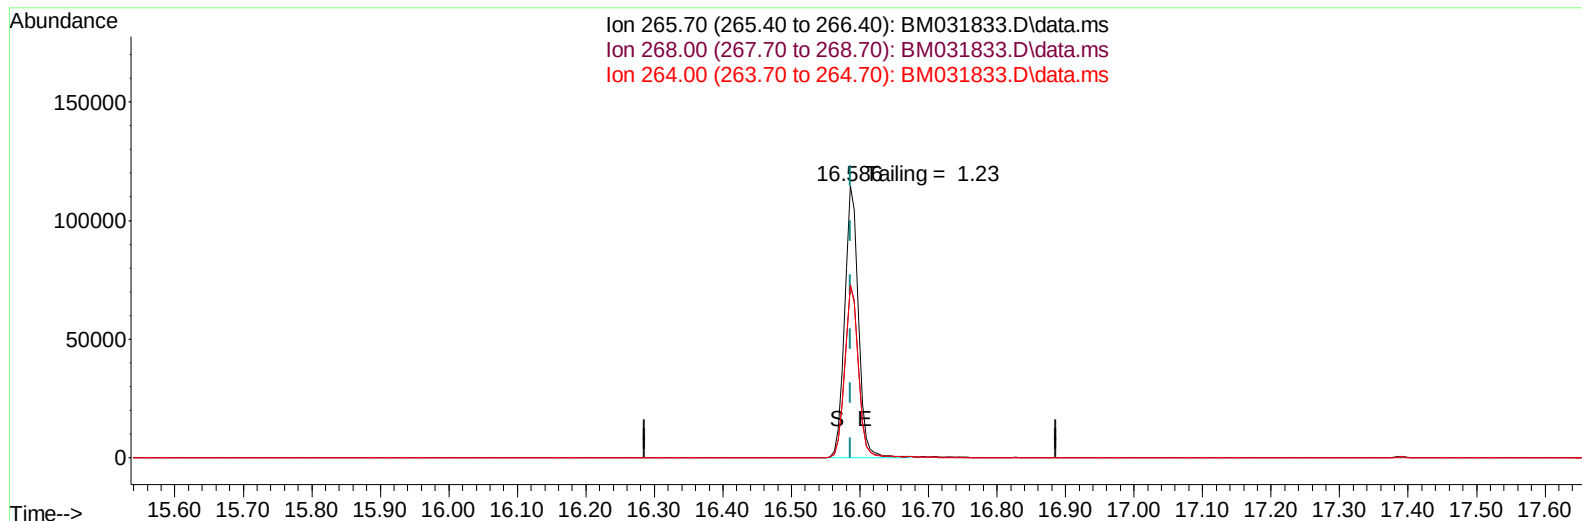

TIC: BM031833.D\data.ms

(70) Pentachlorophenol (C)

16.586min (-0.000) 175864.21 ng




response **158174**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	63.53
264.00	64.90	63.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031833.D
 Acq On : 20 Aug 2021 08:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 20 11:05:31 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 18 14:13:35 2021
 Response via : Initial Calibration

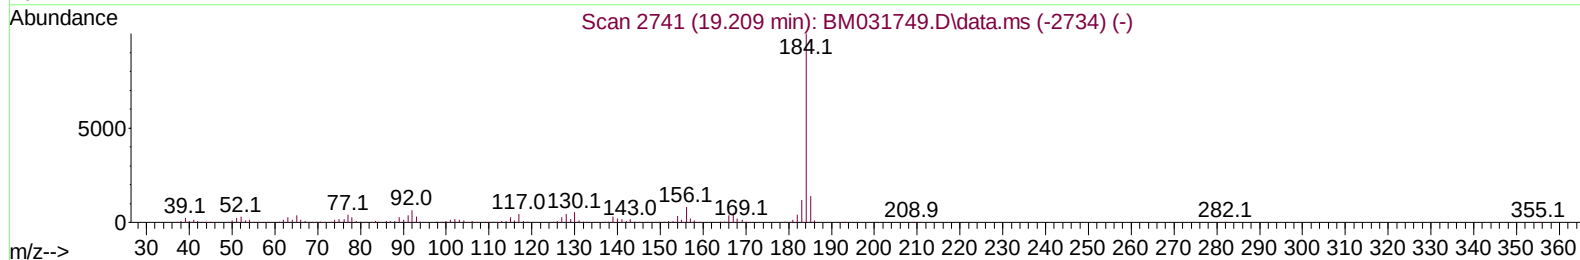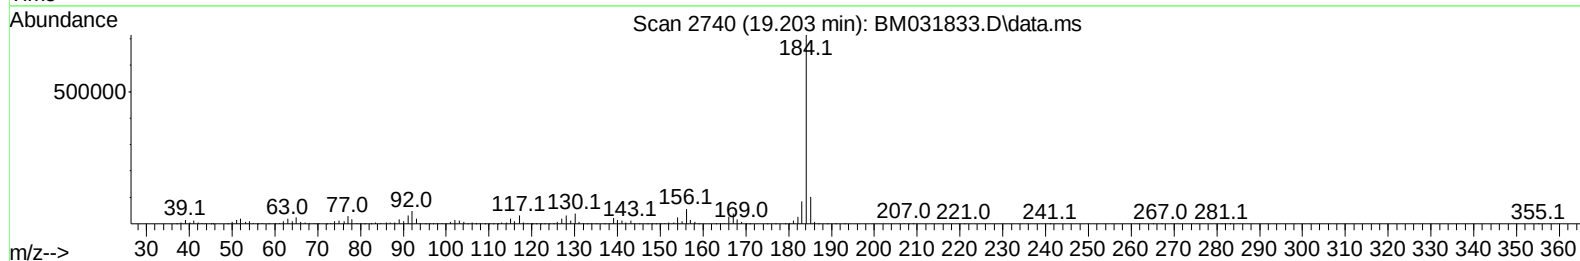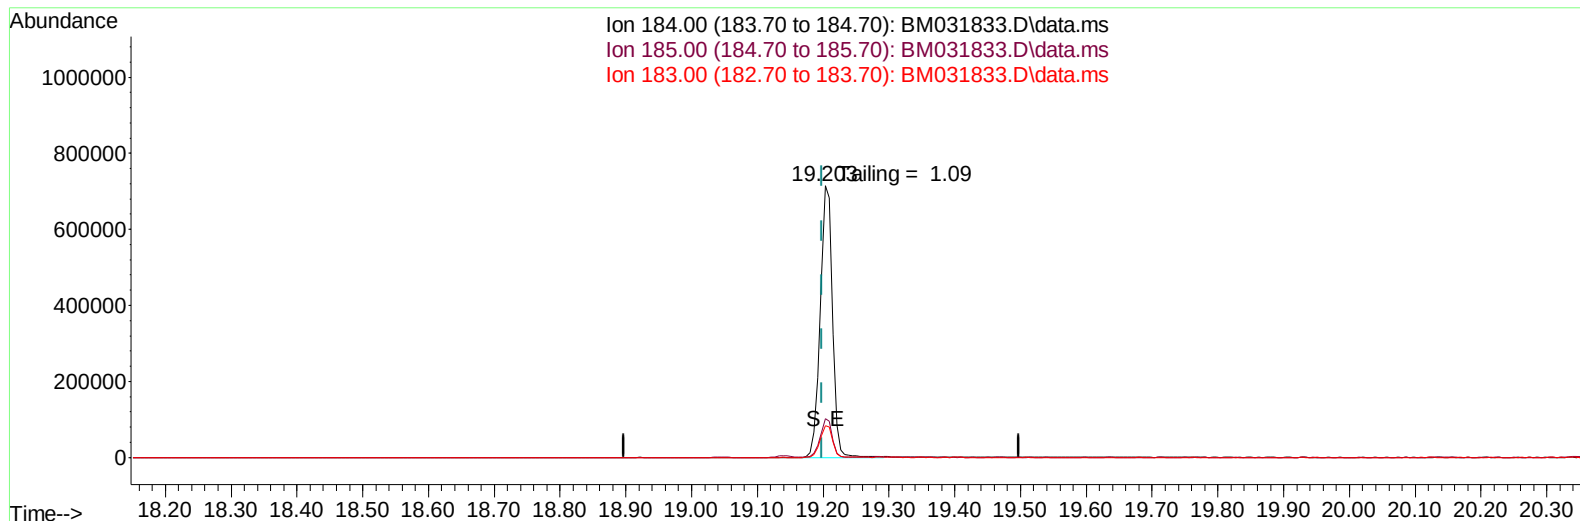

TIC: BM031833.D\data.ms

(77) Benzidine

19.203min (+ 0.006) 215966.00 ng

response 937011

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.30
183.00	12.30	11.80
0.00	0.00	0.00

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/20/2021	BNA_M	<u>BM031833.D</u>
Compound Name	Response	Retention Time
DDT	502369	20.43
DDD	2396	19.99
DDE	700	19.48
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3096	505465	0.61