
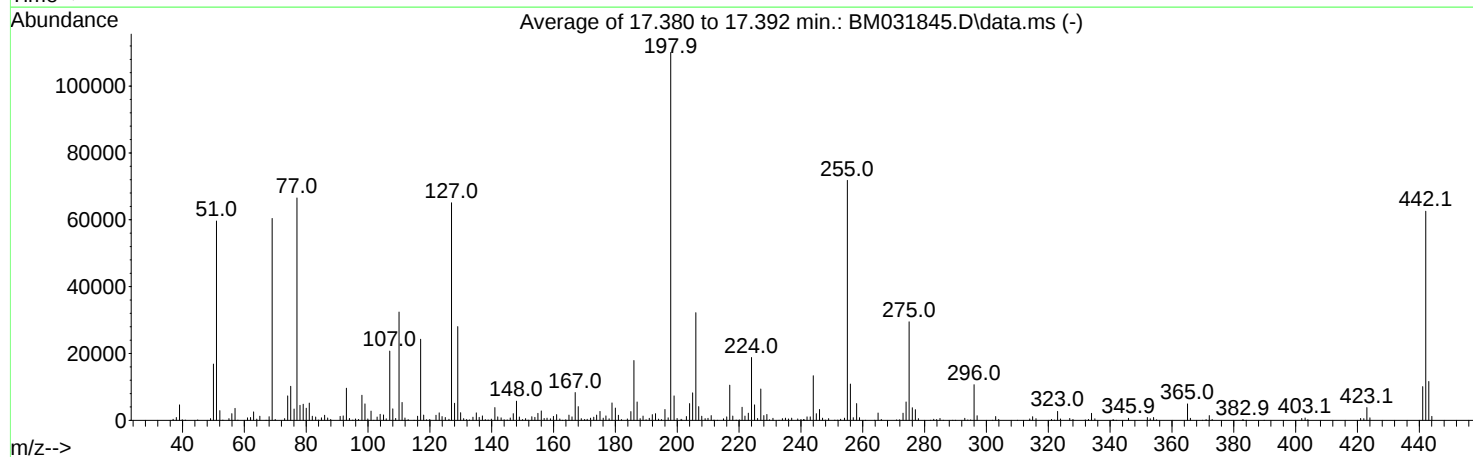


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
 Data File : BM031845.D
 Acq On : 20 Aug 2021 17:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 18 14:13:35 2021

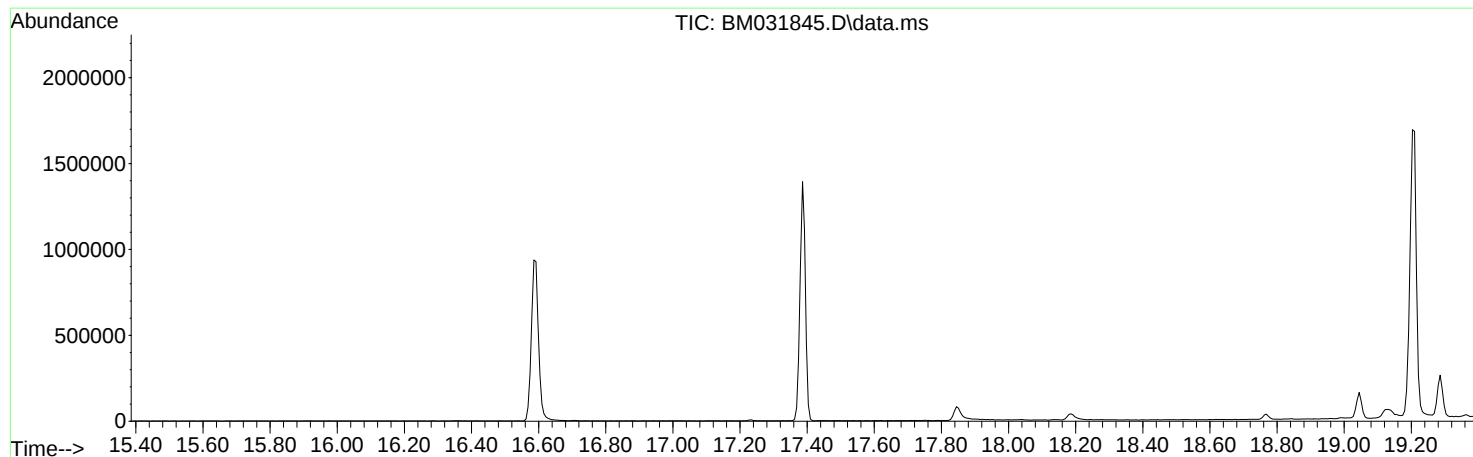




AutoFind: Scans 2430, 2431, 2432; Background Corrected with Scan 2424

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.2	59645	PASS
68	69	0.00	2	1.8	1084	PASS
69	198	0.00	100	54.9	60411	PASS
70	69	0.00	2	0.5	310	PASS
127	198	10	80	59.1	65083	PASS
197	198	0.00	2	0.7	778	PASS
198	198	100	100	100.0	110043	PASS
199	198	5	9	6.7	7322	PASS
275	198	10	60	26.8	29472	PASS
365	198	1	100	4.5	4928	PASS
441	198	0.01	100	9.2	10116	PASS
442	442	50	100	100.0	62576	PASS
443	442	15	24	18.6	11630	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082021\
Data File : BM031845.D
Acq On : 20 Aug 2021 17:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 21 08:08:02 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 18 14:13:35 2021
Response via : Initial Calibration

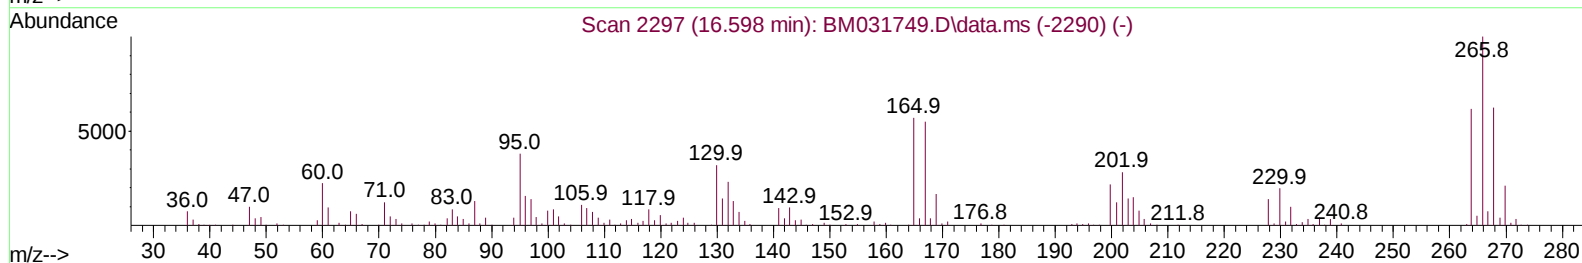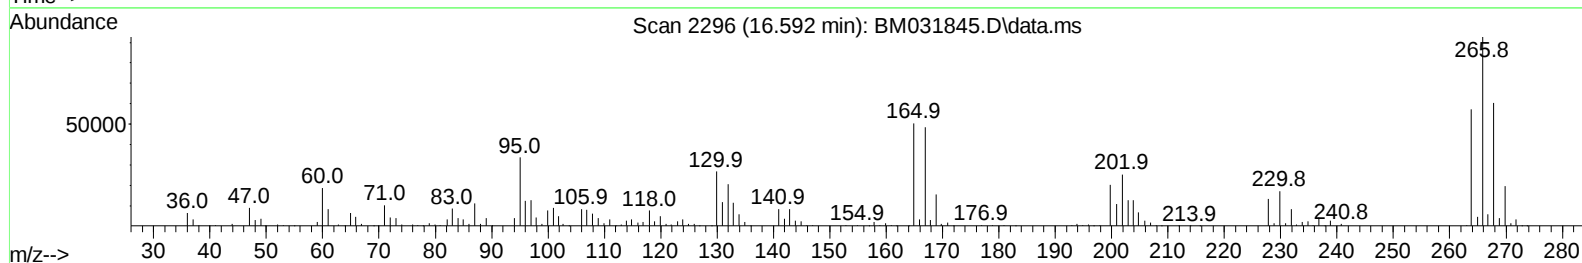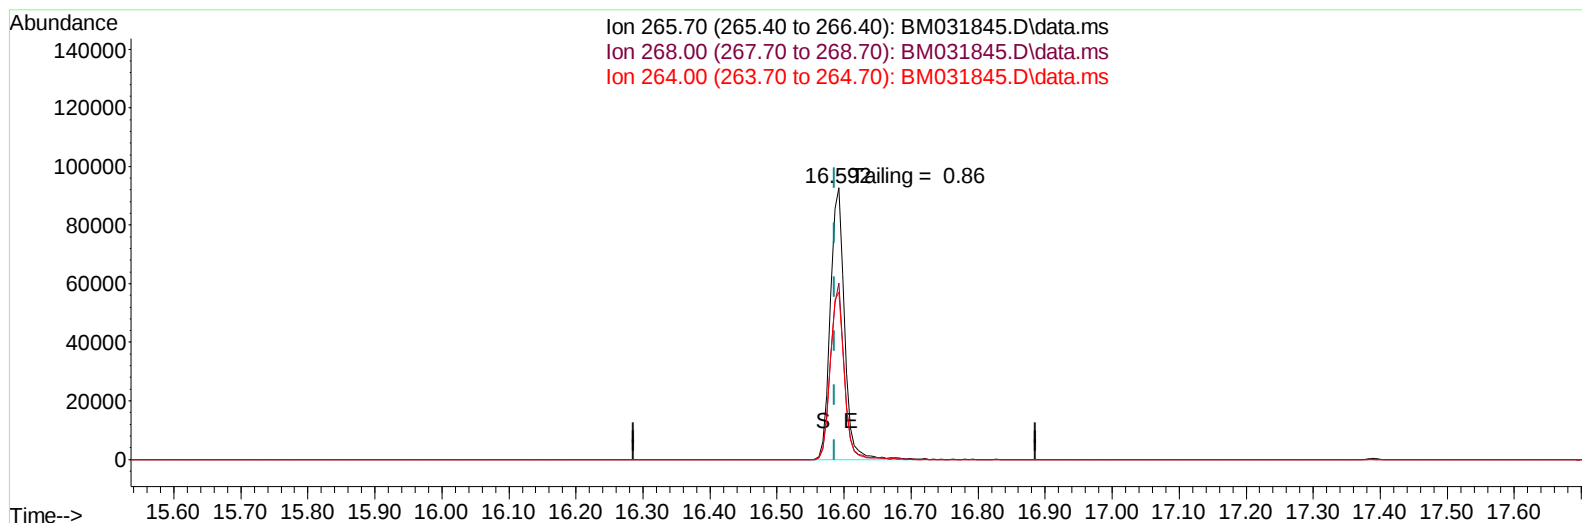

TIC: BM031845.D\data.ms

(70) Pentachlorophenol (C)




16.592min (+ 0.006) 0.00 ng

response 135237

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	65.02
264.00	64.90	61.65
0.00	0.00	0.00

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 21 08:08:02 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 18 14:13:35 2021
Response via : Initial Calibration

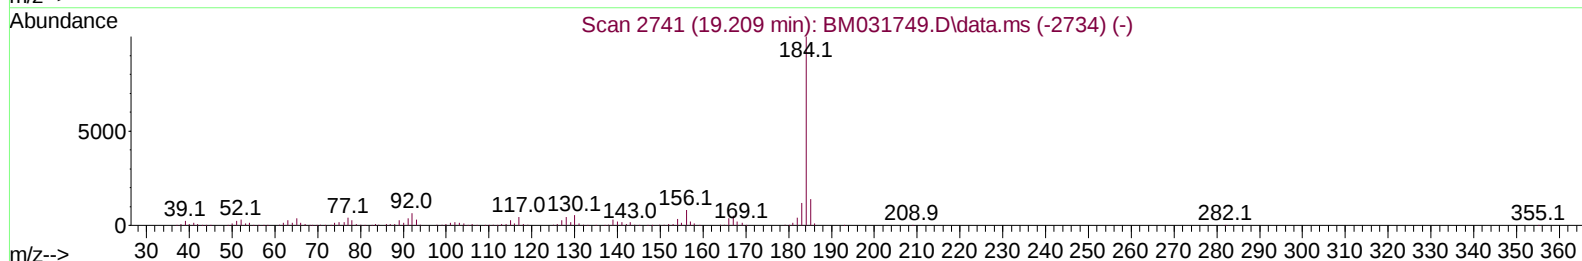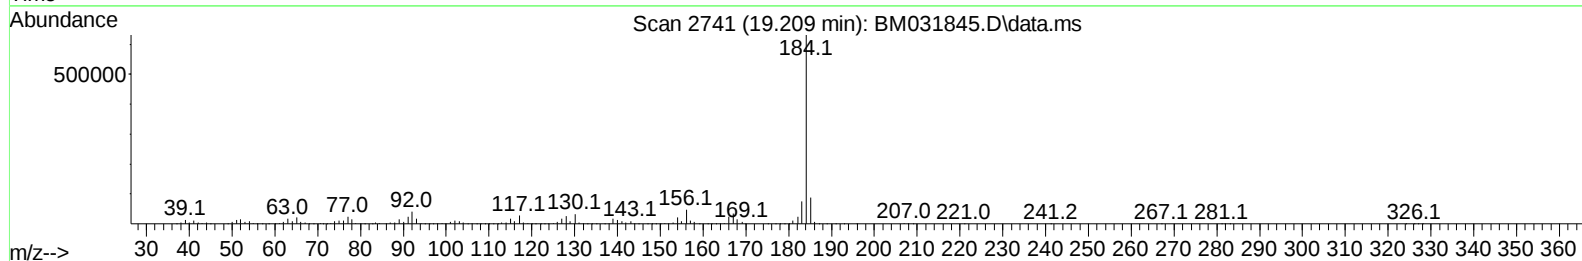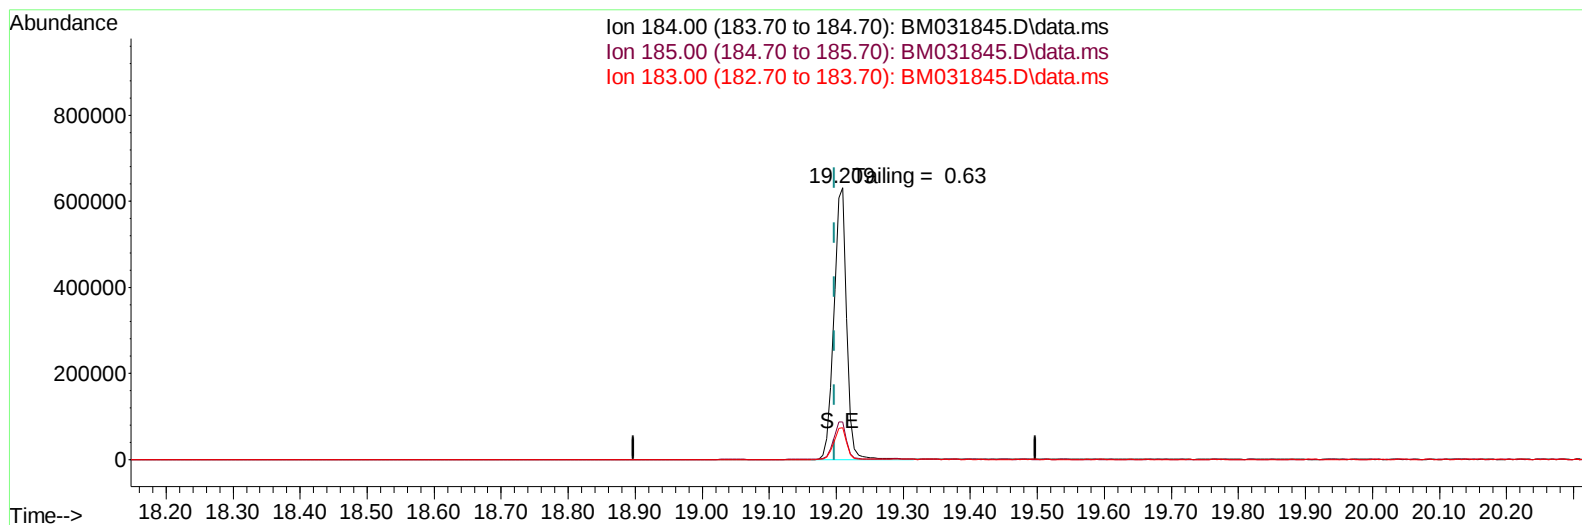

TIC: BM031845.D\data.ms

(77) **Benzidine**

19.209min (+ 0.012) 85280.31 ng

response **831245**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.91
183.00	12.30	11.81
0.00	0.00	0.00

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/20/2021	BNA_M	<u>BM031845.D</u>
Compound Name	Response	Retention Time
DDT	425570	20.439
DDD	5941	19.998
DDE	550	19.48
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6491	432061	1.50