

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082024\
 Data File : BM047269.D
 Acq On : 20 Aug 2024 13:27
 Operator : RC/JU
 Sample : P3643-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 932-K1-SD-0.5-1-081524

Quant Time: Aug 20 14:07:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Aug 11 23:47:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.357	152	216646	20.000	ng	-0.02
21) Naphthalene-d8	10.116	136	806956	20.000	ng	-0.02
39) Acenaphthene-d10	14.022	164	551285	20.000	ng	-0.01
64) Phenanthrene-d10	16.786	188	1228370	20.000	ng	0.00
76) Chrysene-d12	21.027	240	1198327	20.000	ng	0.00
86) Perylene-d12	23.721	264	1157106	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.016	112	1615214	133.219	ng	0.00
7) Phenol-d6	6.575	99	2128647	127.414	ng	-0.01
23) Nitrobenzene-d5	8.504	82	1360099	84.869	ng	-0.02
42) 2,4,6-Tribromophenol	15.533	330	1008213	157.725	ng	0.00
45) 2-Fluorobiphenyl	12.628	172	3030576	84.797	ng	-0.02
79) Terphenyl-d14	19.457	244	5253111	93.932	ng	0.00
Target Compounds						
9) Benzaldehyde	6.522	77	462	Below Cal	Qvalue #	48

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082024\
Data File : BM047269.D
Acq On : 20 Aug 2024 13:27
Operator : RC/JU
Sample : P3643-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
932-K1-SD-0.5-1-081524


Quant Time: Aug 20 14:07:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

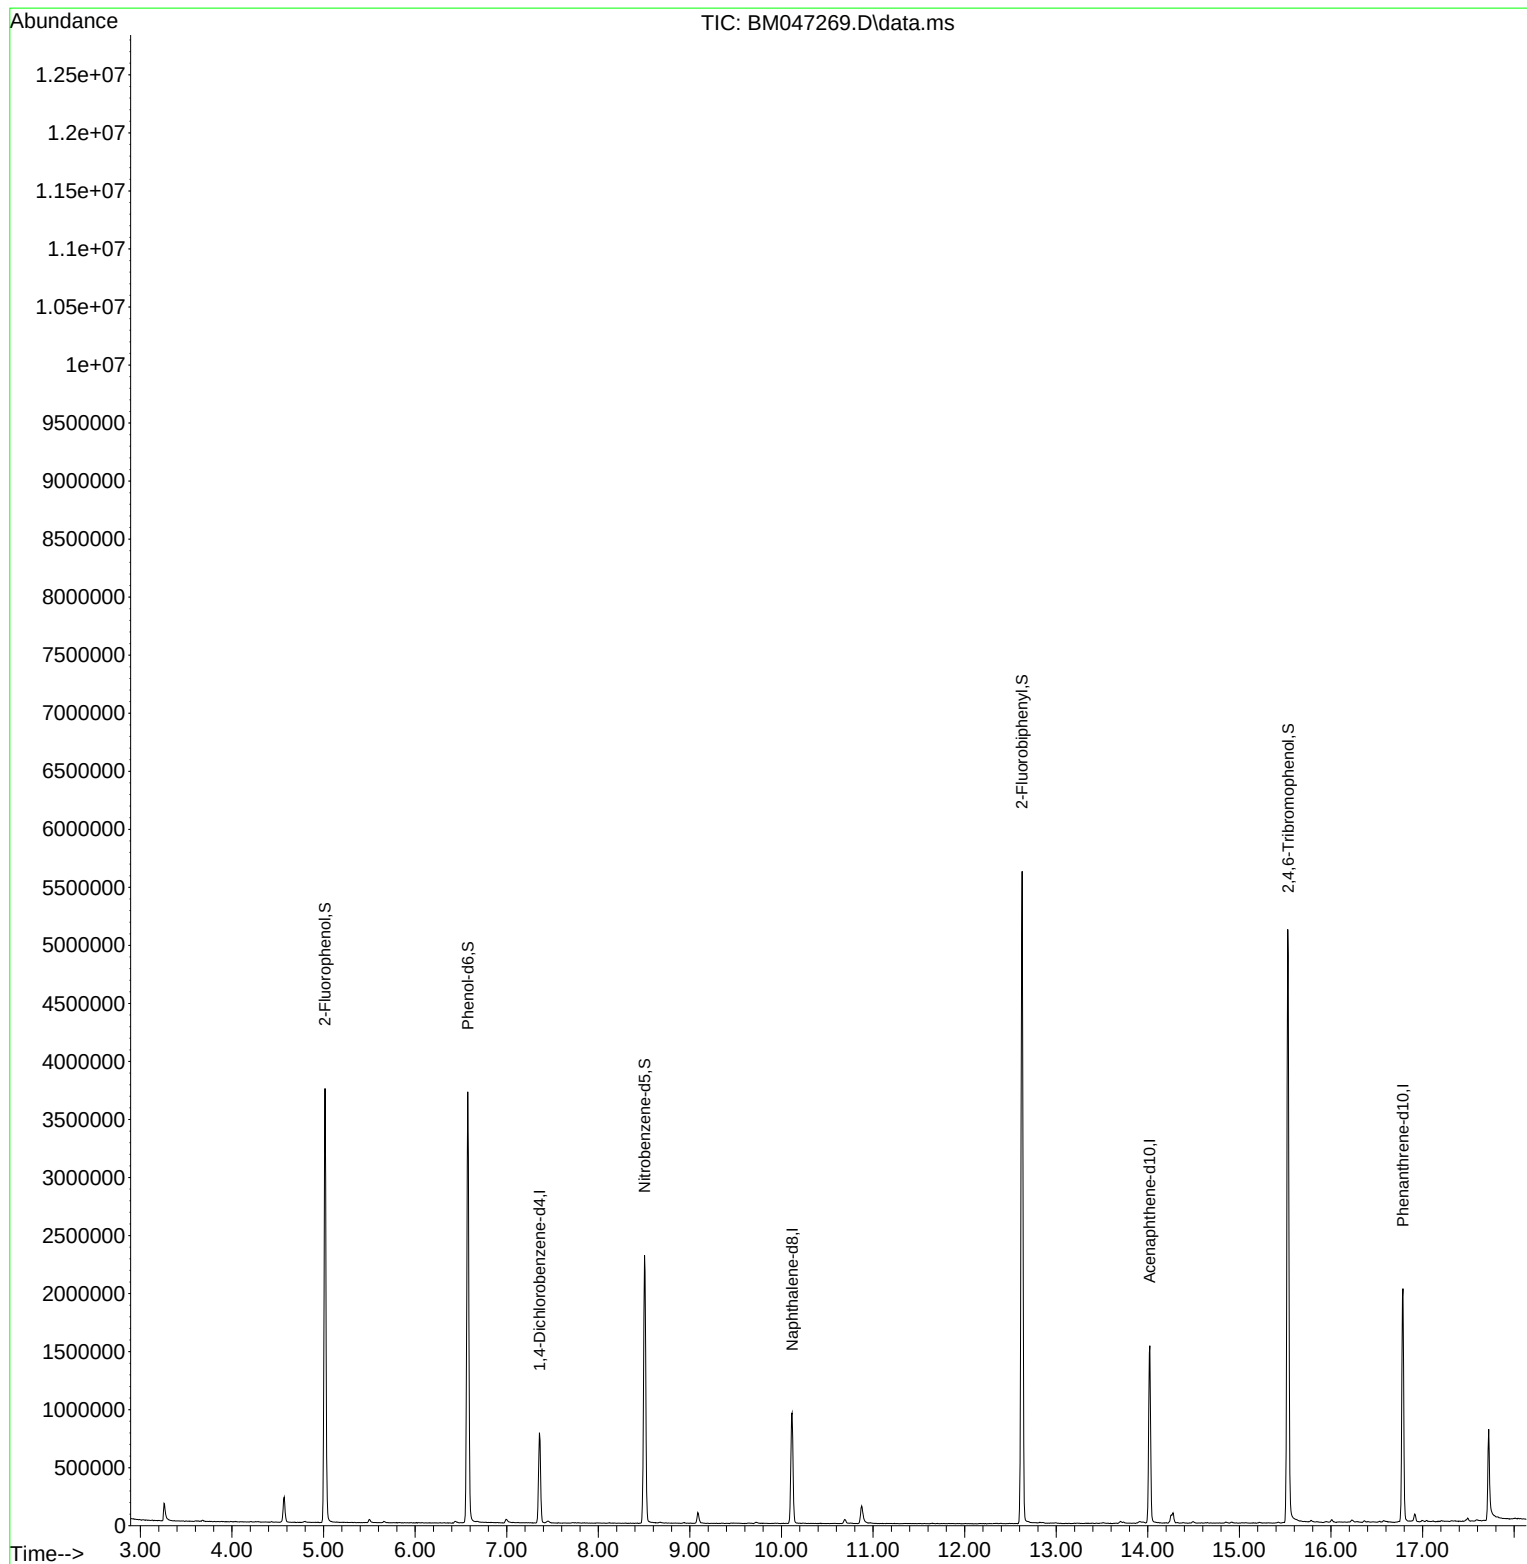


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082024\
Data File : BM047269.D
Acq On : 20 Aug 2024 13:27
Operator : RC/JU
Sample : P3643-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
932-K1-SD-0.5-1-081524

Quant Time: Aug 20 14:07:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration




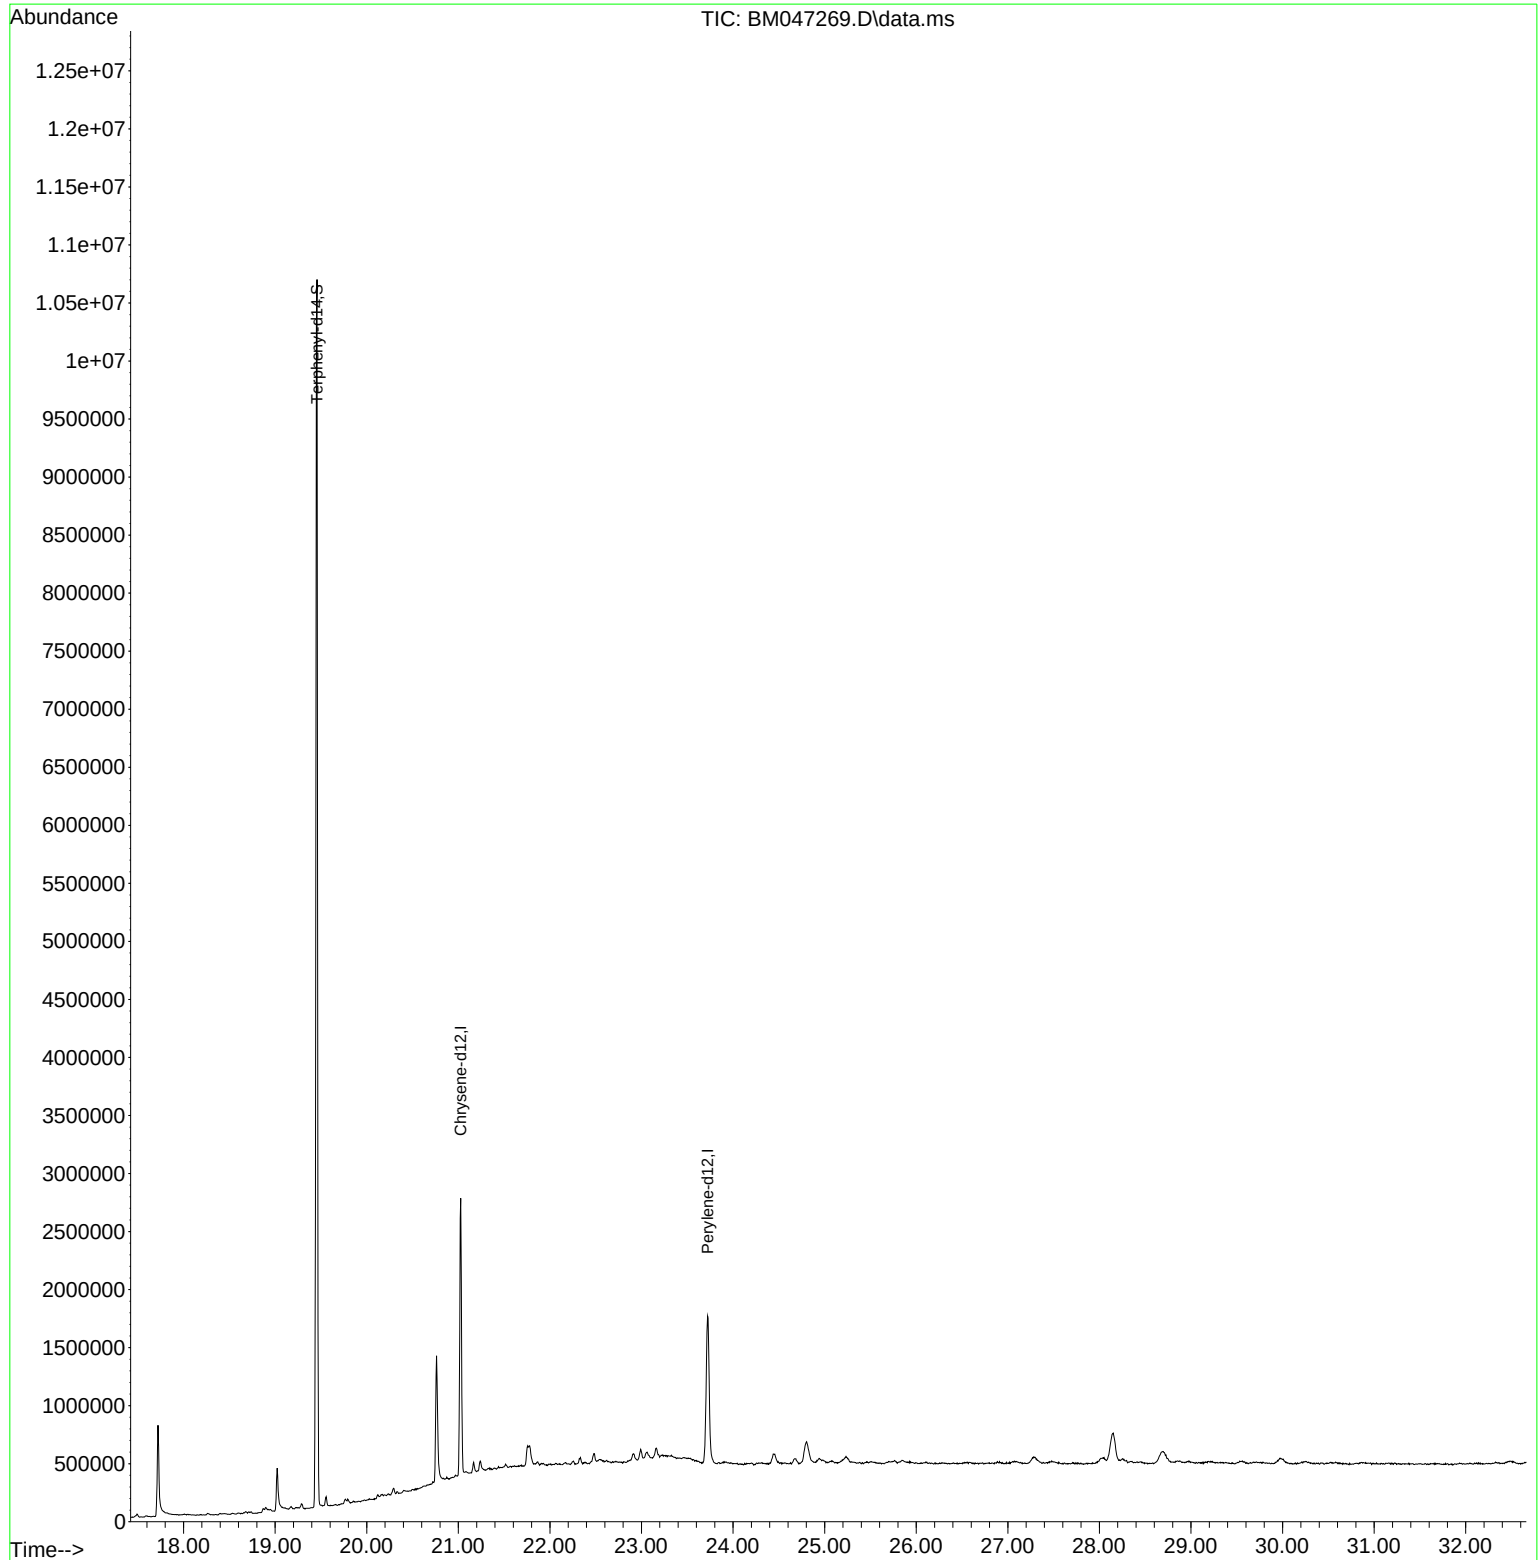


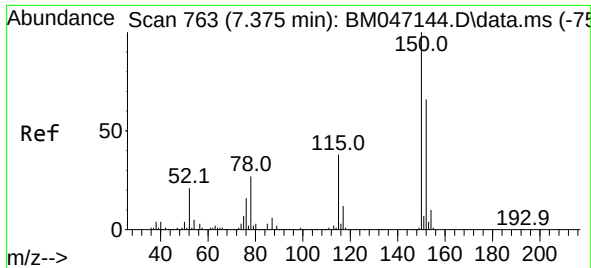

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.357 min Scan# 70
Delta R.T. -0.018 min
Lab File: BM047269.D
Acq: 20 Aug 2024 13:27




Instrument :
BNA_M
ClientSampleId :
932-K1-SD-0.5-1-081524


Tgt Ion:152 Resp: 216646
Ion Ratio Lower Upper
152 100
150 153.4 120.5 180.7
115 54.6 45.5 68.3

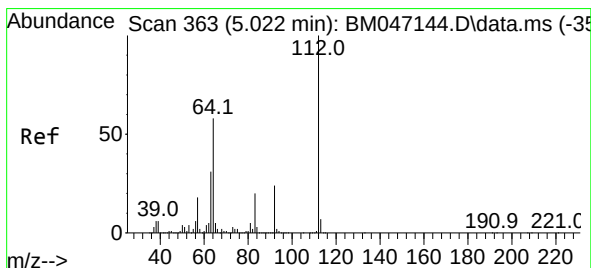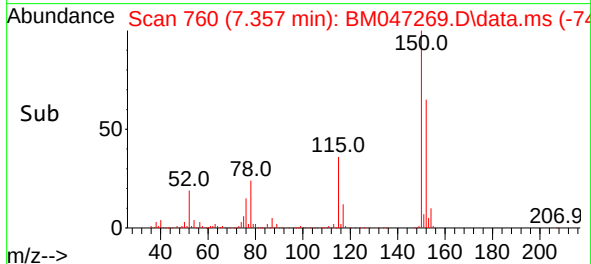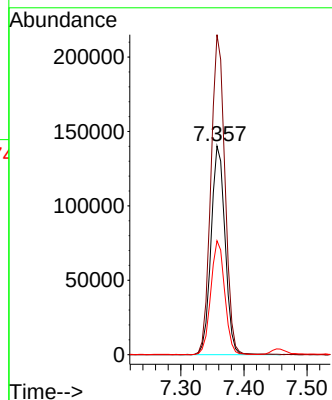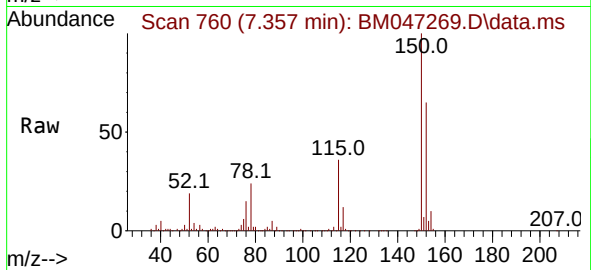

#5
2-Fluorophenol
Concen: 133.219 ng
RT: 5.016 min Scan# 362
Delta R.T. -0.006 min
Lab File: BM047269.D
Acq: 20 Aug 2024 13:27

Tgt Ion:112 Resp: 1615214
Ion Ratio Lower Upper
112 100
64 55.6 46.7 70.1
63 29.2 24.8 37.2

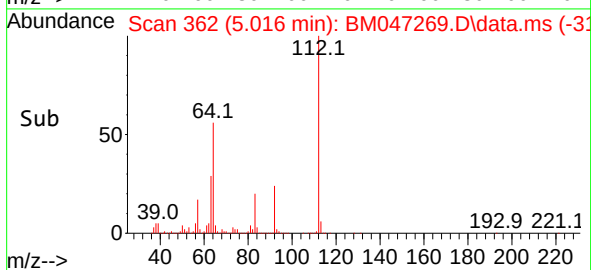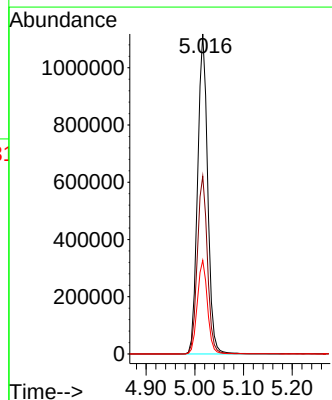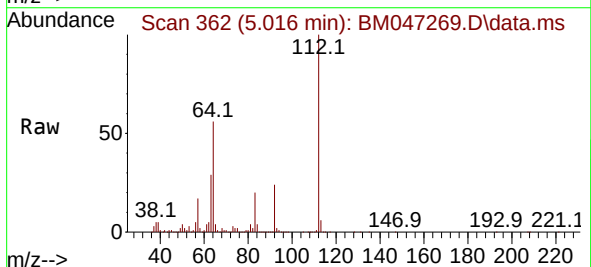




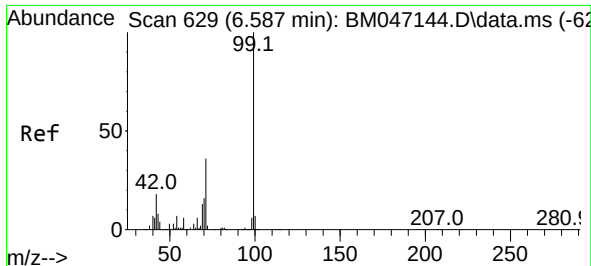


#7
Phenol-d6
Concen: 127.414 ng
RT: 6.575 min Scan# 61
Delta R.T. -0.012 min
Lab File: BM047269.D
Acq: 20 Aug 2024 13:27

Instrument :
BNA_M
ClientSampleId :
932-K1-SD-0.5-1-081524

Tgt Ion: 99 Resp: 2128647




Ion	Ratio	Lower	Upper
99	100		
42	16.4	14.1	21.1
71	35.0	28.5	42.7

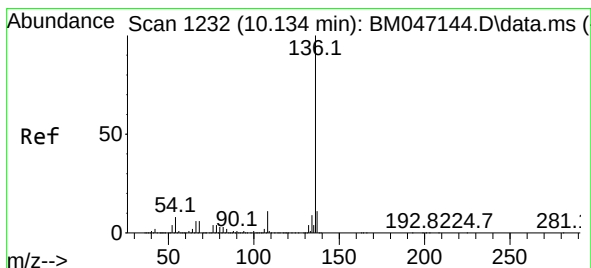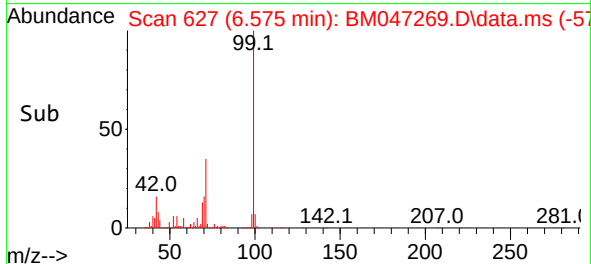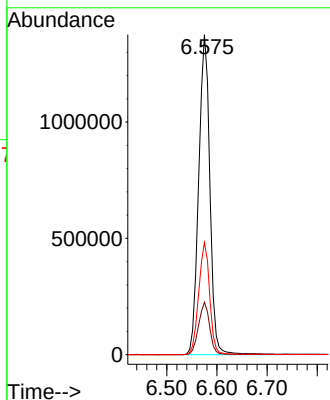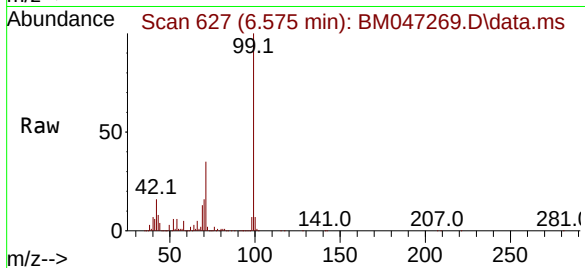


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.116 min Scan# 1229
Delta R.T. -0.018 min
Lab File: BM047269.D
Acq: 20 Aug 2024 13:27

Tgt Ion: 136 Resp: 806956

Ion	Ratio	Lower	Upper
136	100		
137	10.2	8.8	13.2
54	7.0	6.0	9.0
68	5.6	4.8	7.2


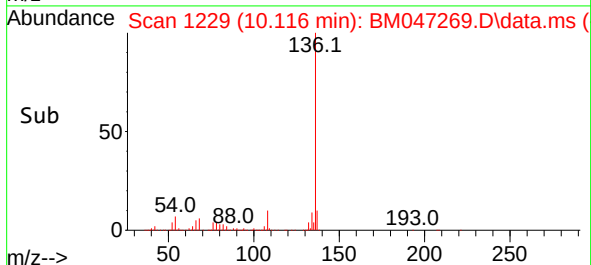
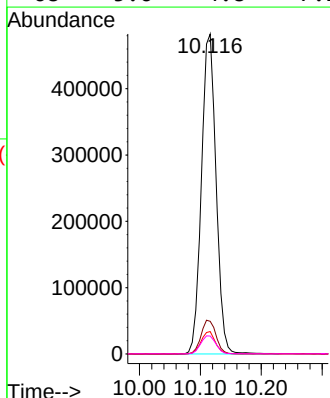
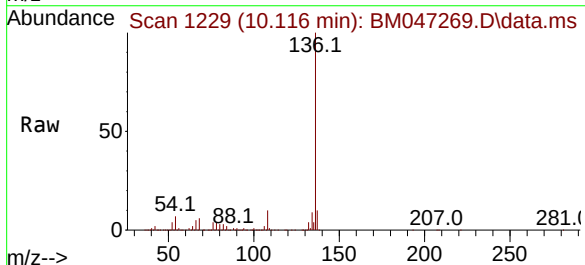


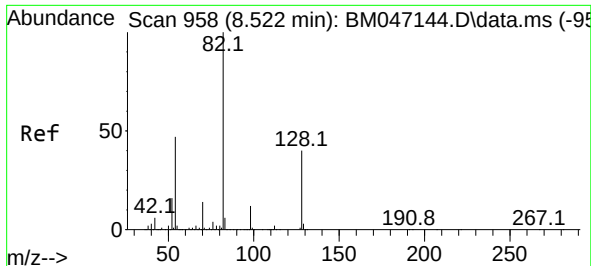

#23
Nitrobenzene-d5
Concen: 84.869 ng
RT: 8.504 min Scan# 91
Delta R.T. -0.018 min
Lab File: BM047269.D
Acq: 20 Aug 2024 13:27




Instrument :
BNA_M
ClientSampleId :
932-K1-SD-0.5-1-081524


Tgt Ion: 82 Resp: 1360099
Ion Ratio Lower Upper
82 100
128 42.7 32.3 48.5
54 44.9 37.4 56.2

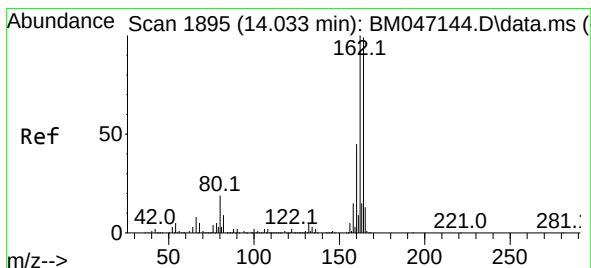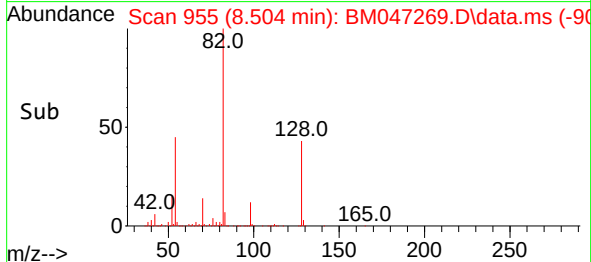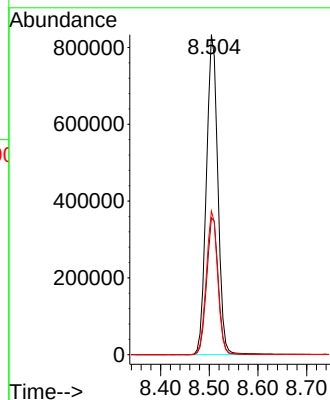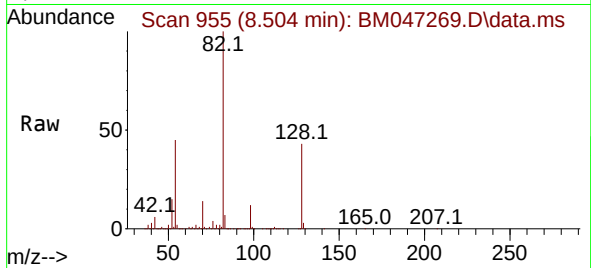

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.022 min Scan# 1893
Delta R.T. -0.012 min
Lab File: BM047269.D
Acq: 20 Aug 2024 13:27

Tgt Ion: 164 Resp: 551285
Ion Ratio Lower Upper
164 100
162 100.3 80.7 121.1
160 44.3 36.0 54.0


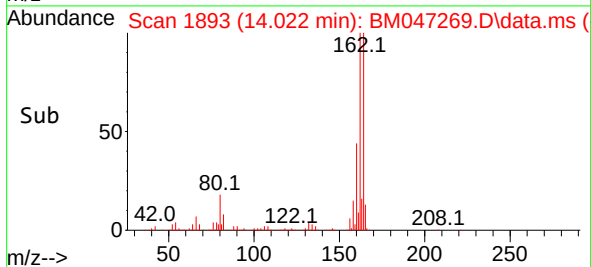
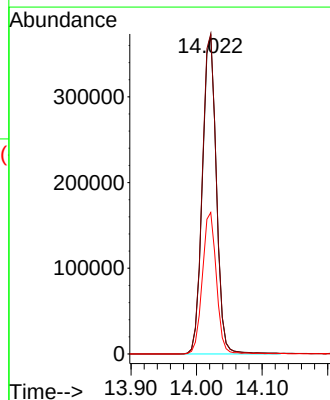
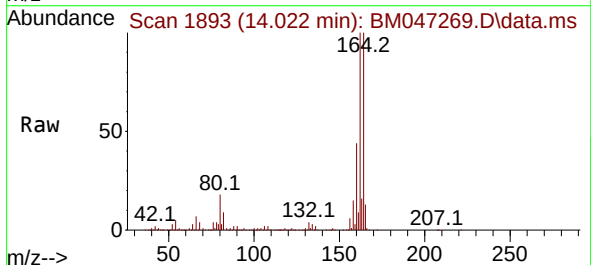


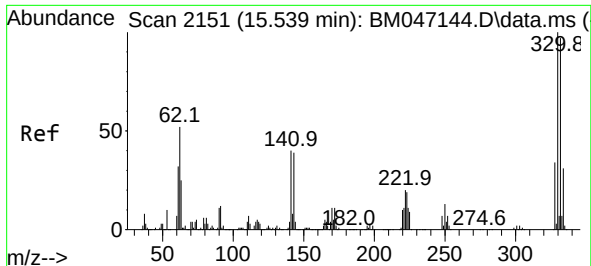

#42
2,4,6-Tribromophenol
Concen: 157.725 ng
RT: 15.533 min Scan# 2151
Delta R.T. -0.006 min
Lab File: BM047269.D
Acq: 20 Aug 2024 13:27




Instrument :
BNA_M
ClientSampleId :
932-K1-SD-0.5-1-081524


Tgt Ion:330 Resp: 1008213
Ion Ratio Lower Upper
330 100
332 96.1 77.4 116.2
141 35.1 31.6 47.4

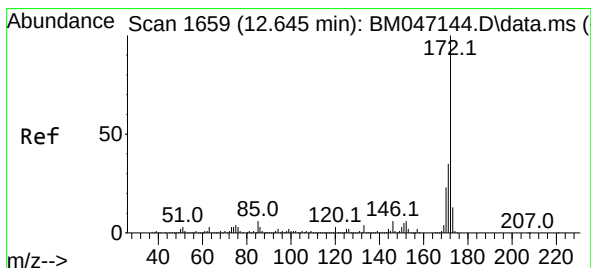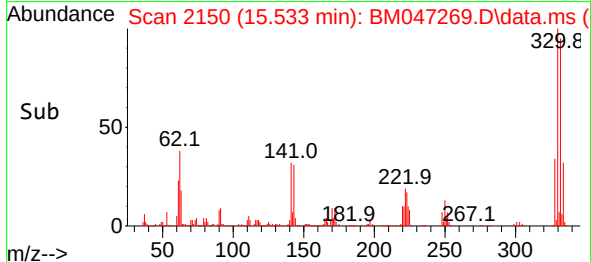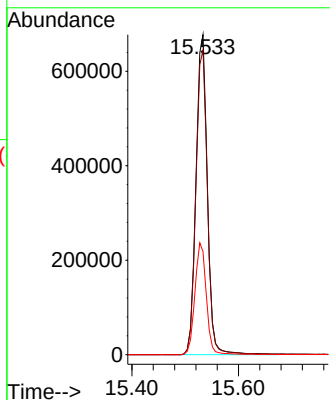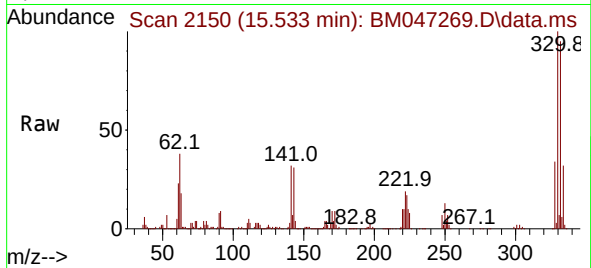

#45
2-Fluorobiphenyl
Concen: 84.797 ng
RT: 12.628 min Scan# 1656
Delta R.T. -0.017 min
Lab File: BM047269.D
Acq: 20 Aug 2024 13:27

Tgt Ion:172 Resp: 3030576
Ion Ratio Lower Upper
172 100
171 35.0 27.8 41.6
170 23.6 18.7 28.1


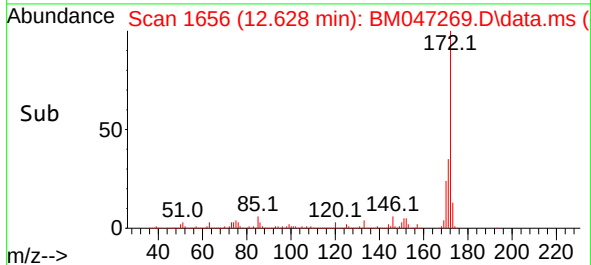
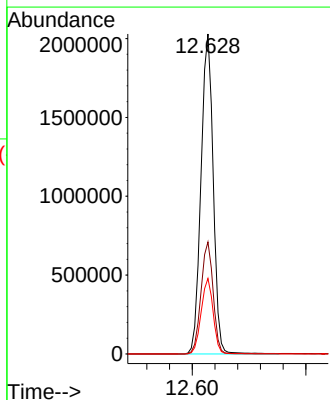
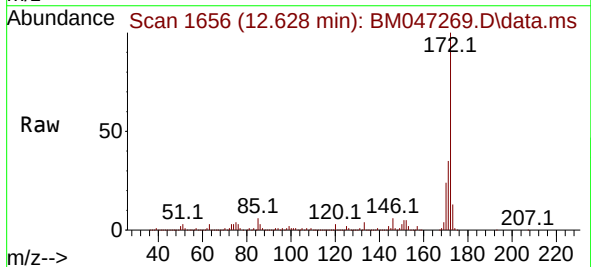


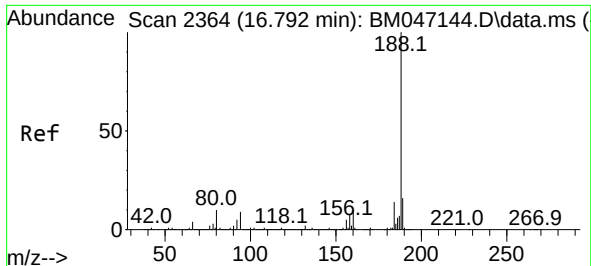

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.786 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM047269.D
Acq: 20 Aug 2024 13:27




Instrument :
BNA_M
ClientSampleId :
932-K1-SD-0.5-1-081524


Tgt Ion:188 Resp: 1228370
Ion Ratio Lower Upper
188 100
94 7.8 7.0 10.6
80 8.8 8.0 12.0

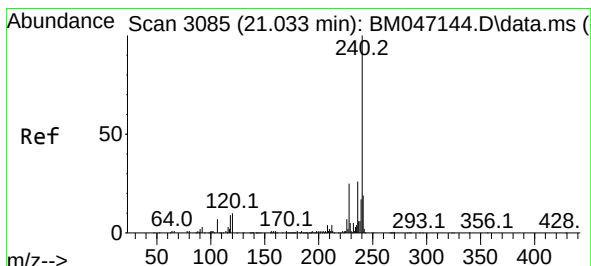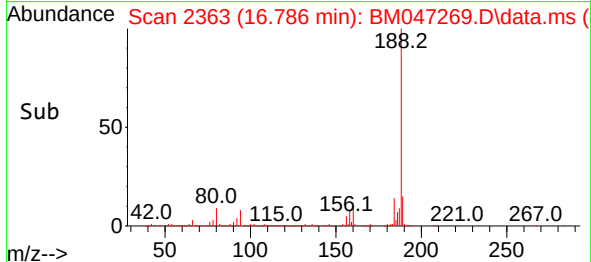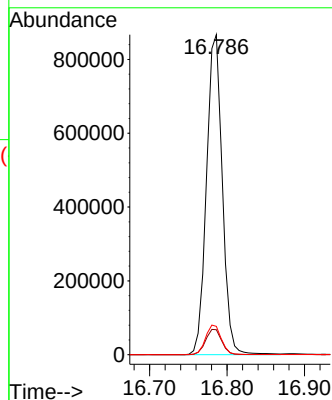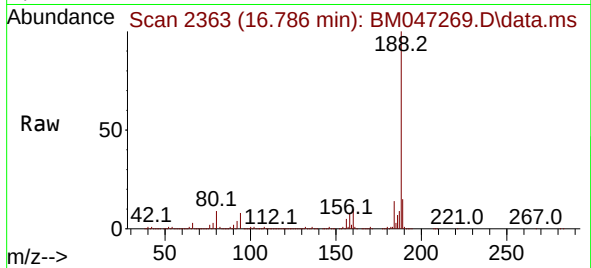

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.027 min Scan# 3084
Delta R.T. -0.006 min
Lab File: BM047269.D
Acq: 20 Aug 2024 13:27

Tgt Ion:240 Resp: 1198327
Ion Ratio Lower Upper
240 100
120 9.0 8.2 12.2
236 25.6 20.6 30.8


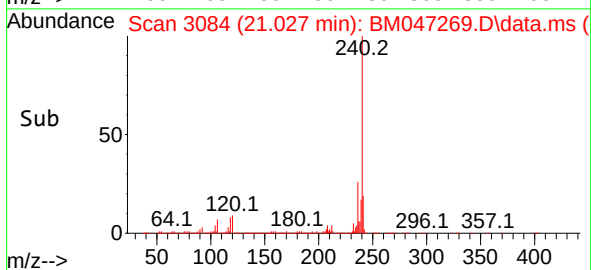
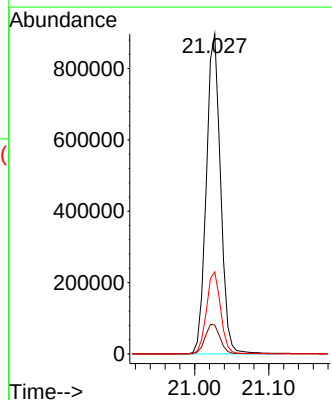
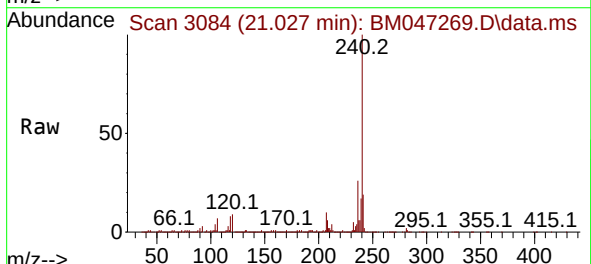


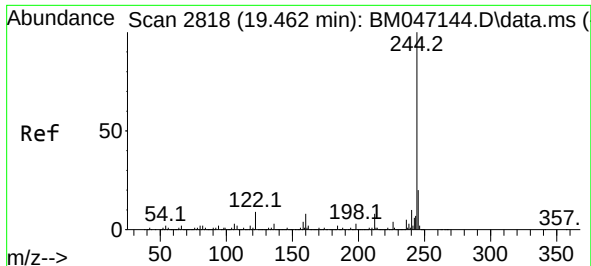

#79
Terphenyl-d14
Concen: 93.932 ng
RT: 19.457 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM047269.D
Acq: 20 Aug 2024 13:27

Instrument :
BNA_M
ClientSampleId :
932-K1-SD-0.5-1-081524

Tgt Ion:244 Resp: 5253111
Ion Ratio Lower Upper
244 100
212 7.5 6.2 9.4
122 8.4 7.1 10.7

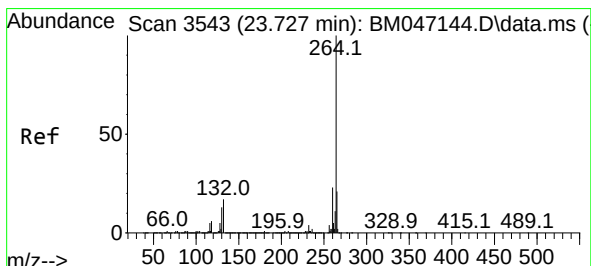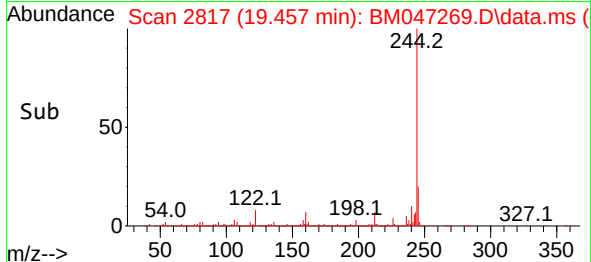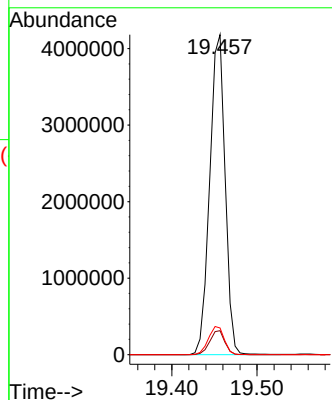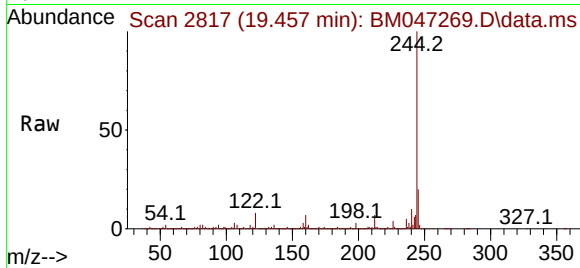

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.721 min Scan# 3542
Delta R.T. -0.006 min
Lab File: BM047269.D
Acq: 20 Aug 2024 13:27

Tgt Ion:264 Resp: 1157106
Ion Ratio Lower Upper
264 100
260 23.2 18.5 27.7
265 22.3 17.3 25.9

