
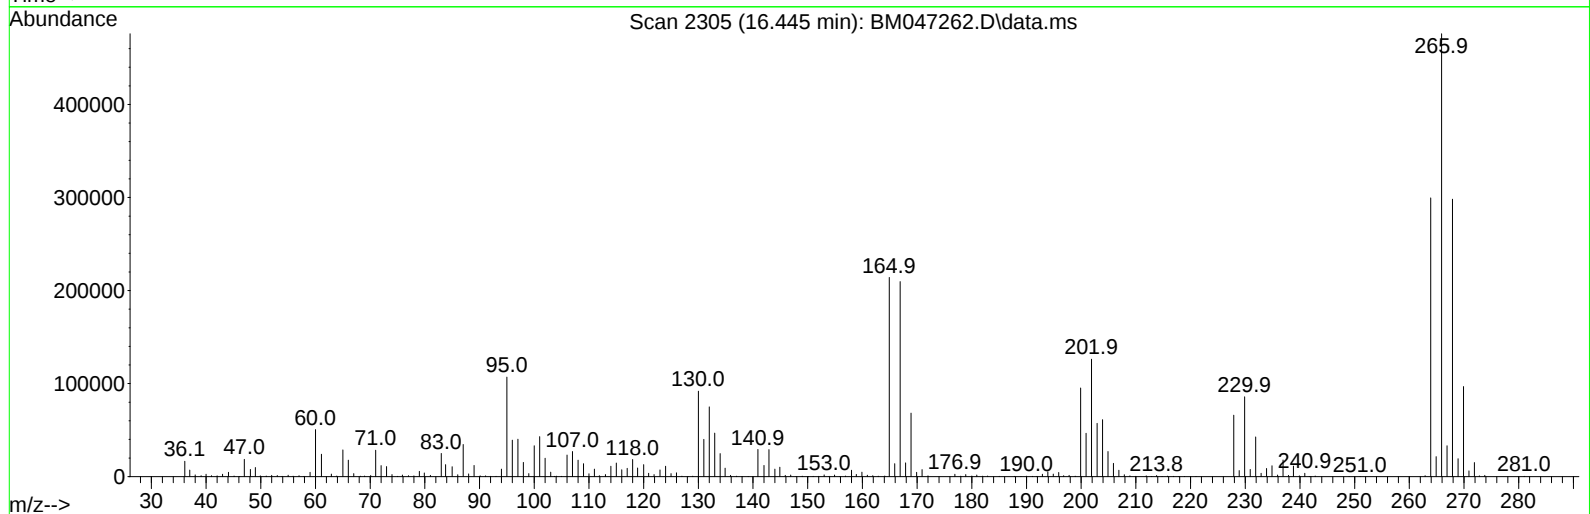


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082024\
Data File : BM047262.D
Acq On : 20 Aug 2024 08:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 10:58:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

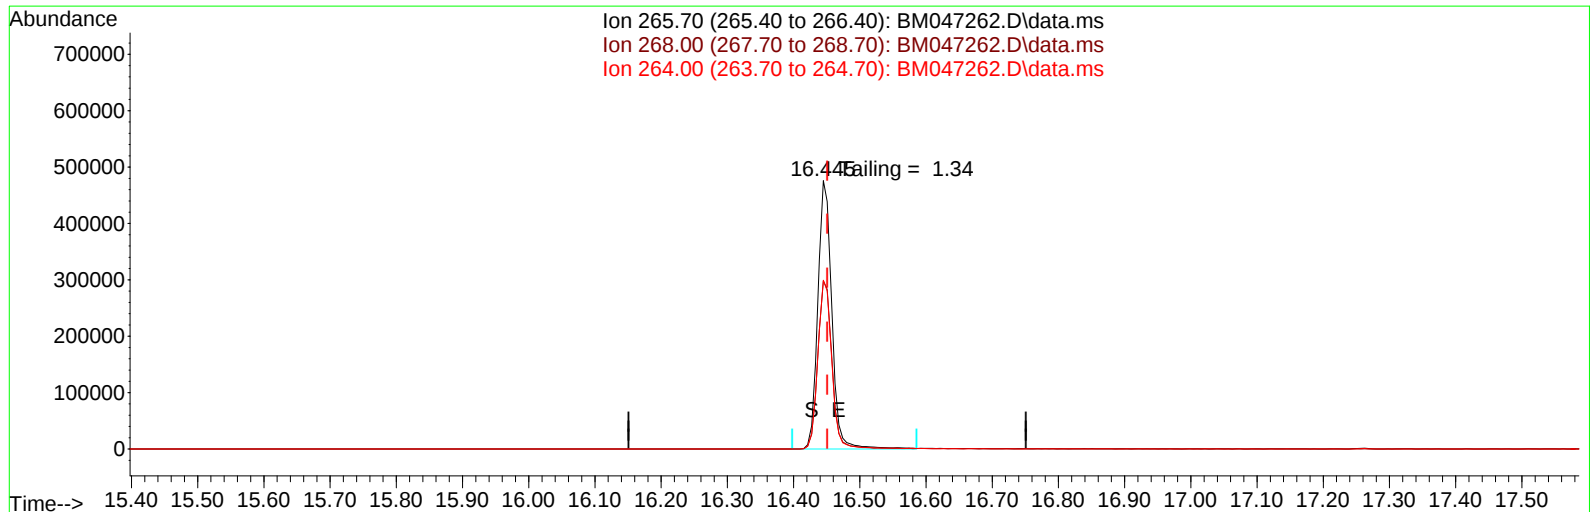

TIC: BM047262.D\data.ms

(70) Pentachlorophenol (C)



16.445min (-0.006) 180601.15 ng

response 698379

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.65
264.00	62.00	62.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082024\
Data File : BM047262.D
Acq On : 20 Aug 2024 08:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 15:16:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

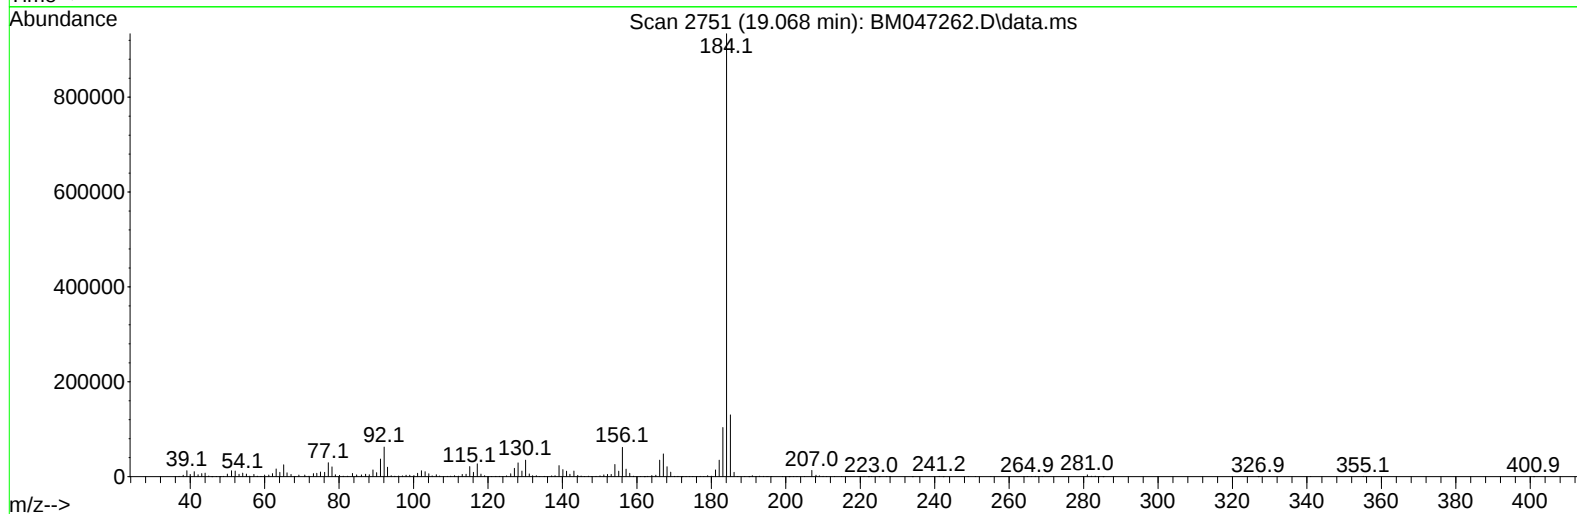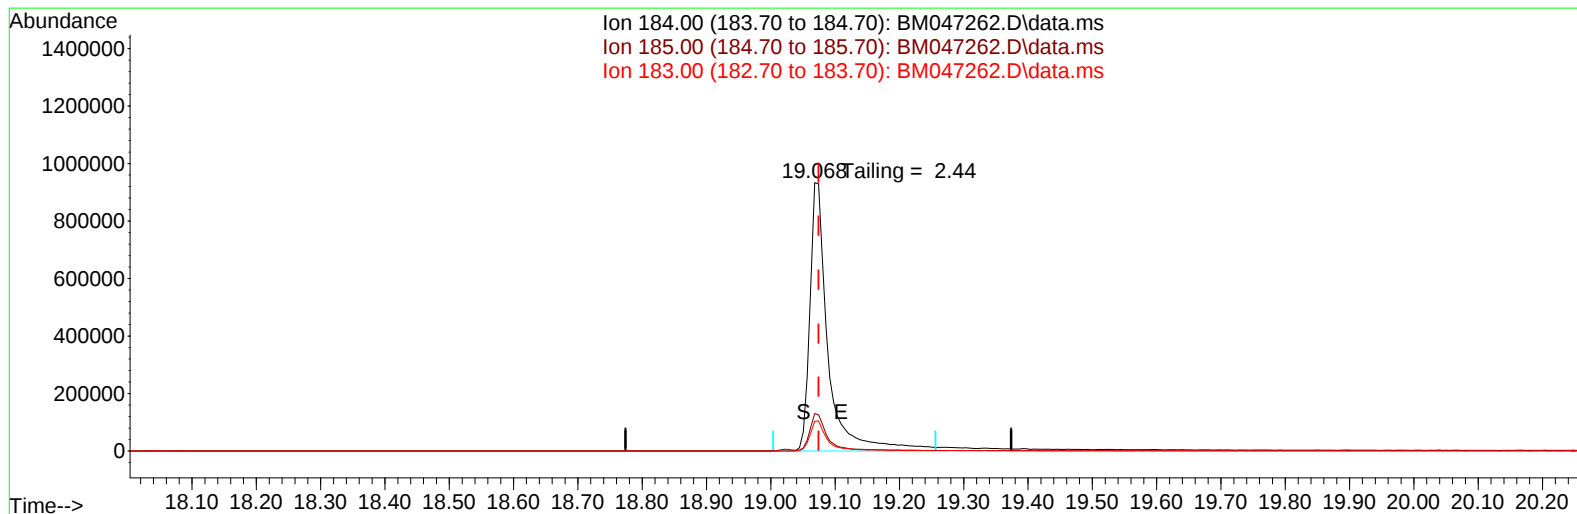

TIC: BM047262.D\data.ms

(77) Benzidine**19.068min (-0.006) 50230.94 ng****response 1855306**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.95
183.00	11.30	11.10
0.00	0.00	0.00