
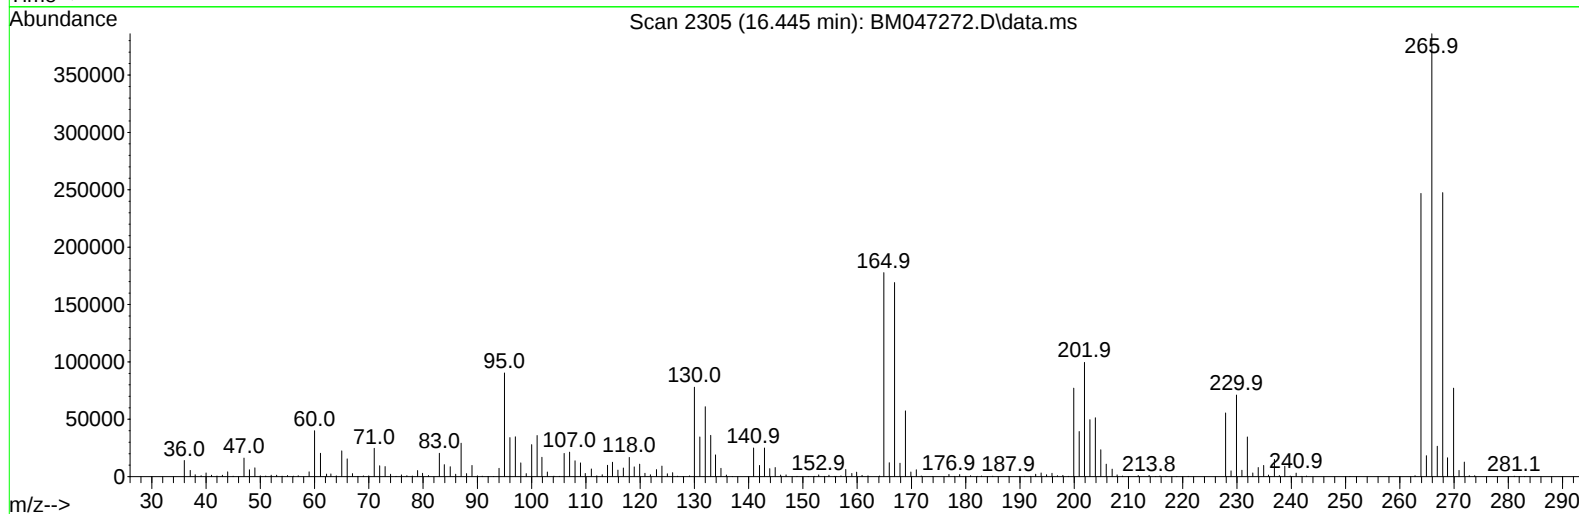


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM082024\  
Data File : BM047272.D  
Acq On : 20 Aug 2024 15:35  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 16:33:10 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM081024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sun Aug 11 23:47:58 2024  
Response via : Initial Calibration

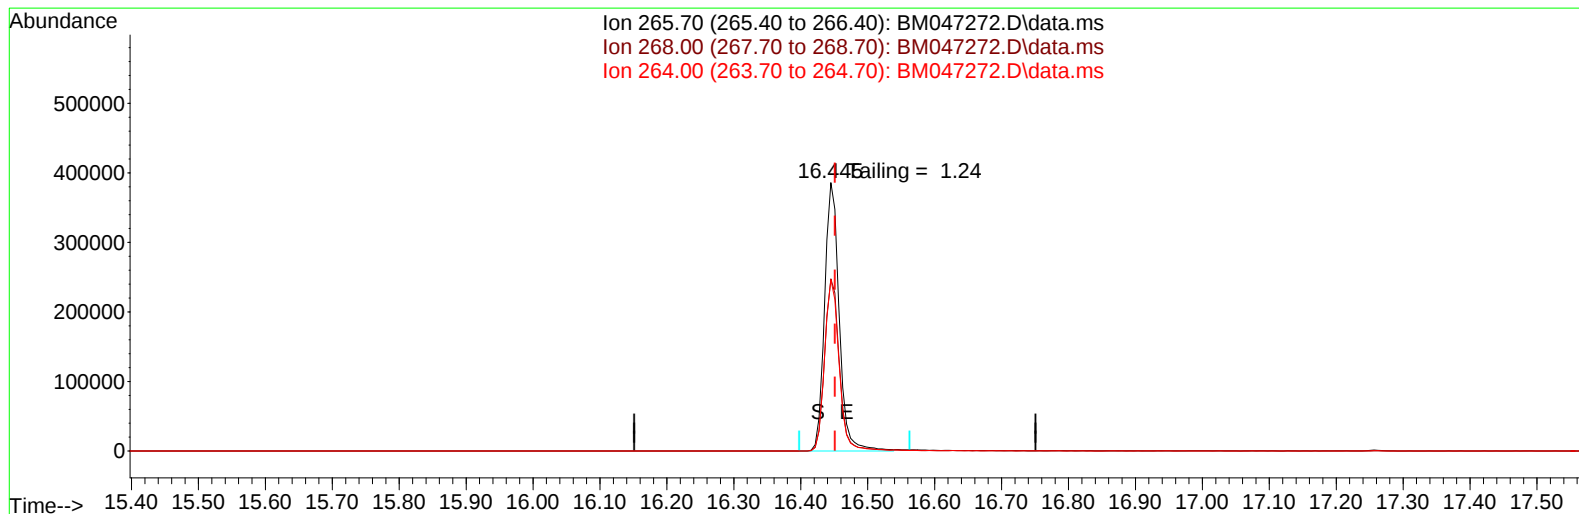

TIC: BM047272.D\data.ms

**(70) Pentachlorophenol (C)**



16.445min (-0.006) 238508.50 ng

response 588500

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 64.14  |
| 264.00 | 62.00  | 63.94  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM082024\  
Data File : BM047272.D  
Acq On : 20 Aug 2024 15:35  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 16:33:10 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM081024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sun Aug 11 23:47:58 2024  
Response via : Initial Calibration

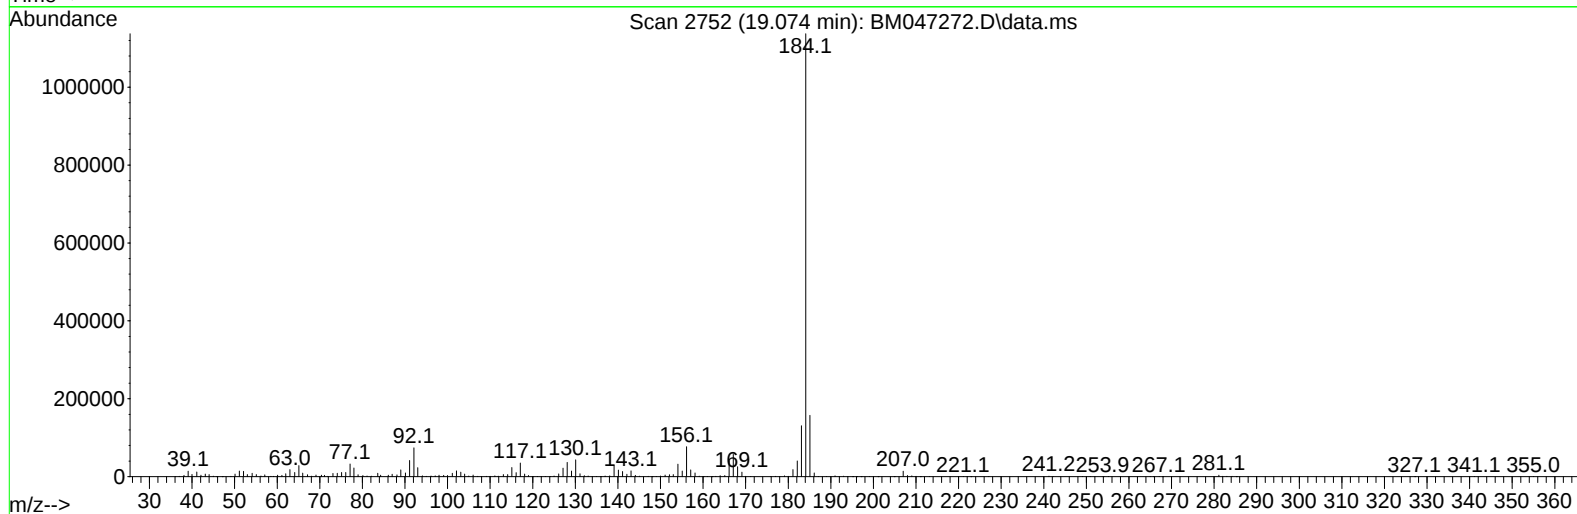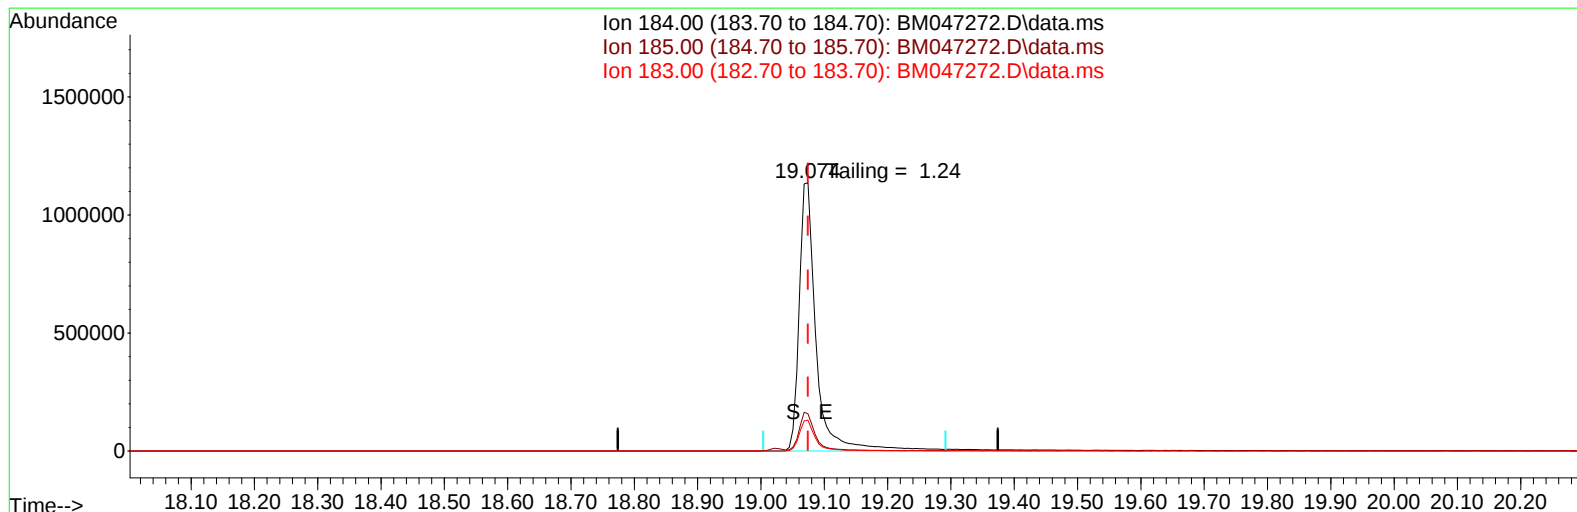

TIC: BM047272.D\data.ms

**(77) Benzidine****19.074min (-0.000) 24392.62 ng****response 2127873**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.70  | 13.84  |
| 183.00 | 11.30  | 11.50  |
| 0.00   | 0.00   | 0.00   |