

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082024\
 Data File : BM047275.D
 Acq On : 20 Aug 2024 18:16
 Operator : RC/JU
 Sample : PB162861BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB162861BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047275.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.569	281	286	293	rBV	272913	357444	3.00%	0.607%
2	5.016	356	362	377	rBV	4387238	6010197	50.46%	10.203%
3	6.575	620	627	641	rBV	3795345	5943101	49.90%	10.089%
4	7.357	754	760	769	rBV	991146	1528763	12.84%	2.595%
5	8.504	947	955	969	rBV	2444998	4091100	34.35%	6.945%
6	10.110	1220	1228	1241	rBV	1143367	1959109	16.45%	3.326%
7	12.628	1648	1656	1675	rBV	5779241	8846874	74.28%	15.019%
8	14.016	1886	1892	1903	rBV	1628608	2429238	20.40%	4.124%
9	15.527	2142	2149	2167	rBV	4110414	6527449	54.80%	11.082%
10	16.780	2353	2362	2377	rBV	1872838	2802152	23.53%	4.757%
11	17.715	2517	2521	2534	rBV2	71826	158525	1.33%	0.269%
12	19.451	2810	2816	2827	rBV	9782179	11910713	100.00%	20.221%
13	21.021	3078	3083	3095	rBV	2116270	3004816	25.23%	5.101%
14	23.721	3535	3542	3559	rVB	1298074	3334502	28.00%	5.661%




Sum of corrected areas: 58903983

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082024\
Data File : BM047275.D
Acq On : 20 Aug 2024 18:16
Operator : RC/JU
Sample : PB162861BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB162861BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

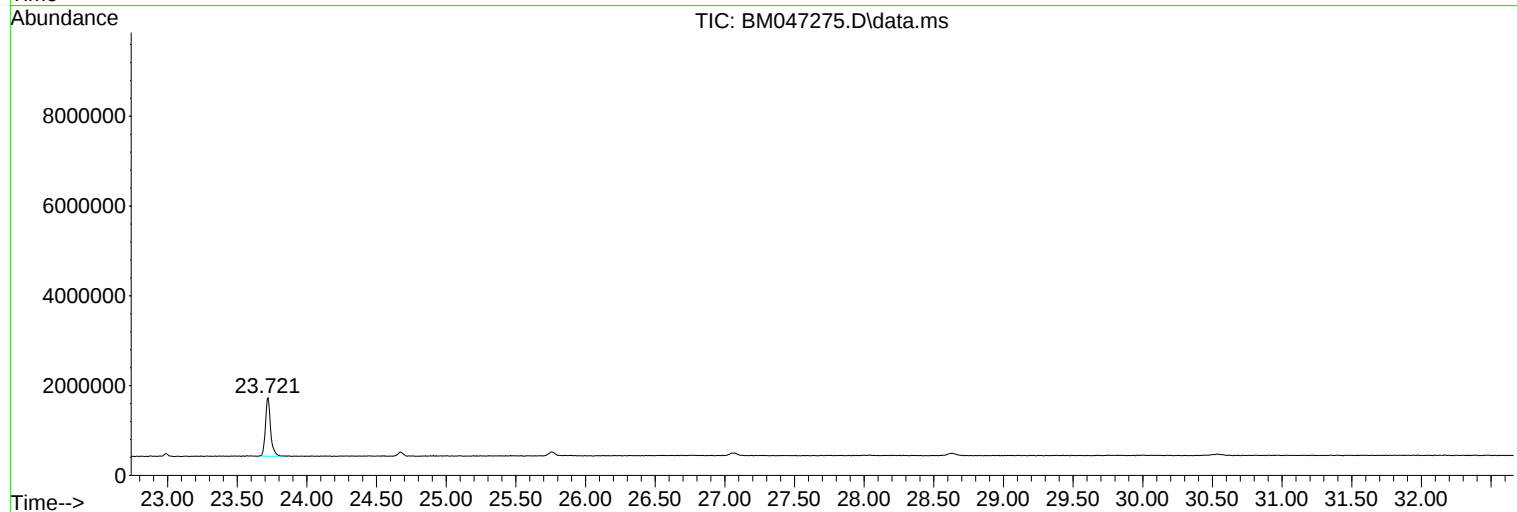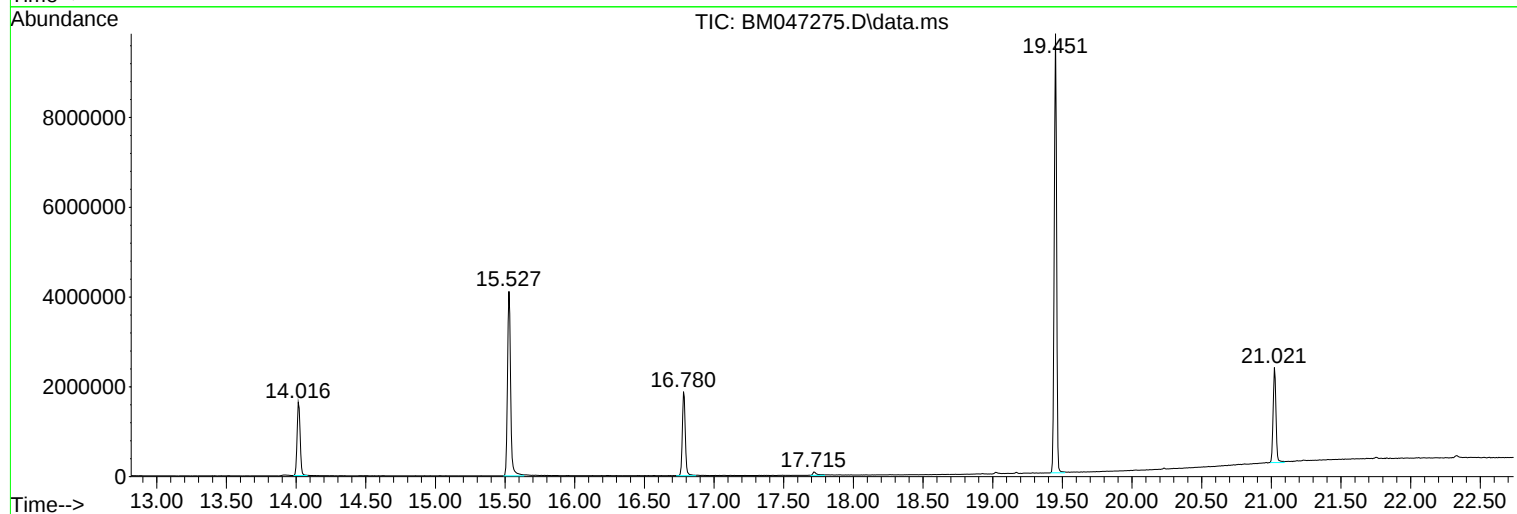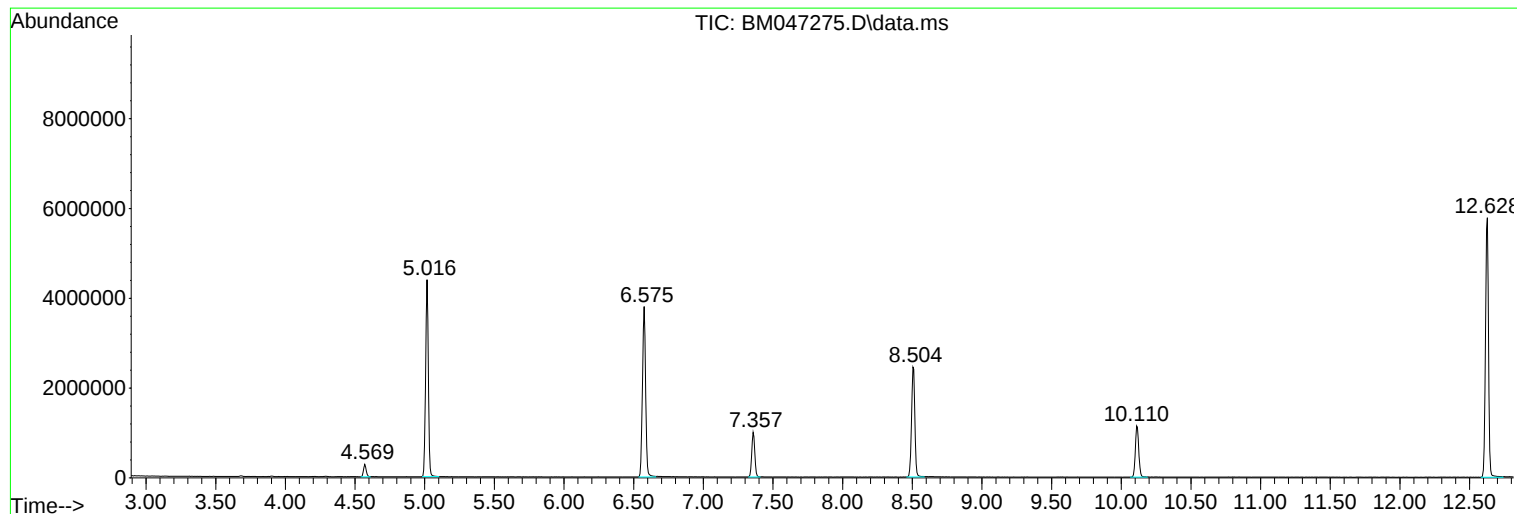

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082024\
Data File : BM047275.D
Acq On : 20 Aug 2024 18:16
Operator : RC/JU
Sample : PB162861BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB162861BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.569	4.68 ng	357444	1,4-Dichlorobenzene-d4	7.357

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	32		
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17		
4	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9		
5	Guanidine	59	CH5N3	000113-00-8	9		

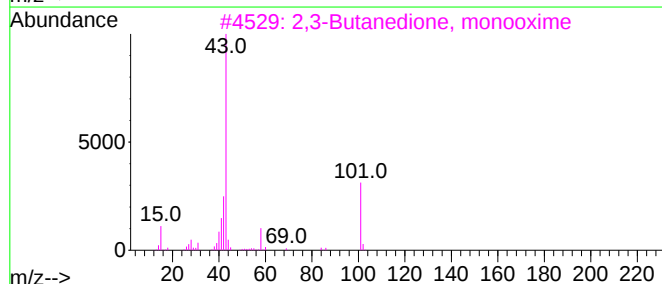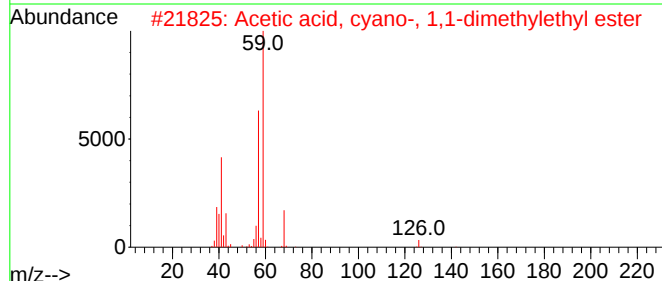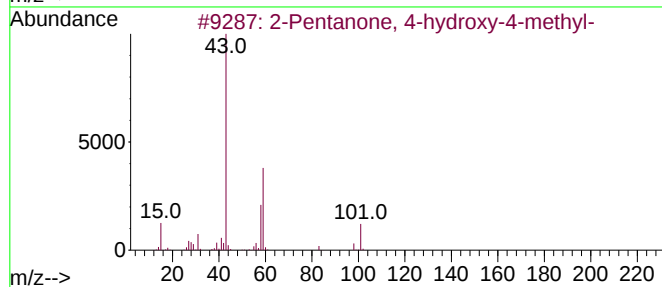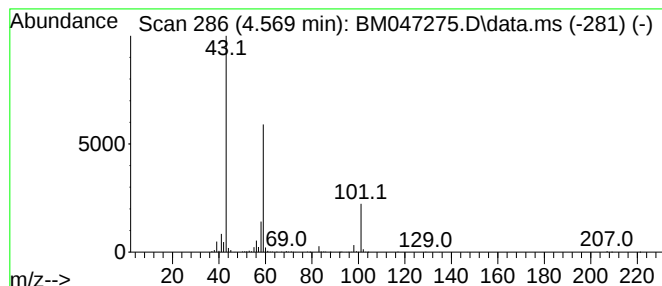

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082024\
Data File : BM047275.D
Acq On : 20 Aug 2024 18:16
Operator : RC/JU
Sample : PB162861BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB162861BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.569	4.7	ng	357444	1	7.357	1528760	20.0