
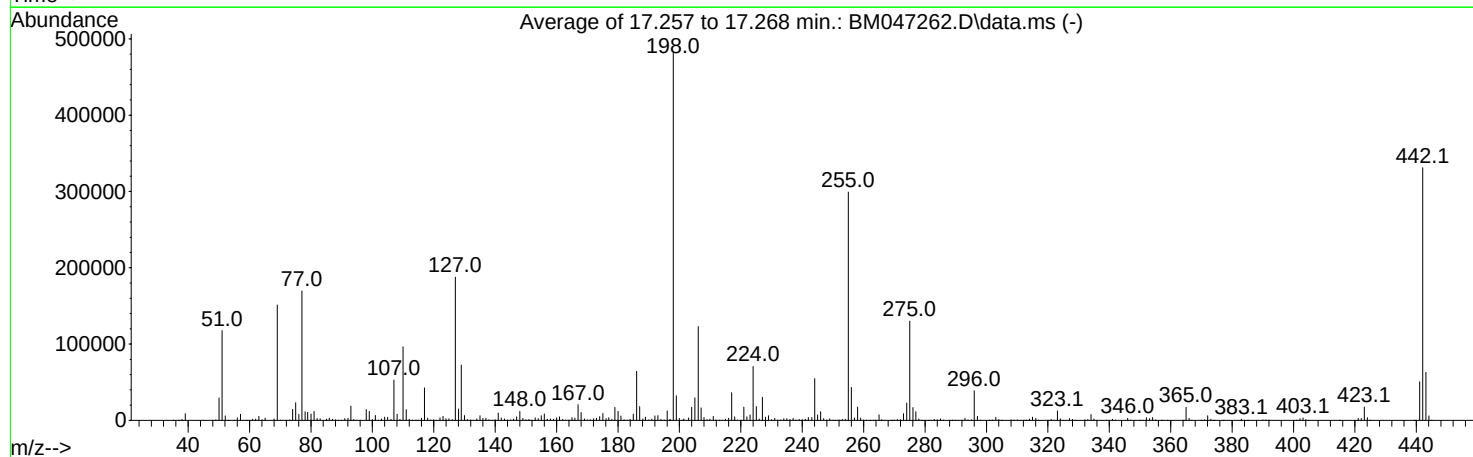


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082024\
Data File : BM047262.D
Acq On : 20 Aug 2024 08:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Aug 11 23:47:58 2024

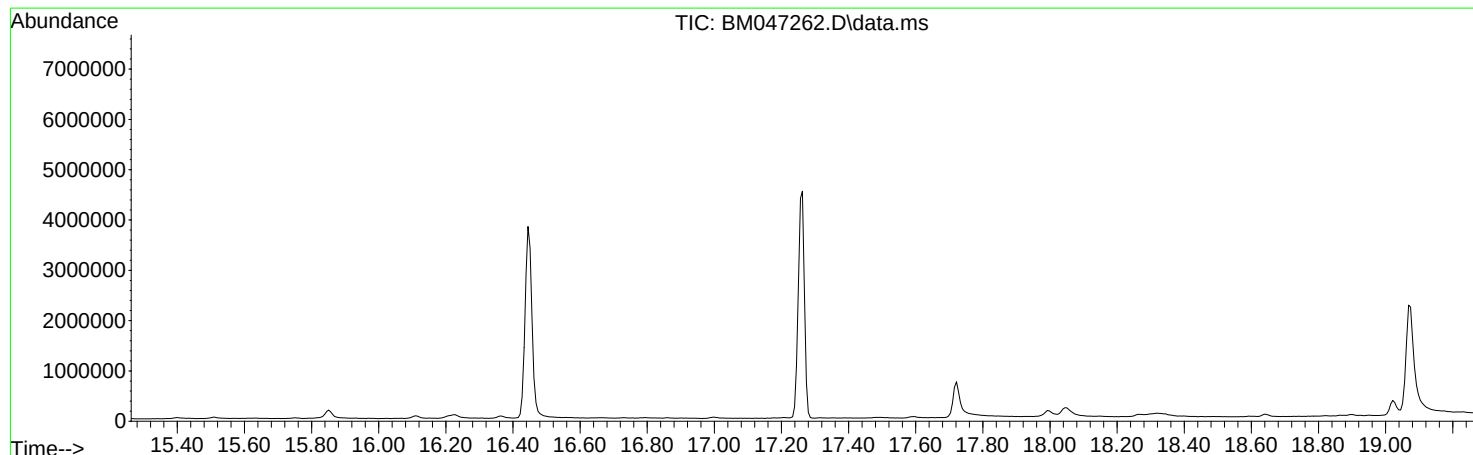

AutoFind: Scans 2443, 2444, 2445; Background Corrected with Scan 2434

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.4	117648	PASS
68	69	0.00	2	1.3	1897	PASS
69	198	0.00	100	31.4	151144	PASS
70	69	0.00	2	0.3	456	PASS
127	198	10	80	38.9	187746	PASS
197	198	0.00	2	0.2	957	PASS
198	198	100	100	100.0	482112	PASS
199	198	5	9	6.7	32411	PASS
275	198	10	60	26.9	129923	PASS
365	198	1	100	3.6	17183	PASS
441	198	0.01	100	10.5	50629	PASS
442	442	50	100	100.0	331221	PASS
443	442	15	24	19.0	62899	PASS

DDT Breakdown



Date	Instrument Name	DFTPP Data File
8/20/2024	BNA_M	<u>BM047262.D</u>
Compound Name	Response	Retention Time
DDT	1792853	20.315
DDD	95970	19.874
DDE	5034	19.362
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
101004	1893857	5.33

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082024\
Data File : BM047262.D
Acq On : 20 Aug 2024 08:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 20 10:58:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

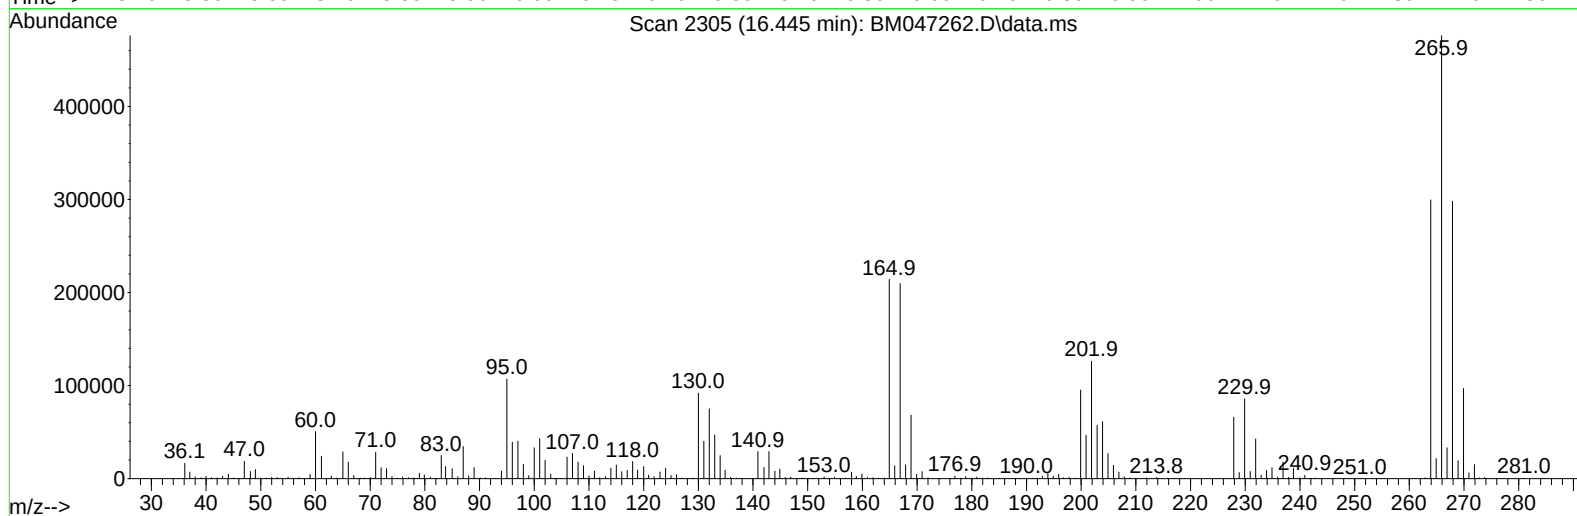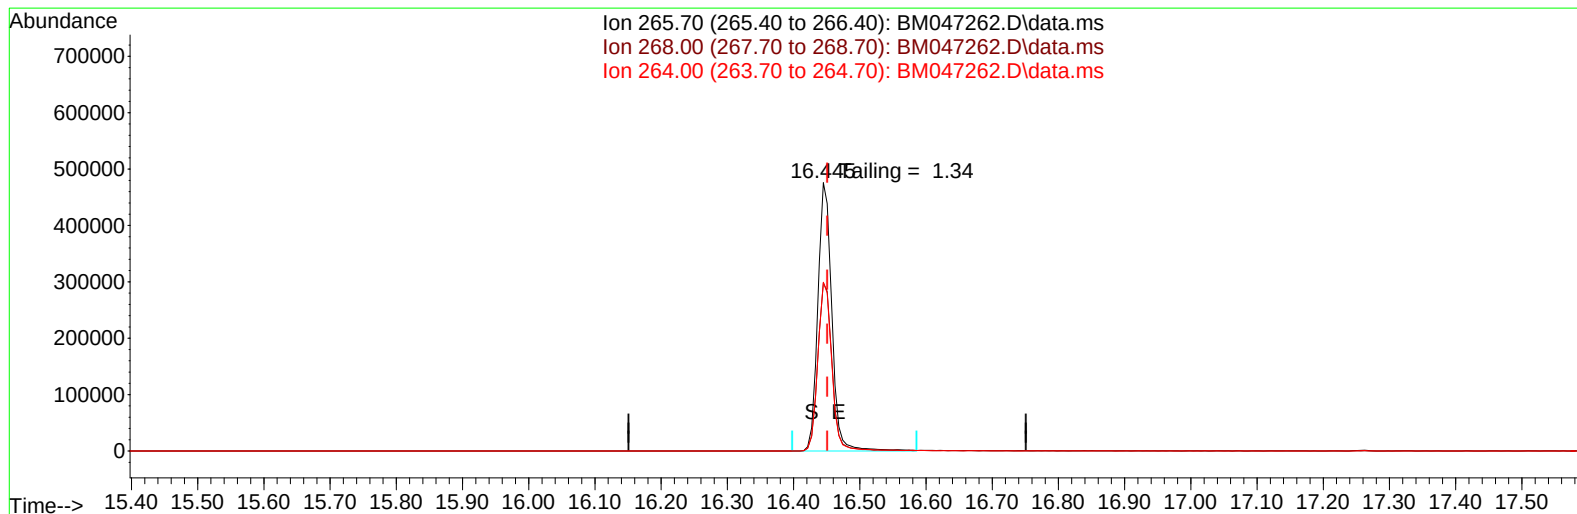

TIC: BM047262.D\data.ms

(70) Pentachlorophenol (C)

16.445min (-0.006) 180601.15 ng



response 698379

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.65
264.00	62.00	62.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082024\
Data File : BM047262.D
Acq On : 20 Aug 2024 08:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 20 15:16:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

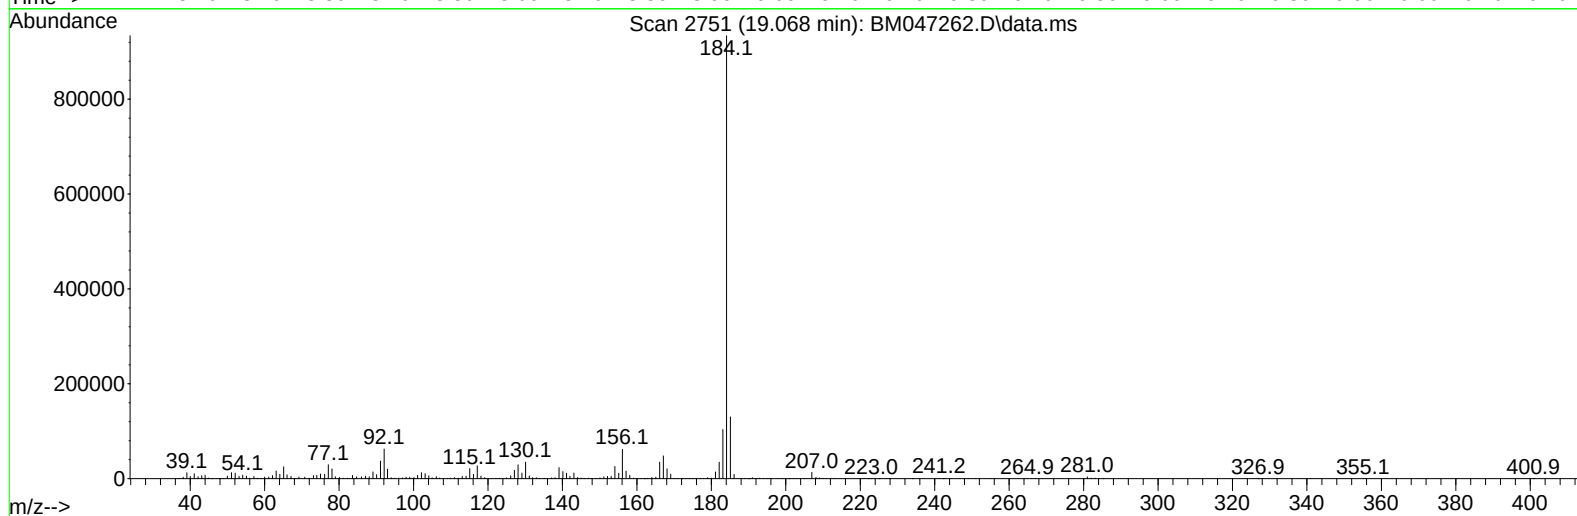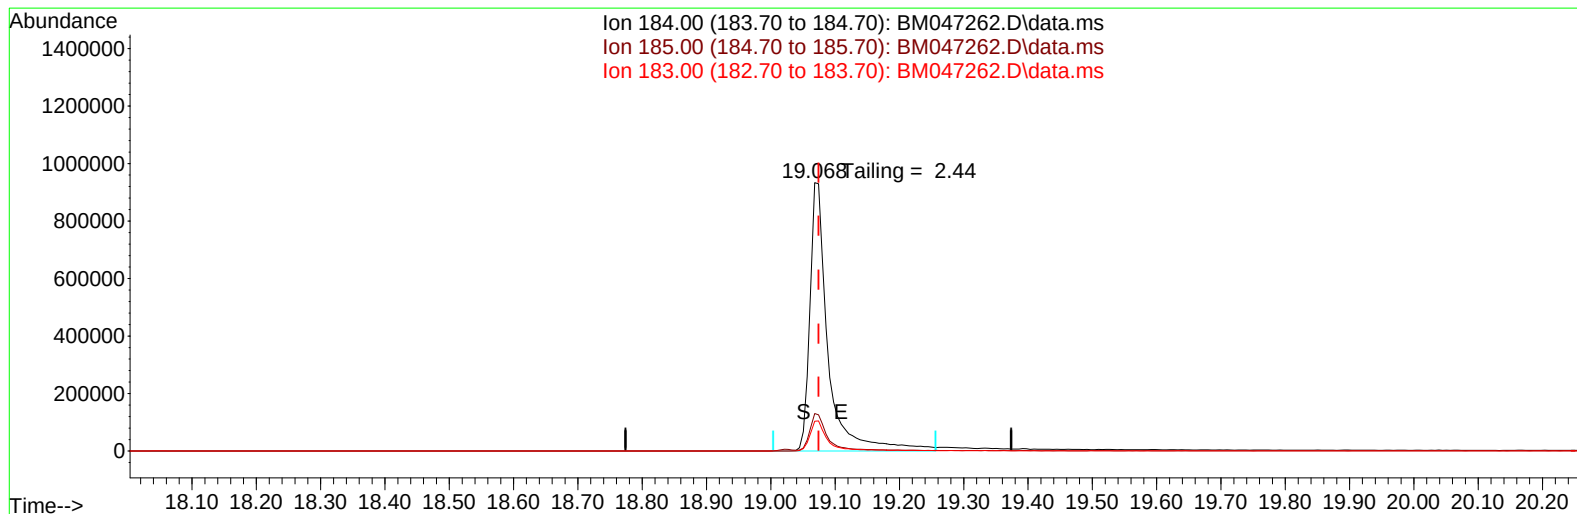

TIC: BM047262.D\data.ms

(77) Benzidine**19.068min (-0.006) 50230.94 ng****response 1855306**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.95
183.00	11.30	11.10
0.00	0.00	0.00