


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082024\
Data File : BM047272.D
Acq On : 20 Aug 2024 15:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Aug 11 23:47:58 2024

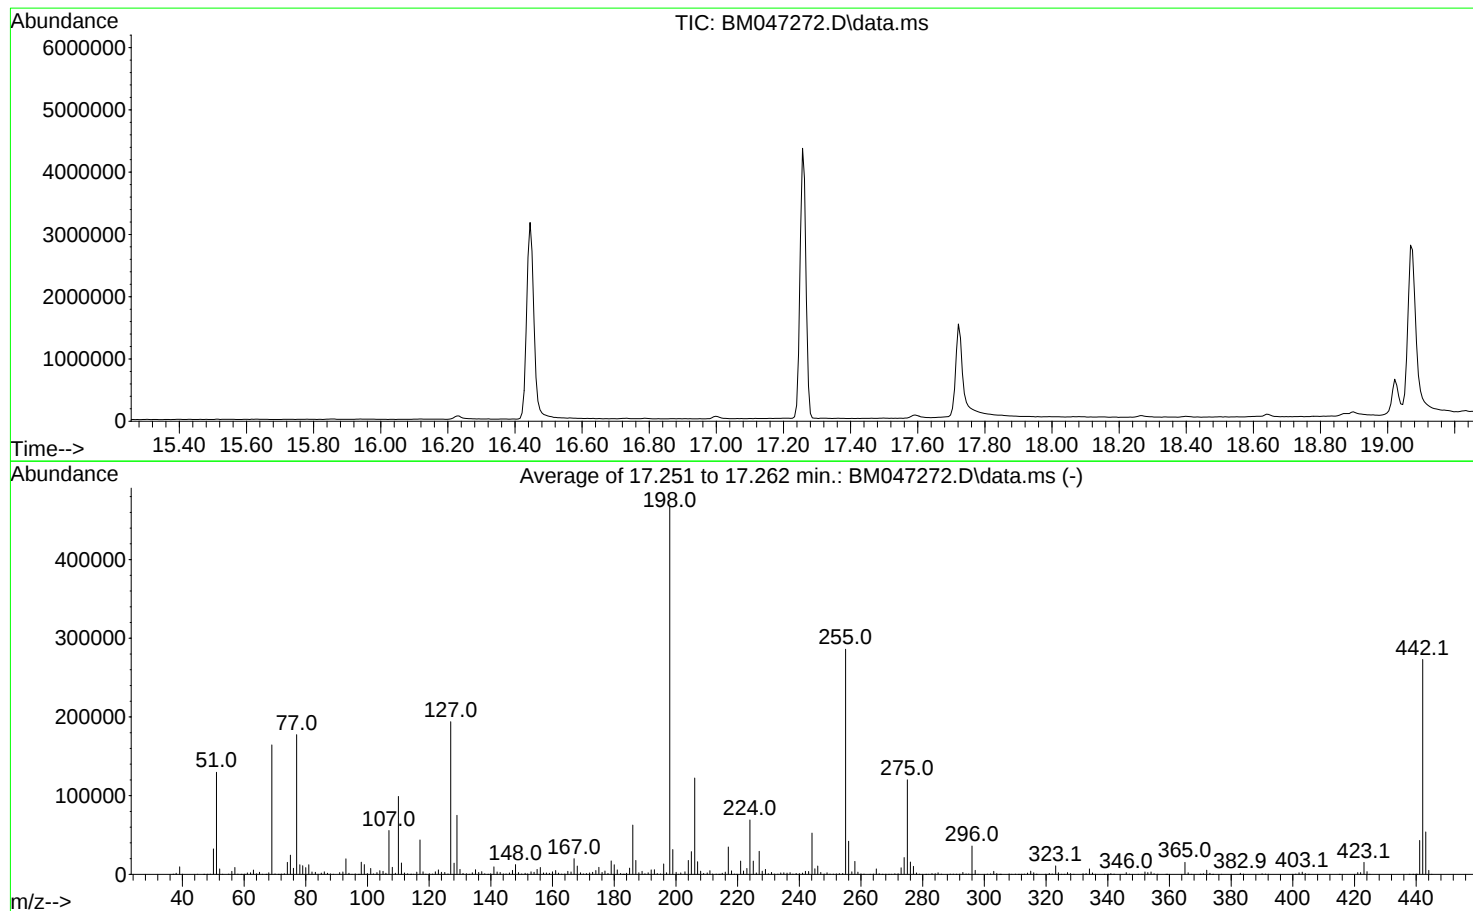

AutoFind: Scans 2442, 2443, 2444; Background Corrected with Scan 2435

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	27.7	129703	PASS
68	69	0.00	2	1.3	2093	PASS
69	198	0.00	100	35.2	164504	PASS
70	69	0.00	2	0.4	648	PASS
127	198	10	80	41.5	193906	PASS
197	198	0.00	2	0.4	2004	PASS
198	198	100	100	100.0	467435	PASS
199	198	5	9	6.7	31467	PASS
275	198	10	60	25.7	120144	PASS
365	198	1	100	3.3	15332	PASS
441	198	0.01	100	9.2	43072	PASS
442	442	50	100	100.0	273109	PASS
443	442	15	24	19.8	53989	PASS

DDT Breakdown



Date	Instrument Name	DFTPP Data File
8/20/2024	BNA_M	<u>BM047272.D</u>
Compound Name	Response	Retention Time
DDT	1424618	20.315
DDD	68922	19.874
DDE	3372	19.356
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
72294	1496912	4.83

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082024\
Data File : BM047272.D
Acq On : 20 Aug 2024 15:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 20 16:33:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

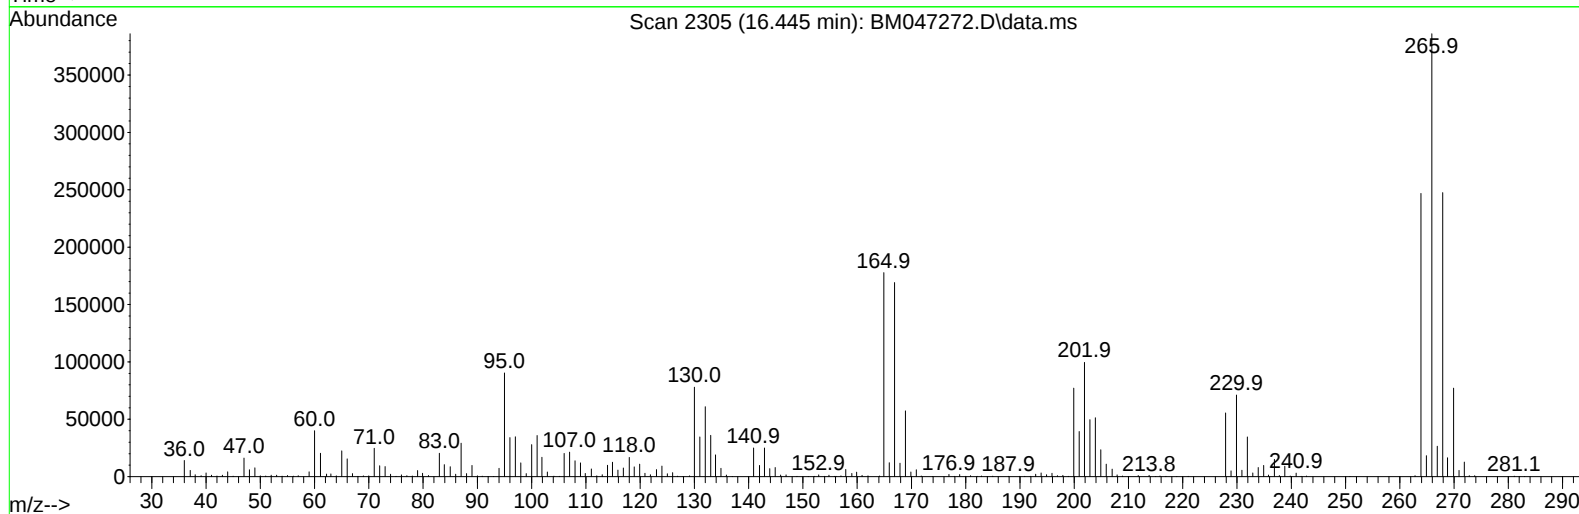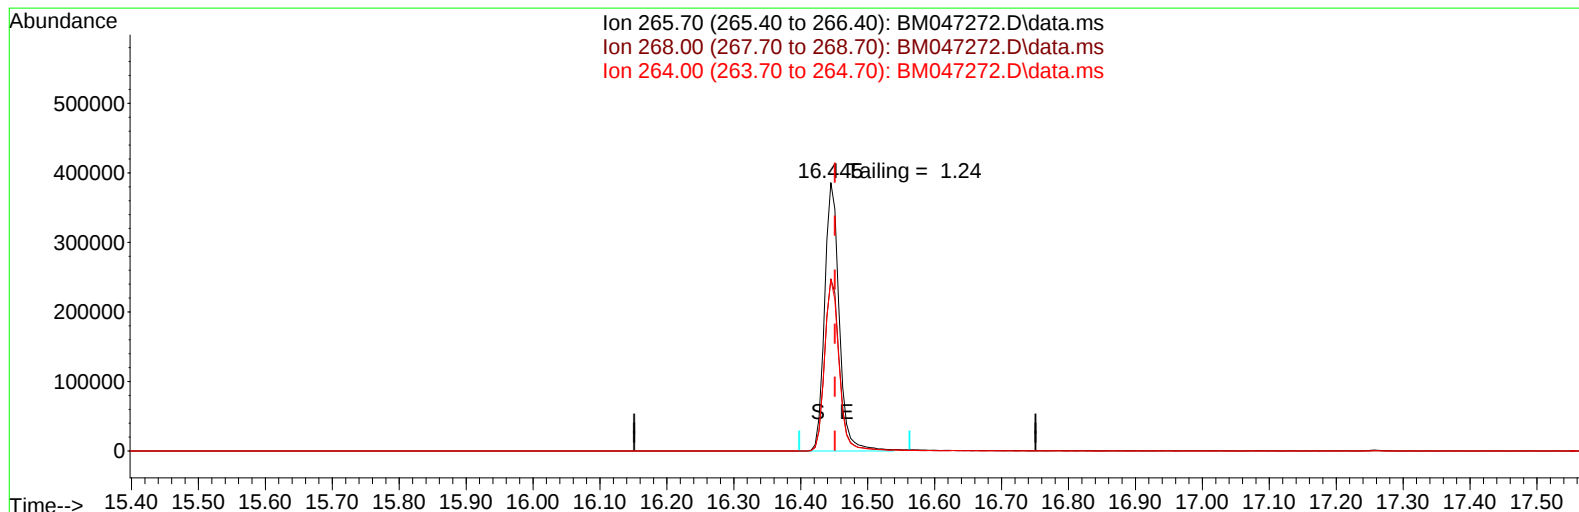

TIC: BM047272.D\data.ms

(70) Pentachlorophenol (C)

16.445min (-0.006) 238508.50 ng



response 588500

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.14
264.00	62.00	63.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082024\
Data File : BM047272.D
Acq On : 20 Aug 2024 15:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 20 16:33:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

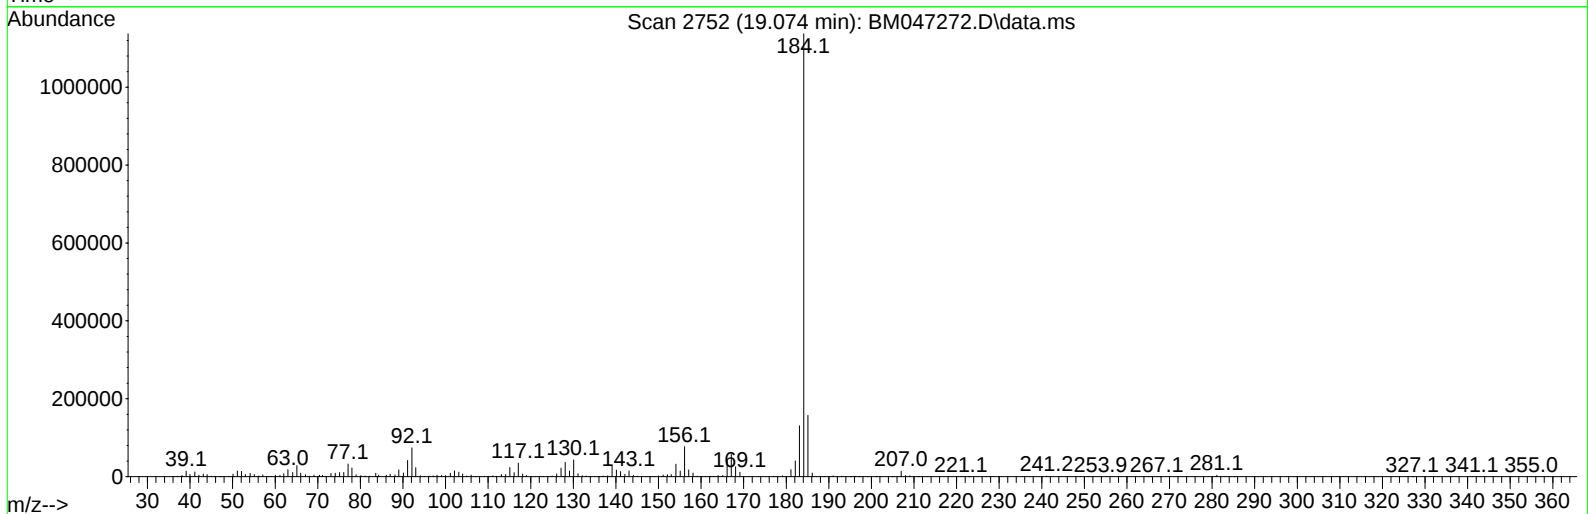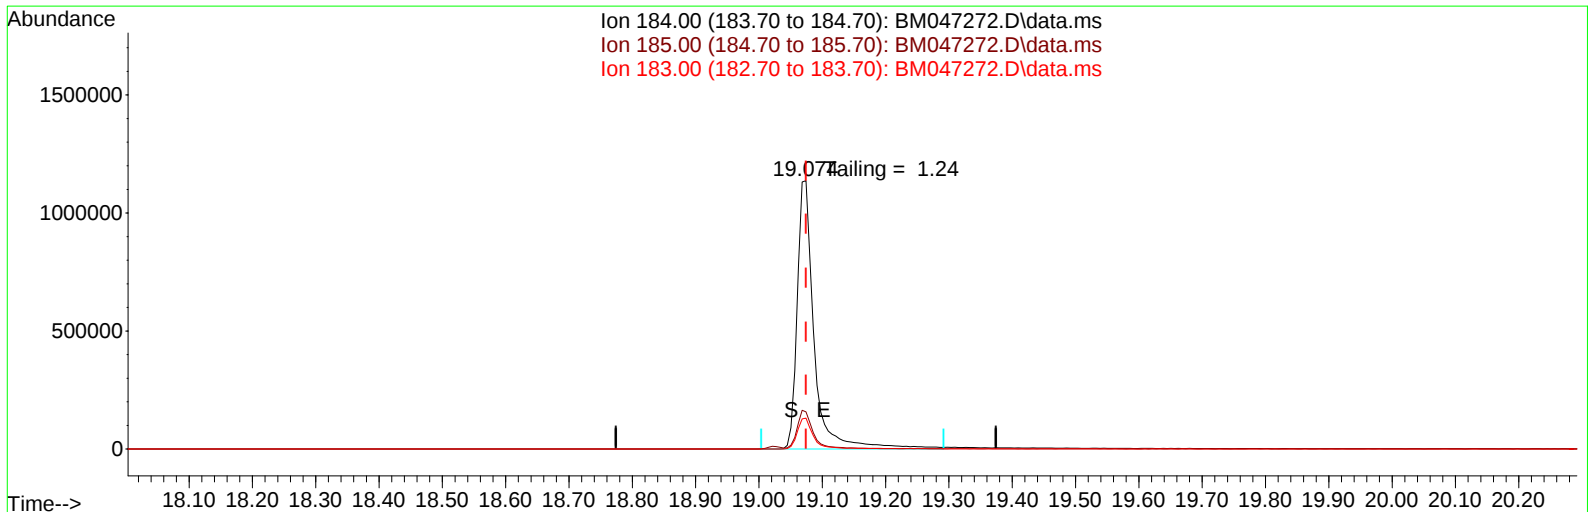

TIC: BM047272.D\data.ms

(77) Benzidine**19.074min (-0.000) 24392.62 ng****response 2127873**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.84
183.00	11.30	11.50
0.00	0.00	0.00