


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082124\
Data File : BM047289.D
Acq On : 21 Aug 2024 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Aug 11 23:47:58 2024

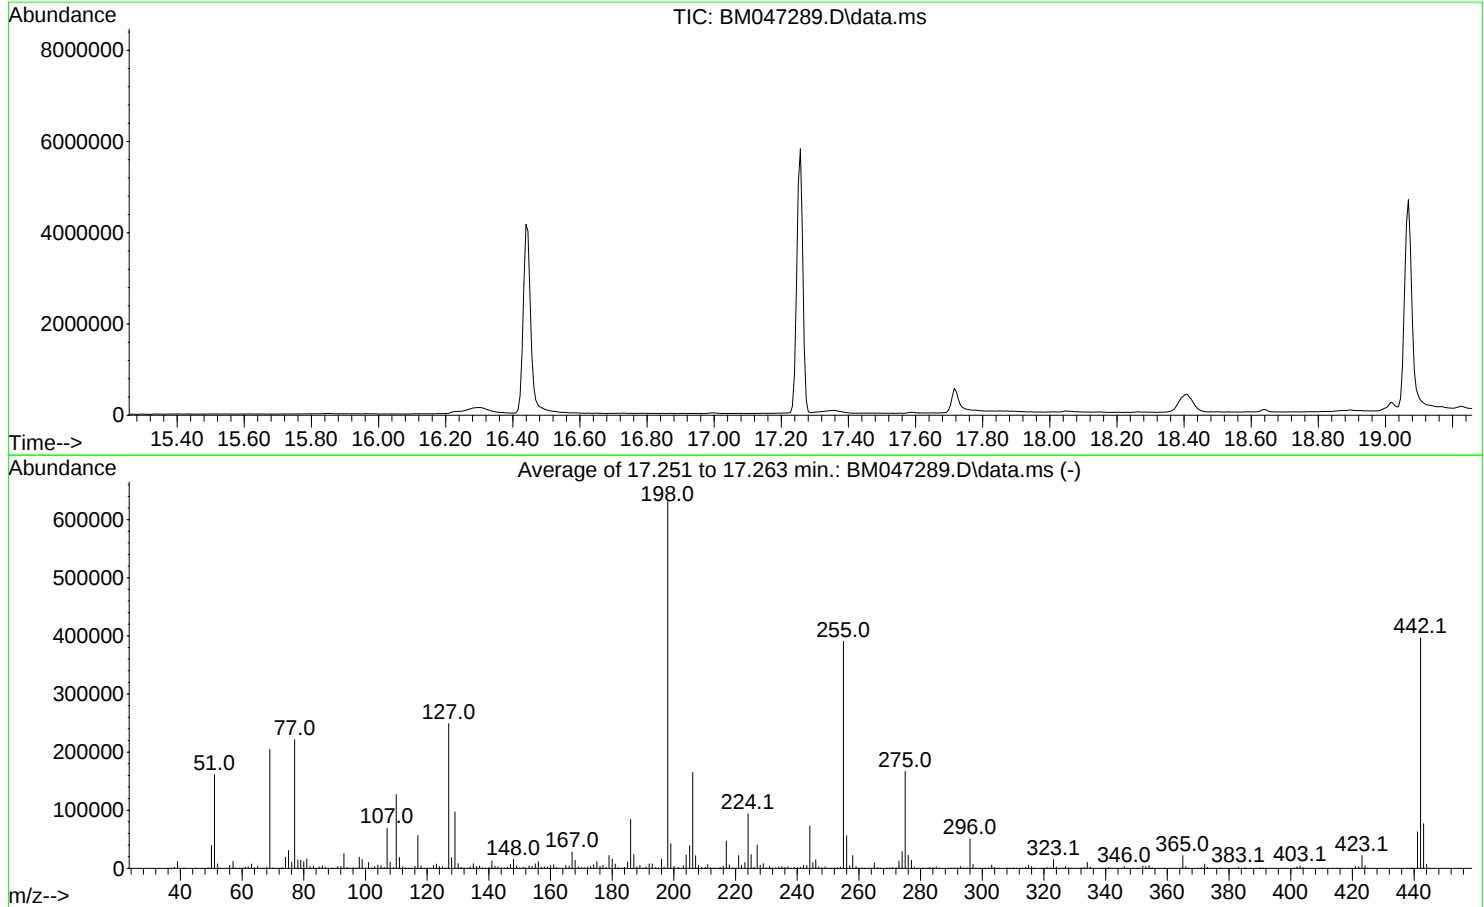

AutoFind: Scans 2442, 2443, 2444; Background Corrected with Scan 2435

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.5	161163	PASS
68	69	0.00	2	1.3	2576	PASS
69	198	0.00	100	32.4	204916	PASS
70	69	0.00	2	0.4	723	PASS
127	198	10	80	39.4	249067	PASS
197	198	0.00	2	0.3	1653	PASS
198	198	100	100	100.0	632939	PASS
199	198	5	9	6.7	42483	PASS
275	198	10	60	26.4	166827	PASS
365	198	1	100	3.5	22171	PASS
441	198	0.01	100	9.9	62925	PASS
442	442	50	100	100.0	396416	PASS
443	442	15	24	19.4	76837	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/21/2024	BNA_M	<u>BM047289.D</u>
Compound Name	Response	Retention Time
DDT	2042202	20.315
DDD	65525	19.868
DDE	2039	19.351
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
67564	2109766	3.20

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082124\
Data File : BM047289.D
Acq On : 21 Aug 2024 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 21 11:01:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

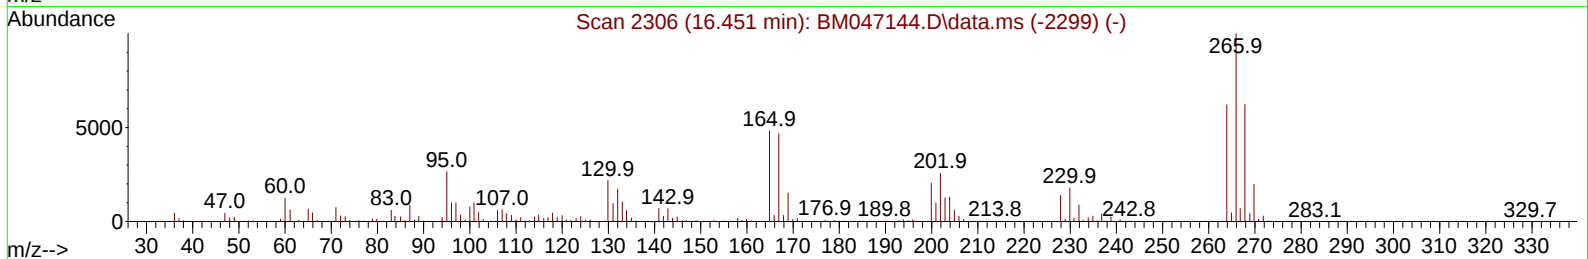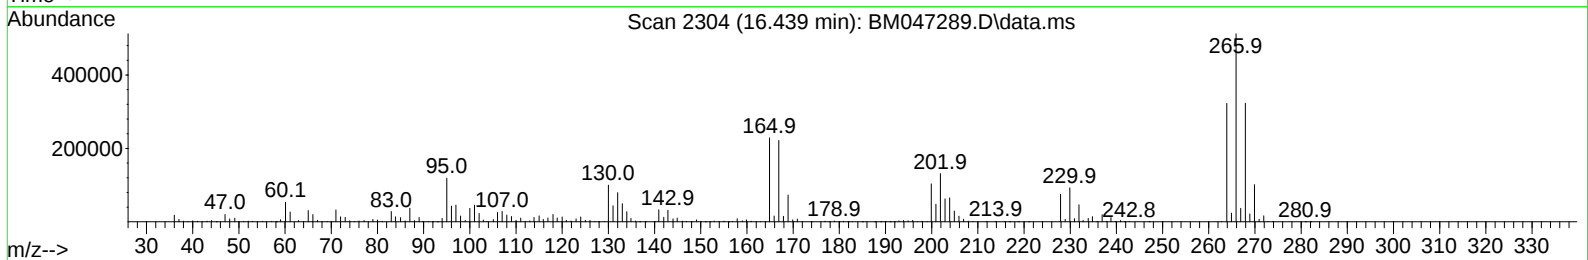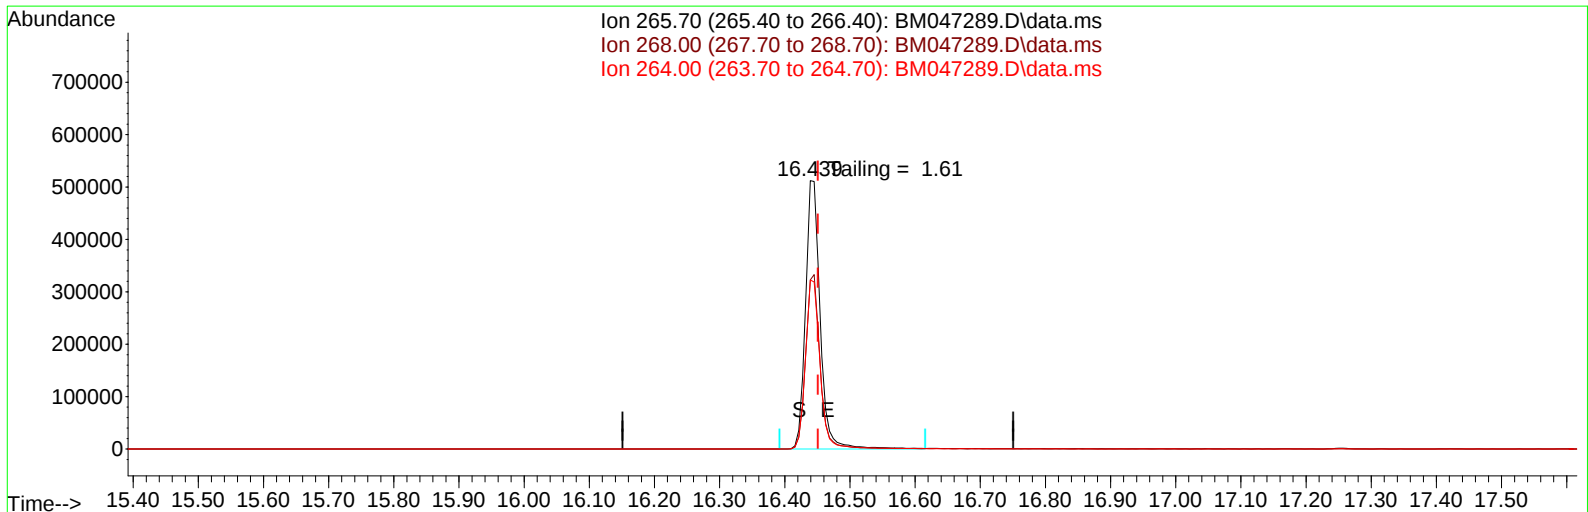

TIC: BM047289.D\data.ms

(70) Pentachlorophenol (C)

16.439min (-0.012) 0.00 ng




response 801900

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.06
264.00	62.00	62.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082124\
Data File : BM047289.D
Acq On : 21 Aug 2024 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 21 11:01:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

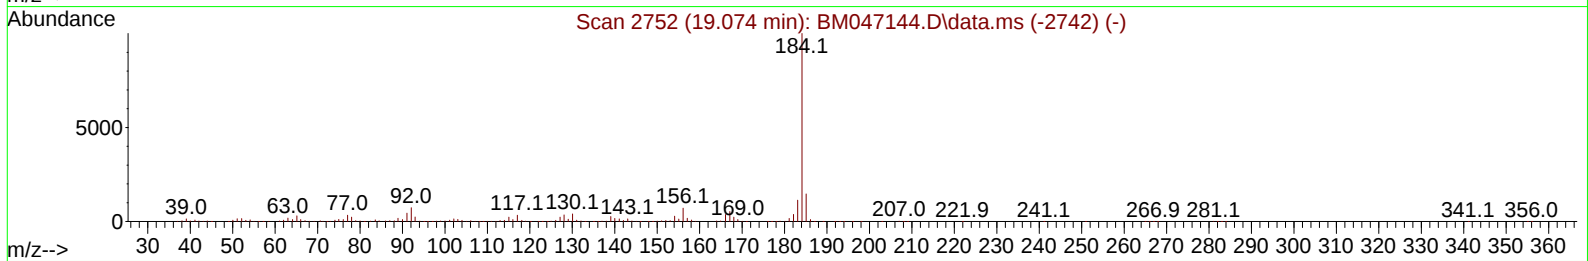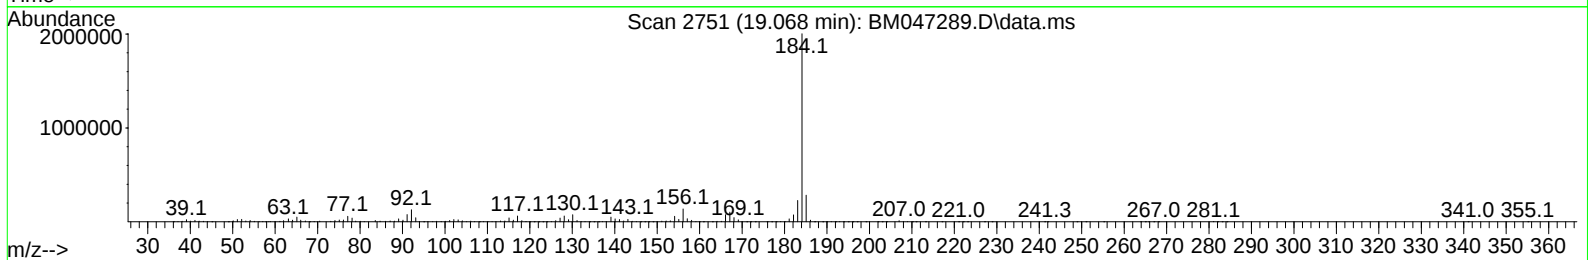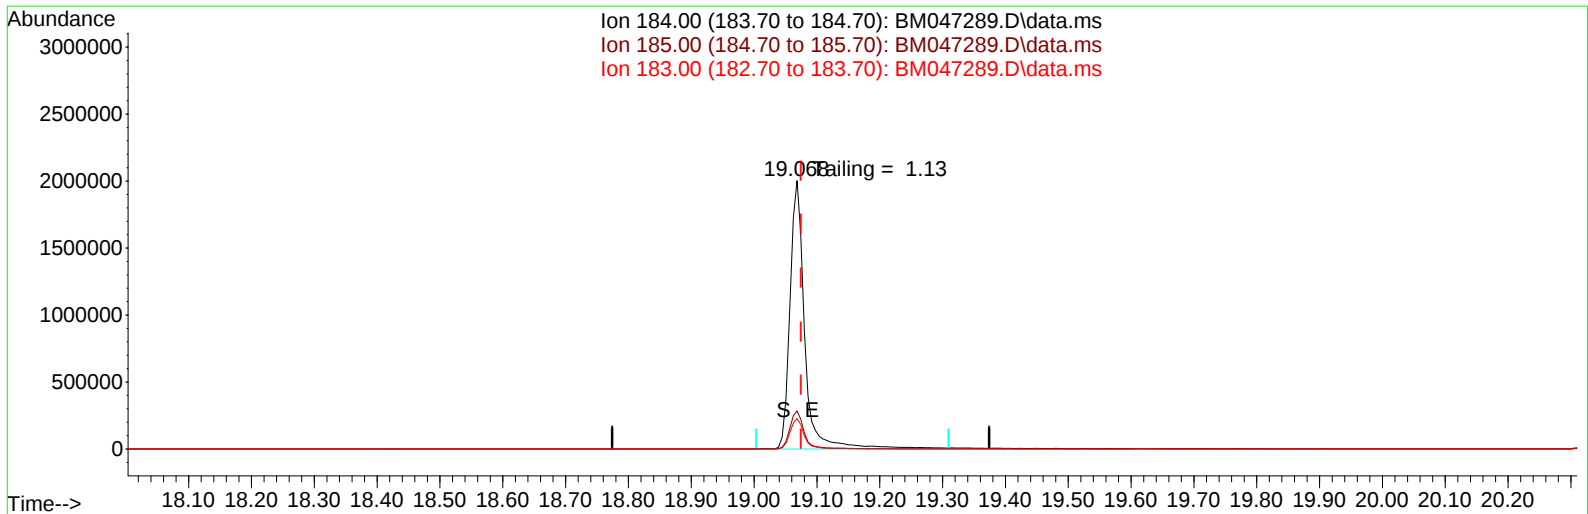

TIC: BM047289.D\data.ms

(77) Benzidine

19.068min (-0.006) 145798.11 ng

response 3298330

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.18
183.00	11.30	11.37
0.00	0.00	0.00