
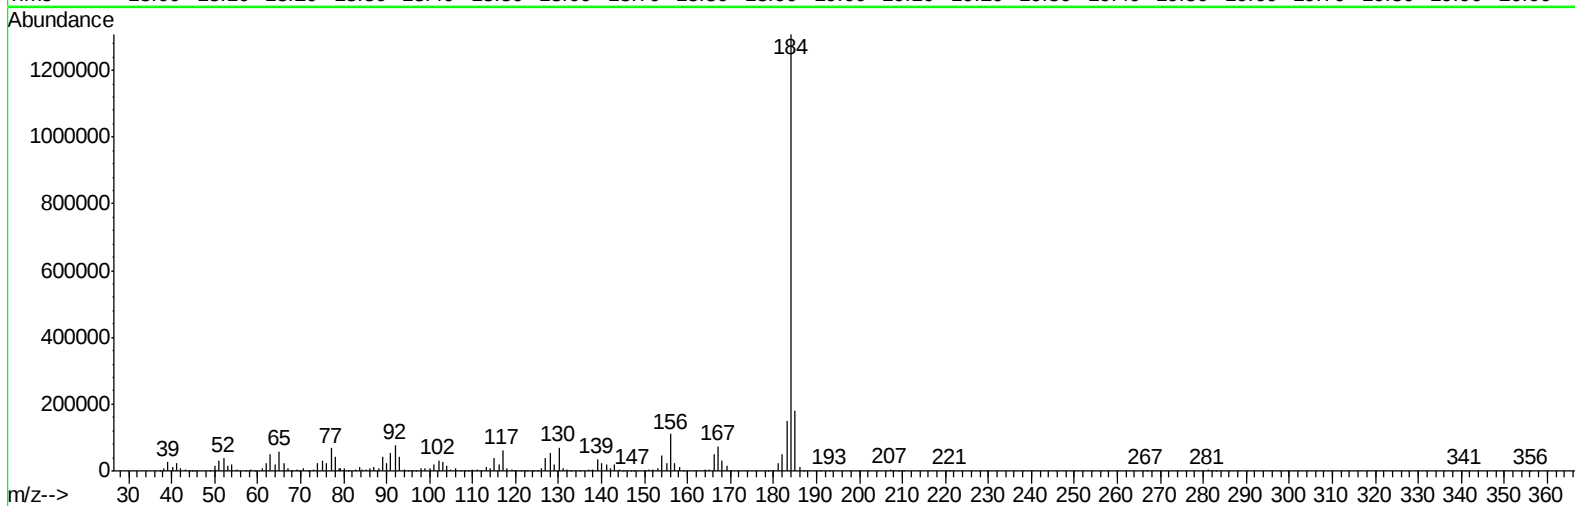


Data Path : Z:\HPCHEM1\BNA M\Data\BM082217\  
Data File : BM011326.D  
Acq On : 22 Aug 2017 14:30  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 04:18:41 2017  
Quant Method : Z:\HPCHEM1\BNA M\Methods\8270-BM072617.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 16 02:25:04 2017  
Response via : Initial Calibration

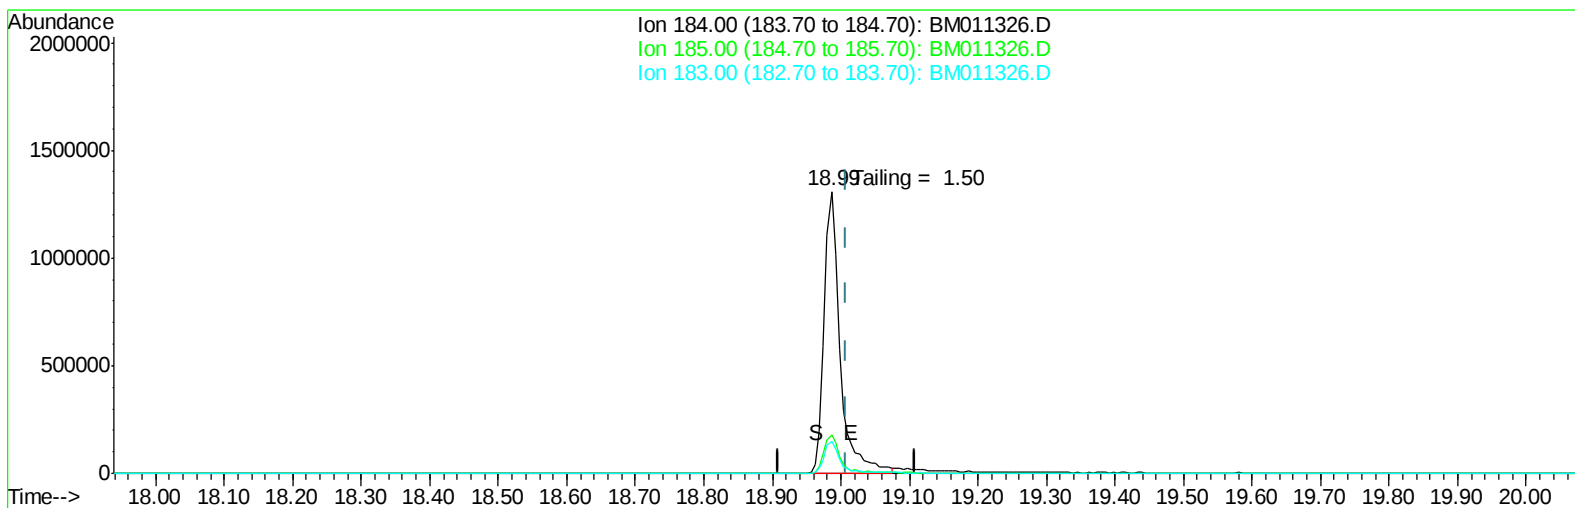

TIC: BM011326.D

(76) Benzidine



18.986min (-0.023) 5100.39ng

response 2101837

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.10 | 13.73 |
| 183.00 | 11.10 | 11.36 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA M\Data\BM082217\  
Data File : BM011326.D  
Acq On : 22 Aug 2017 14:30  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 04:18:41 2017  
Quant Method : Z:\HPCHEM1\BNA M\Methods\8270-BM072617.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 16 02:25:04 2017  
Response via : Initial Calibration

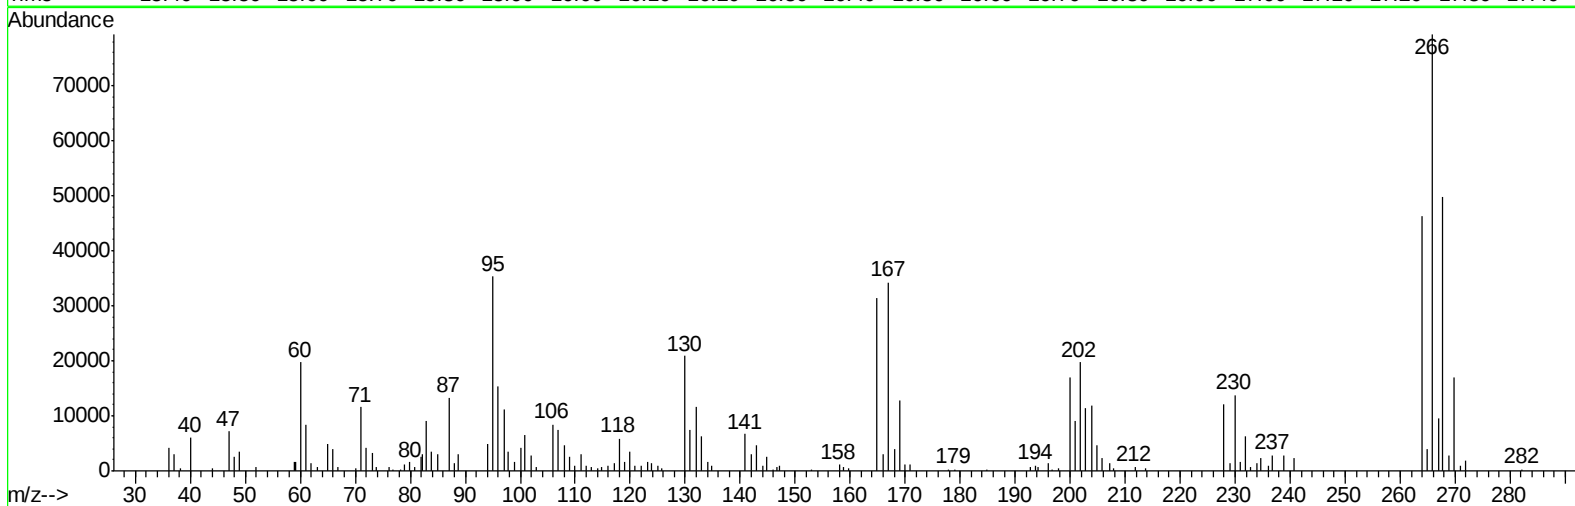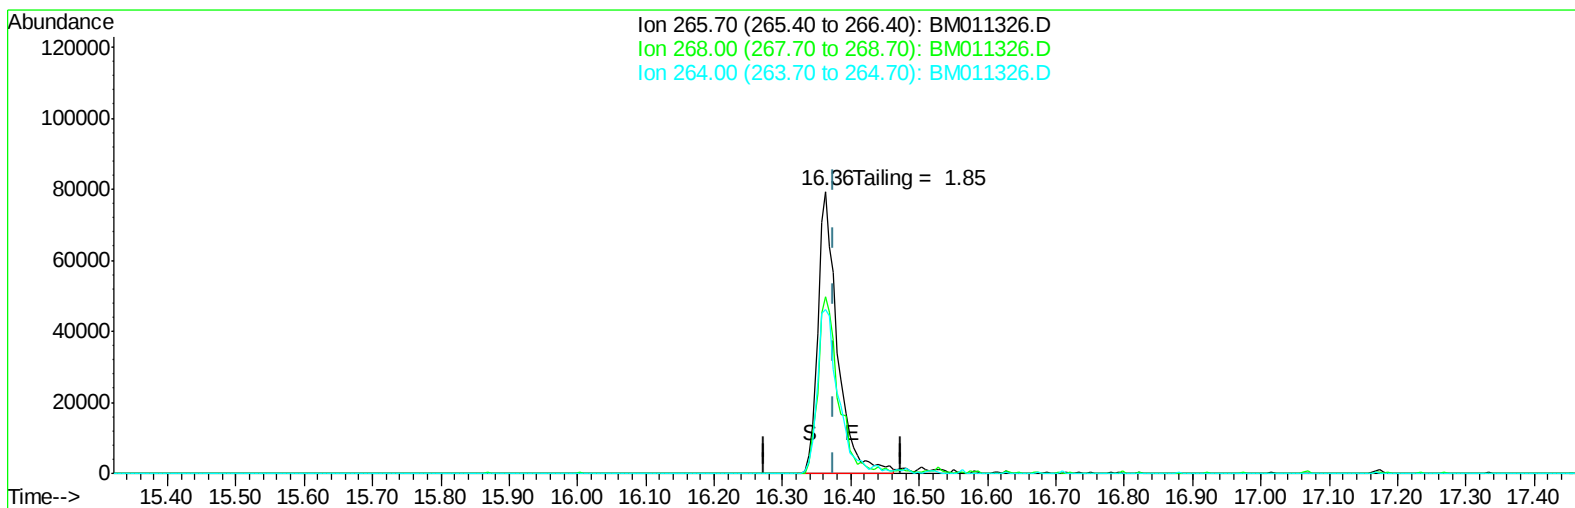

TIC: BM011326.D

(69) Pentachlorophenol (C)

16.363min (-0.012) 1587.52ng

response 159308

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 65.00 | 62.73 |
| 264.00 | 61.20 | 58.38 |
| 0.00   | 0.00  | 0.00  |