


Data Path : U:\HPCHEM1\BNA M\Data\BM082217\
 Data File : BM011326.D
 Acq On : 22 Aug 2017 14:30
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\Methods\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 16 02:25:04 2017

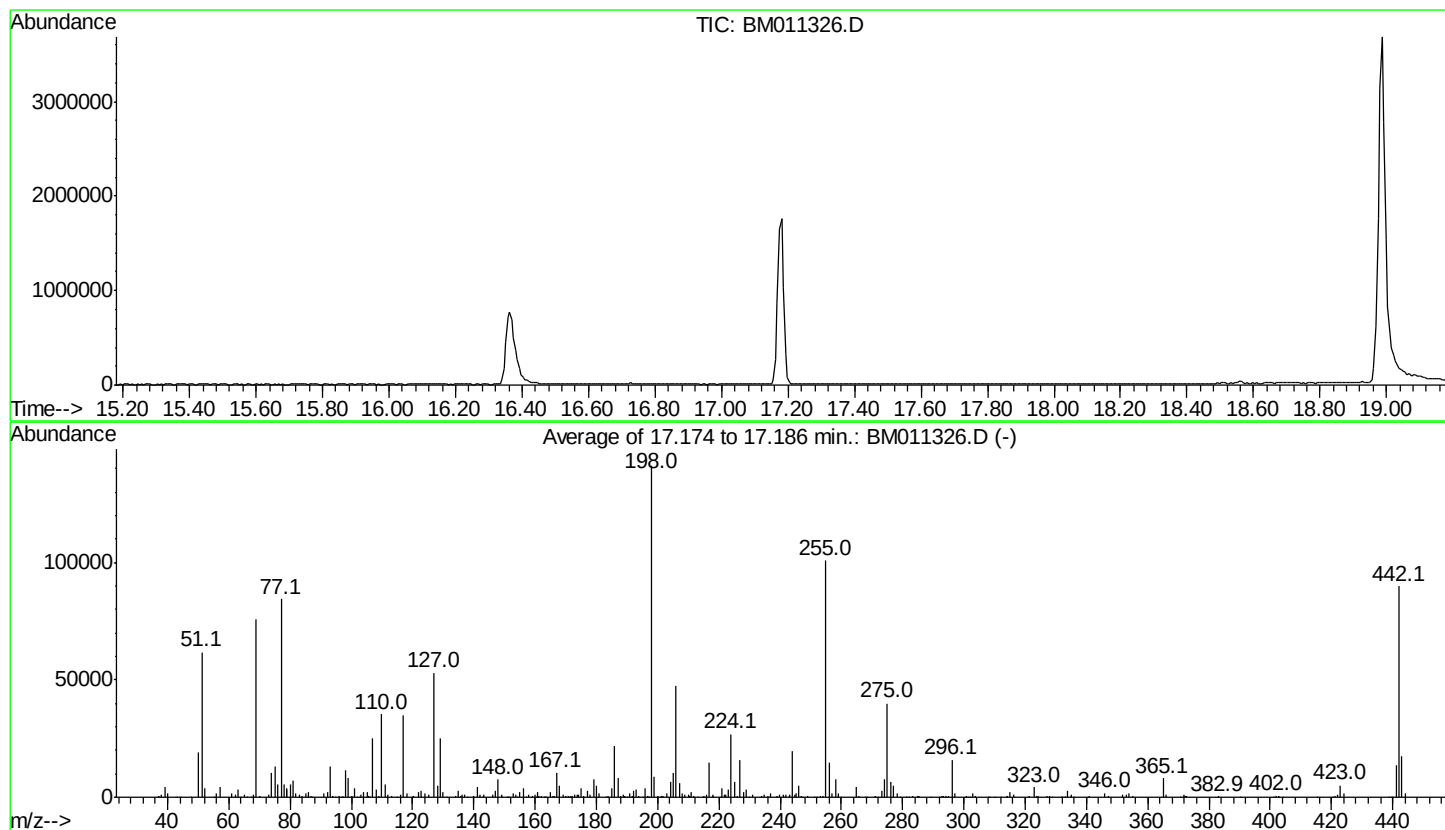

AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.7	61725	PASS
68	69	0.00	2	1.8	1366	PASS
69	198	0.00	100	53.8	75994	PASS
70	69	0.00	2	0.5	387	PASS
127	198	10	80	37.6	53218	PASS
197	198	0.00	2	0.6	802	PASS
198	198	100	100	100.0	141376	PASS
199	198	5	9	6.1	8597	PASS
275	198	10	60	28.3	40045	PASS
365	198	1	100	5.8	8136	PASS
441	442	0.01	24	15.2	13659	PASS
442	198	50	100	63.6	89968	PASS
443	442	15	24	19.3	17344	PASS