

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036369.D
 Acq On : 22 Aug 2022 16:51
 Operator : CG/JU
 Sample : PB147152BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 23 01:03:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 23 00:55:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.792	152	223290	20.000	ng/ul	0.00
20) Naphthalene-d8	10.592	136	977717	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.439	164	528143	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.180	188	909085	20.000	ng/ul	0.00
79) Chrysene-d12	21.362	240	742881	20.000	ng/ul	0.00
88) Perylene-d12	23.691	264	760512	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	35876	6.123	ng/uL	0.00
4) Pyridine-d5	3.628	84	523172	32.380	ng/ul	0.00
7) Phenol-d5	6.975	99	644895	33.836	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	441294	36.783	ng/ul	0.00
11) 2-Chlorophenol-d4	7.328	132	520480	34.756	ng/ul	0.00
15) 4-Methylphenol-d8	8.516	113	503980	35.414	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	265075	35.759	ng/ul	0.00
24) 2-Nitrophenol-d4	9.686	143	258682	34.403	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	439180	32.688	ng/ul	0.00
31) 4-Chloroaniline-d4	10.745	131	709228	34.051	ng/ul	0.00
46) Dimethylphthalate-d6	13.857	166	1269160	37.984	ng/ul	0.00
49) Acenaphthylene-d8	14.133	160	1529772	36.708	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	141485	22.348	ng/ul	0.00
60) Fluorene-d10	15.427	176	1091099	36.138	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	105702	22.616	ng/ul	0.00
73) Anthracene-d10	17.280	188	1518331	37.562	ng/ul	0.00
81) Pyrene-d10	19.574	212	1564151	40.589	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.539	264	1443166	38.704	ng/ul	0.00


Target Compounds					Qvalue	
17) N-Nitroso-di-n-propyla...	8.516	70	12747	1.119	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036369.D
Acq On : 22 Aug 2022 16:51
Operator : CG/JU
Sample : PB147152BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Aug 23 01:03:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 23 00:55:01 2022
Response via : Initial Calibration

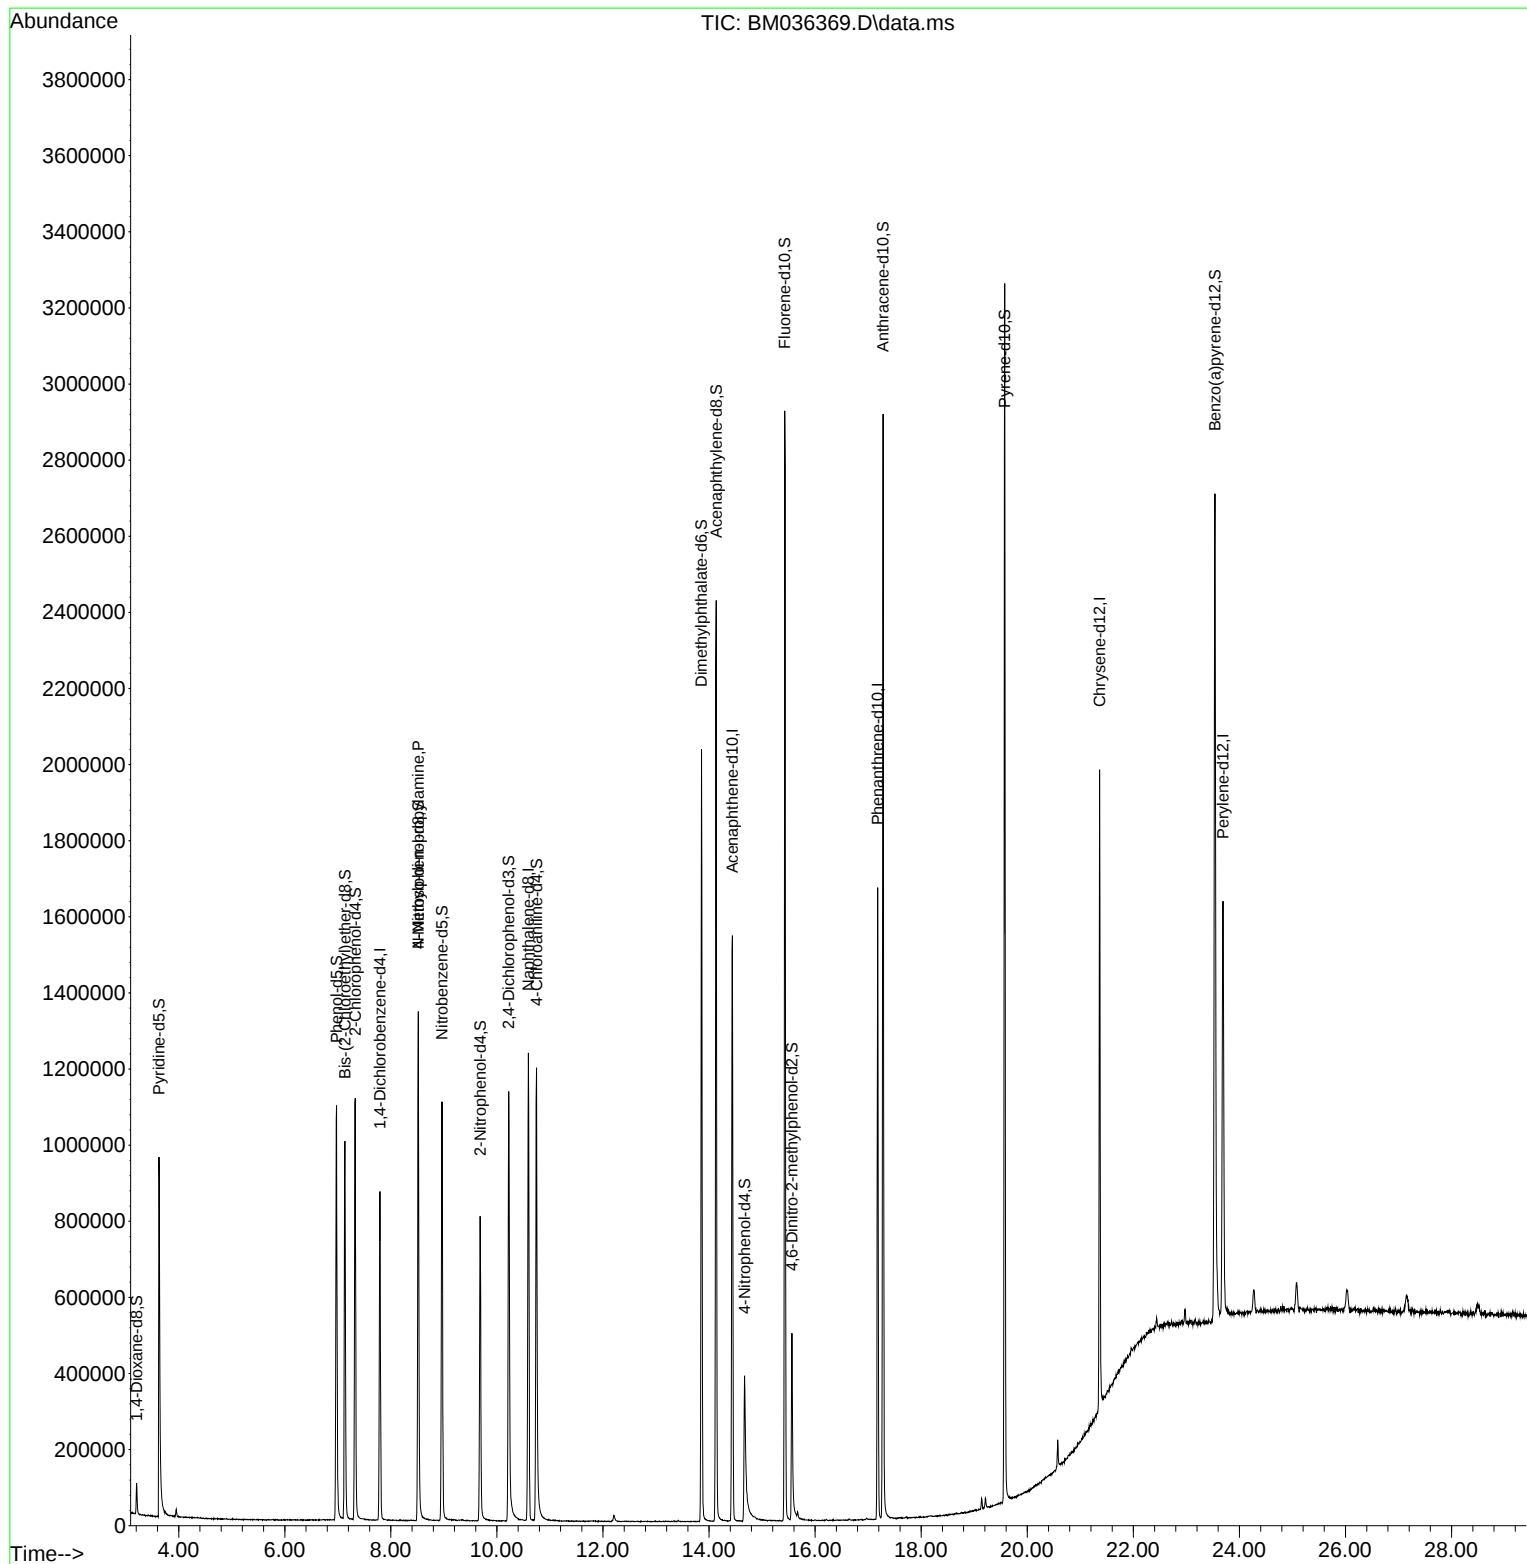

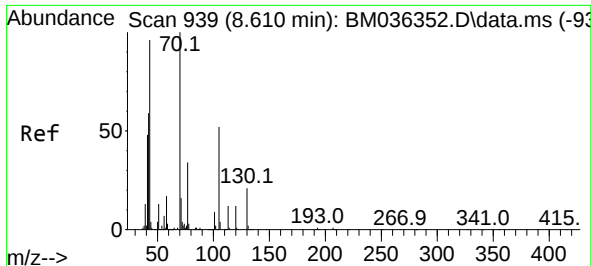

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.119 ng/ul
 RT: 8.516 min Scan# 91
 Delta R.T. -0.094 min
 Lab File: BM036369.D
 Acq: 22 Aug 2022 16:51

Instrument :
 BNA_M
 ClientSampleId :

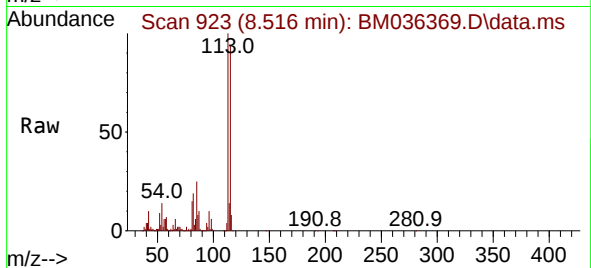

Tgt Ion: 70	Resp: 12747
Ion Ratio	Lower Upper
70	100
42	402.9 49.6 74.4#
101	0.0 8.1 12.1#
130	0.0 18.4 27.6#

