

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036374.D
 Acq On : 22 Aug 2022 19:55
 Operator : CG/JU
 Sample : N4521-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 23 01:05:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 23 00:55:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	220658	20.000	ng/u1	0.00
20) Naphthalene-d8	10.592	136	990748	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.439	164	568205	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.180	188	976077	20.000	ng/u1	0.00
79) Chrysene-d12	21.362	240	758019	20.000	ng/u1	0.00
88) Perylene-d12	23.692	264	781809	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	27617	4.770	ng/uL	0.00
4) Pyridine-d5	3.646	84	70846	4.437	ng/u1	0.02
7) Phenol-d5	6.975	99	107222	5.693	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	391928	33.058	ng/u1	0.00
11) 2-Chlorophenol-d4	7.328	132	338479	22.872	ng/u1	0.00
15) 4-Methylphenol-d8	8.516	113	215342	15.312	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	232680	30.976	ng/u1	0.00
24) 2-Nitrophenol-d4	9.681	143	215294	28.256	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	355252	26.094	ng/u1	0.00
31) 4-Chloroaniline-d4	10.745	131	332695	15.763	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	1231897	34.270	ng/u1	0.00
49) Acenaphthylene-d8	14.133	160	1446982	32.274	ng/u1	0.00
54) 4-Nitrophenol-d4	14.686	143	18280	2.684	ng/u1	0.02
60) Fluorene-d10	15.427	176	1083684	33.362	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	120476	24.008	ng/u1	0.00
73) Anthracene-d10	17.280	188	1668462	38.443	ng/u1	0.00
81) Pyrene-d10	19.574	212	1649961	41.961	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.539	264	1464974	38.218	ng/u1	0.00
Target Compounds						
59) Diethylphthalate	15.263	149	75091	2.059	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036374.D
Acq On : 22 Aug 2022 19:55
Operator : CG/JU
Sample : N4521-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Aug 23 01:05:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 23 00:55:01 2022
Response via : Initial Calibration

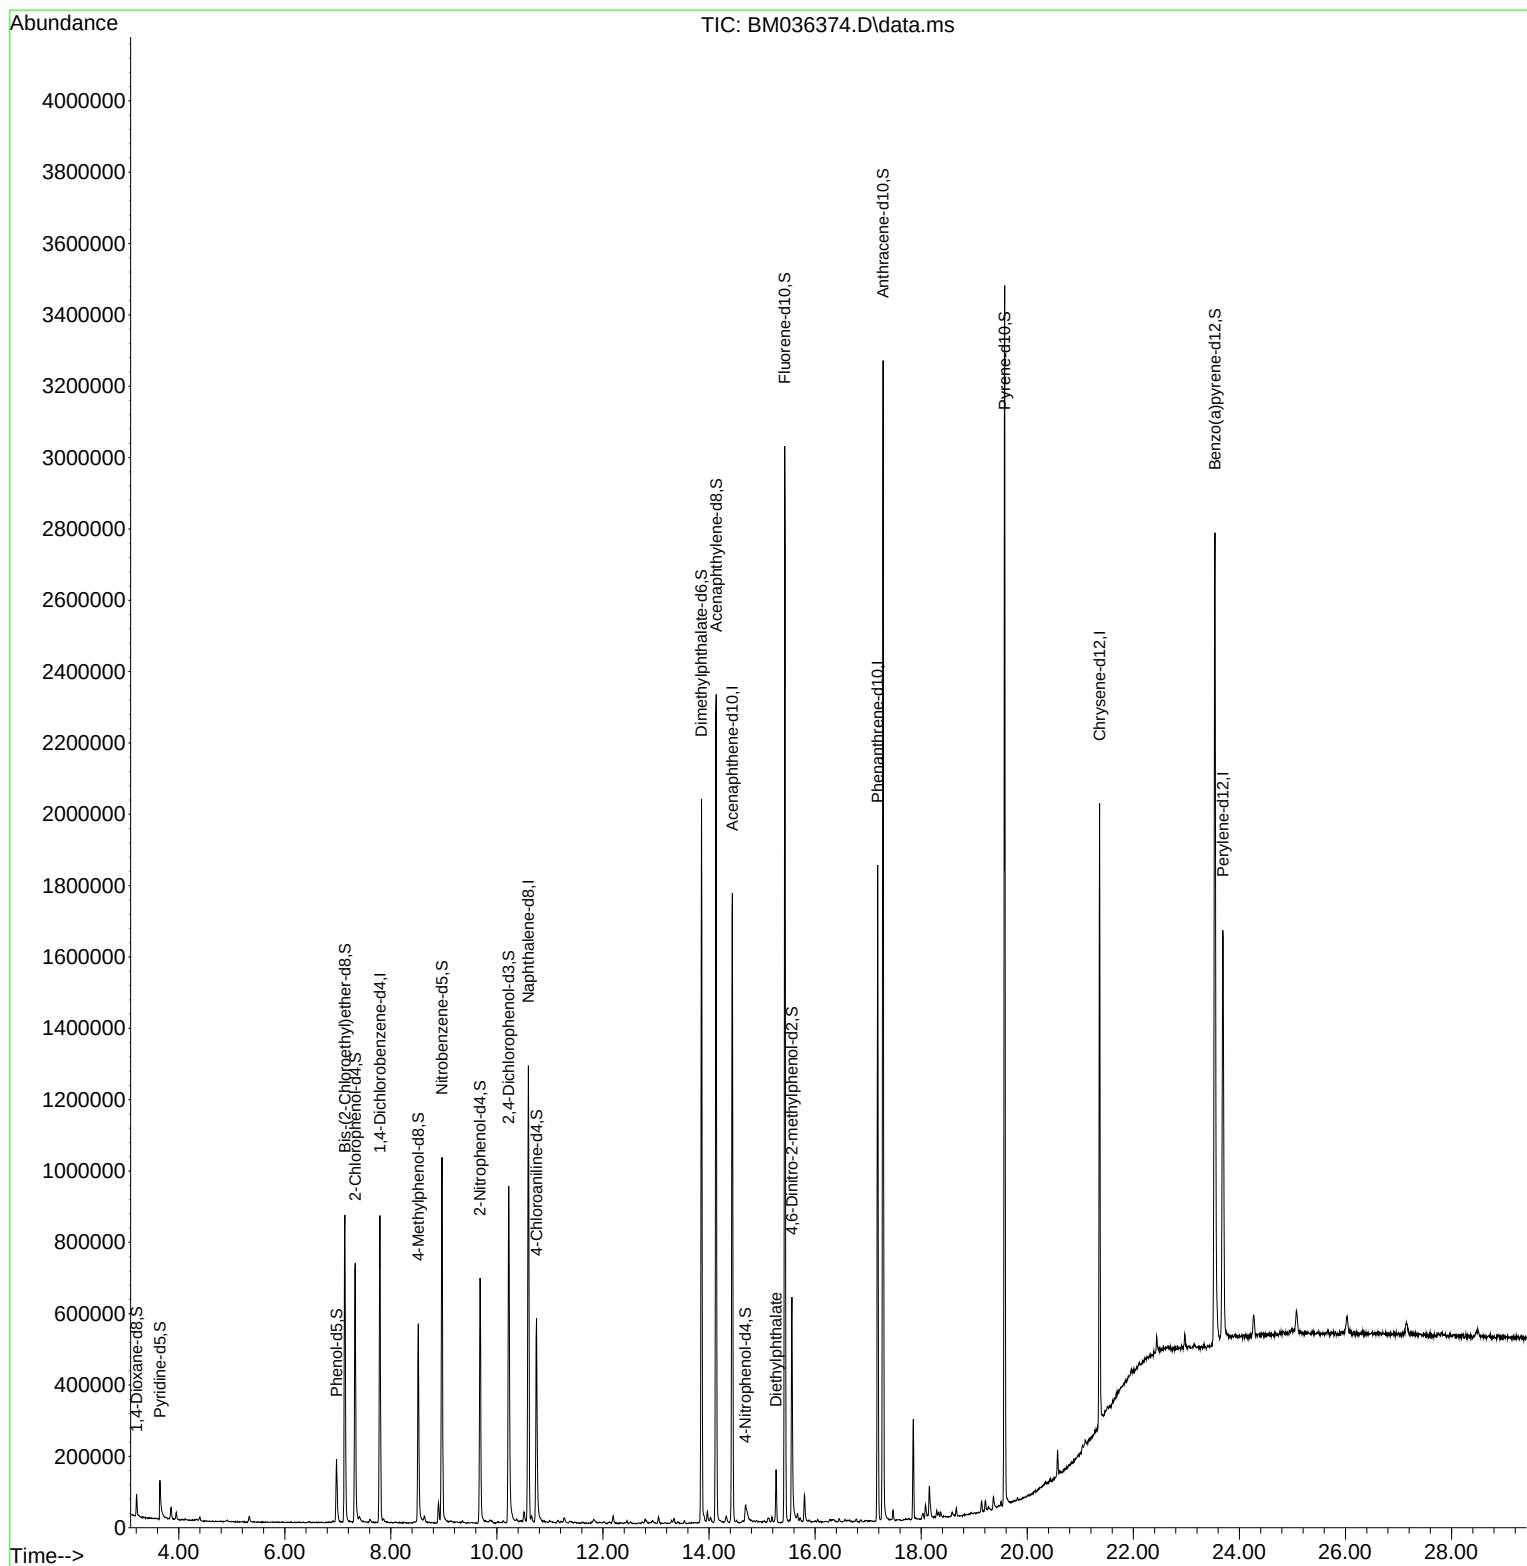

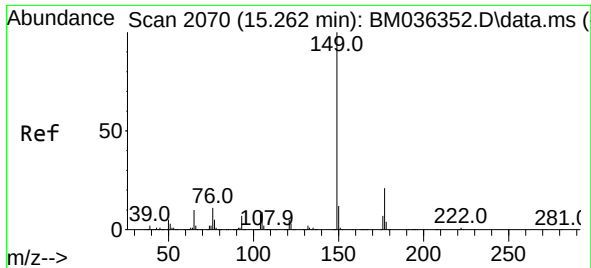

#59

Diethylphthalate

Concen: 2.059 ng/ul

RT: 15.263 min Scan# 20

Delta R.T. 0.000 min


Lab File: BM036374.D

Acq: 22 Aug 2022 19:55

Instrument :

BNA_M

ClientSampleId :

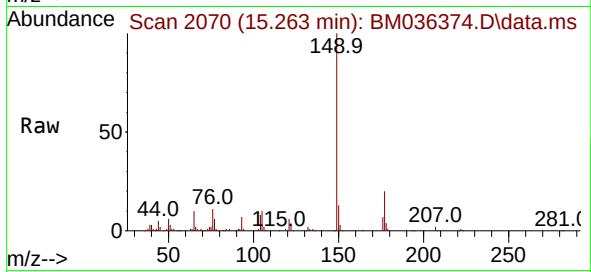

Tgt Ion:149 Resp: 75091

Ion Ratio Lower Upper

149 100

177 20.3 16.8 25.2

150 12.7 10.2 15.4

