

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036388.D
 Acq On : 23 Aug 2022 13:19
 Operator : CG/JU
 Sample : N4251-11
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 24 00:58:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 23 00:55:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	214353	20.000	ng/u1	0.00
20) Naphthalene-d8	10.592	136	982363	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.433	164	585977	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.180	188	1045462	20.000	ng/u1	0.00
79) Chrysene-d12	21.362	240	719494	20.000	ng/u1	0.00
88) Perylene-d12	23.692	264	732990	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	22873	4.067	ng/uL	0.00
4) Pyridine-d5	3.646	84	77377	4.989	ng/u1	0.02
7) Phenol-d5	6.975	99	75852	4.146	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	340697	29.582	ng/u1	0.00
11) 2-Chlorophenol-d4	7.322	132	265467	18.466	ng/u1	0.00
15) 4-Methylphenol-d8	8.516	113	156755	11.474	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	199612	26.800	ng/u1	0.00
24) 2-Nitrophenol-d4	9.681	143	172852	22.879	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	294670	21.829	ng/u1	0.00
31) 4-Chloroaniline-d4	10.745	131	435874	20.828	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	1192045	32.155	ng/u1	0.00
49) Acenaphthylene-d8	14.127	160	1325475	28.667	ng/u1	0.00
54) 4-Nitrophenol-d4	14.704	143	8031	1.143	ng/u1	0.04
60) Fluorene-d10	15.427	176	1074058	32.063	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	97042	18.055	ng/u1	0.00
73) Anthracene-d10	17.280	188	1624938	34.955	ng/u1	0.00
81) Pyrene-d10	19.574	212	1538629	41.225	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.539	264	1236169	34.397	ng/u1	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	11.922	107	15152	1.085	ng/u1	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036388.D
Acq On : 23 Aug 2022 13:19
Operator : CG/JU
Sample : N4251-11
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Aug 24 00:58:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 23 00:55:01 2022
Response via : Initial Calibration

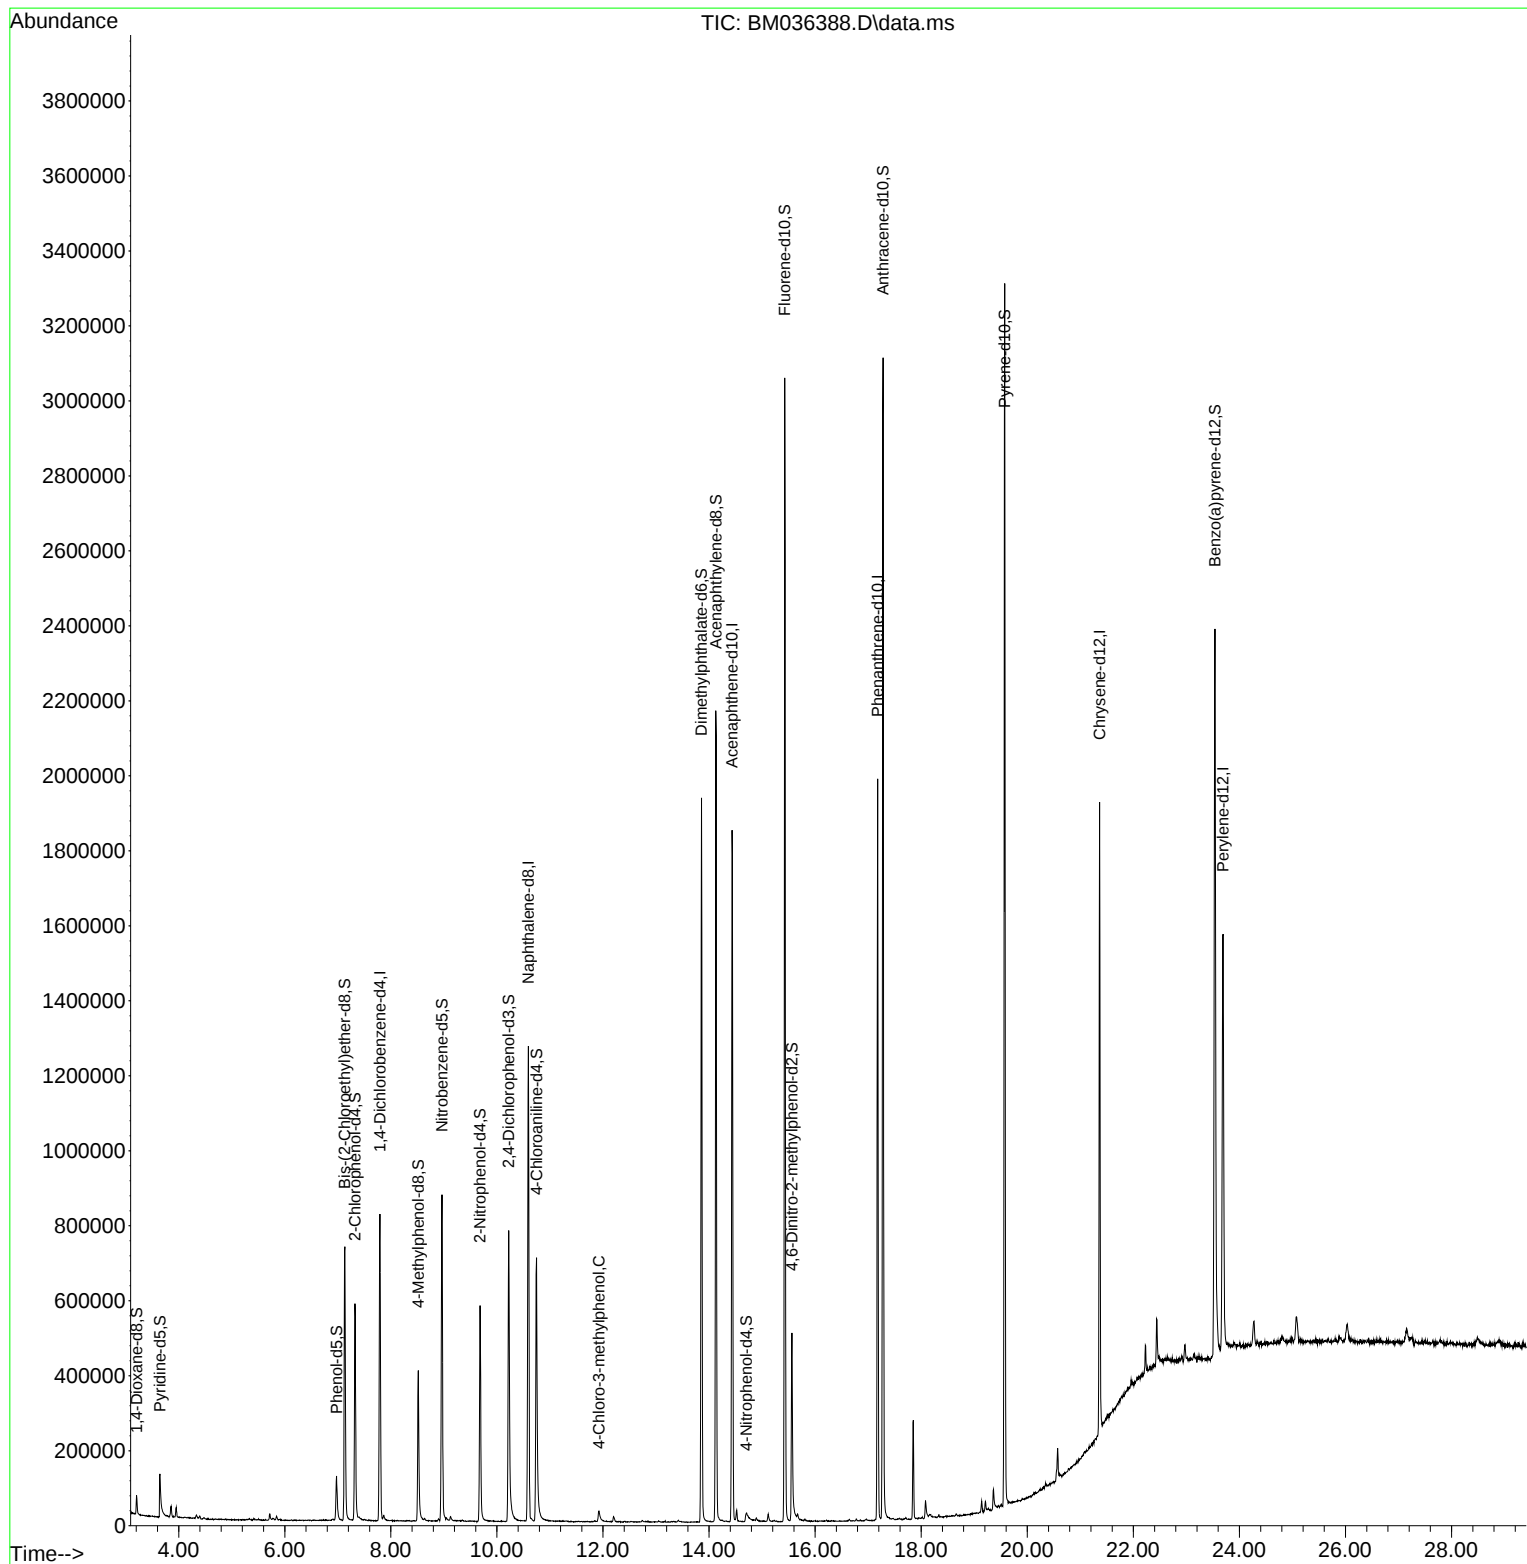

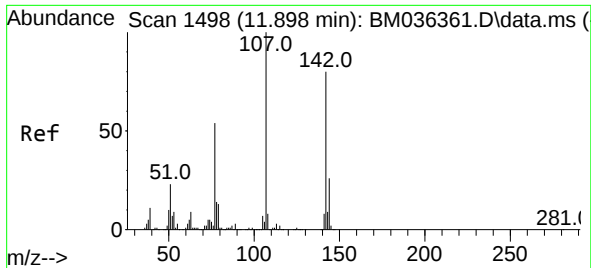

#35
 4-Chloro-3-methylphenol
 Concen: 1.085 ng/ul
 RT: 11.922 min Scan# 1
 Delta R.T. 0.024 min
 Lab File: BM036388.D
 Acq: 23 Aug 2022 13:19

Instrument :
 BNA_M
 ClientSampleId :

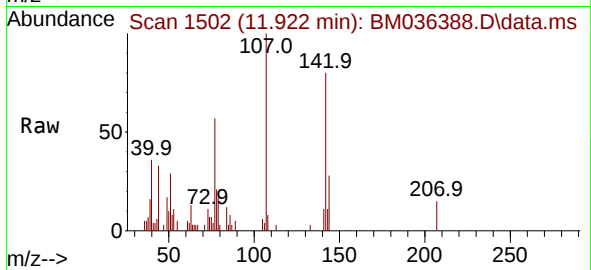

Tgt Ion:	107	Resp:	15152
Ion	Ratio	Lower	Upper
107	100		
144	27.5	20.3	30.5
142	79.7	64.4	96.6

