




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036365.D
Acq On : 22 Aug 2022 14:25
Operator : CG/JU
Sample : N4251-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN68

Manual IntegrationsAPPROVED

Quant Time: Aug 23 01:01:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 23 00:55:01 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/23/2022
Supervised By :Sohil Jodhani 08/24/2022

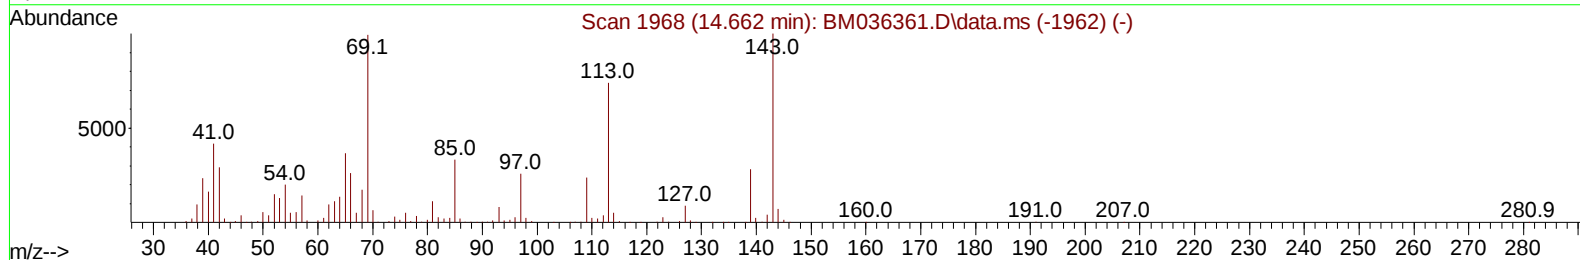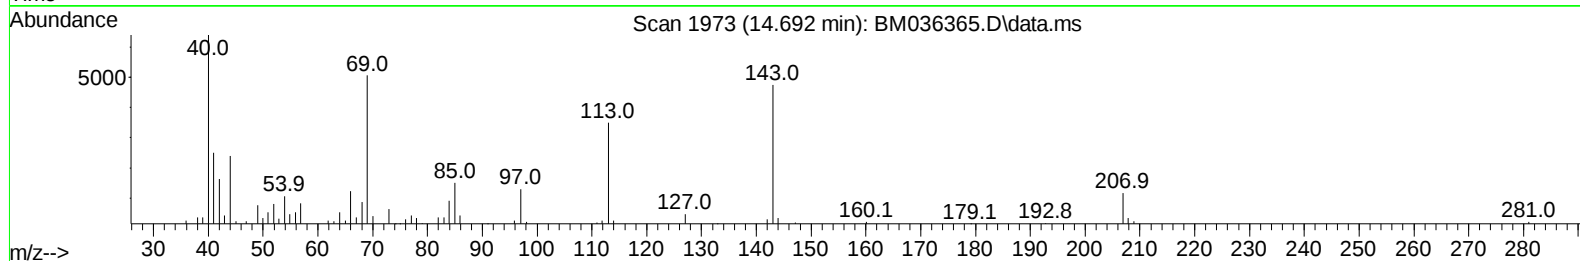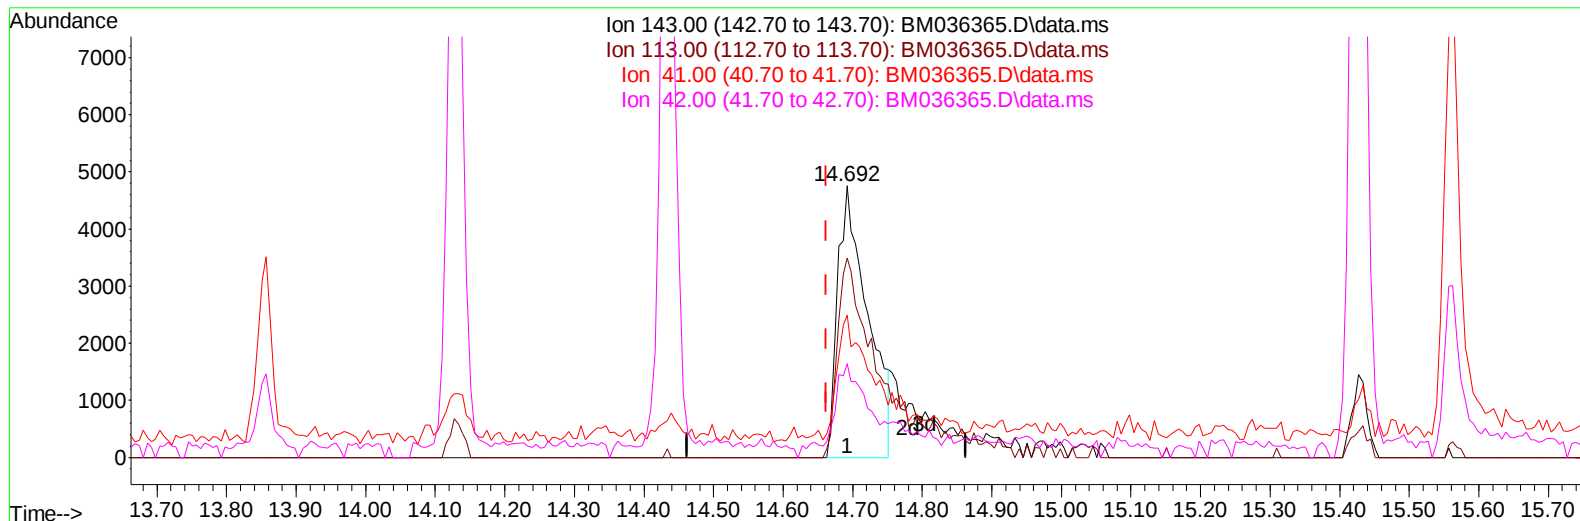

TIC: BM036365.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.692min (+ 0.030) 2.04 ng/u1

response 14218

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	61.40	73.54
41.00	41.00	52.59#
42.00	29.30	34.52




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036365.D
Acq On : 22 Aug 2022 14:25
Operator : CG/JU
Sample : N4251-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN68

Manual IntegrationsAPPROVED

Quant Time: Aug 23 01:01:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 23 00:55:01 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/23/2022
Supervised By :Sohil Jodhani 08/24/2022

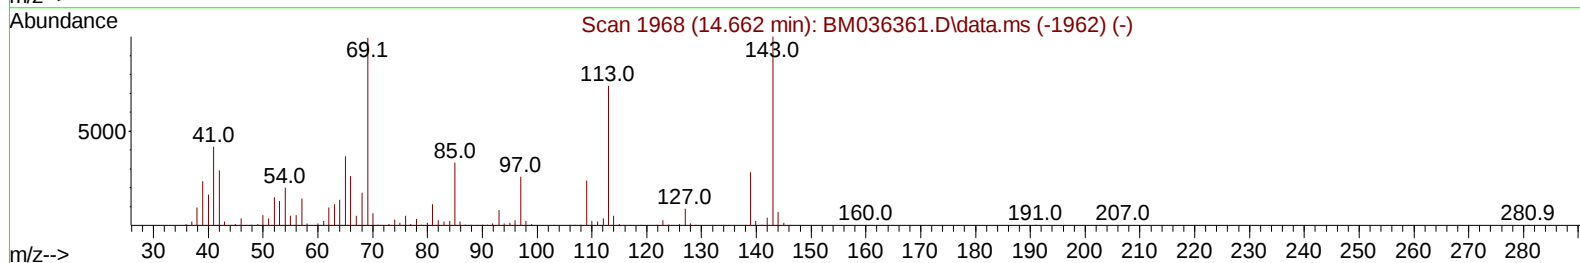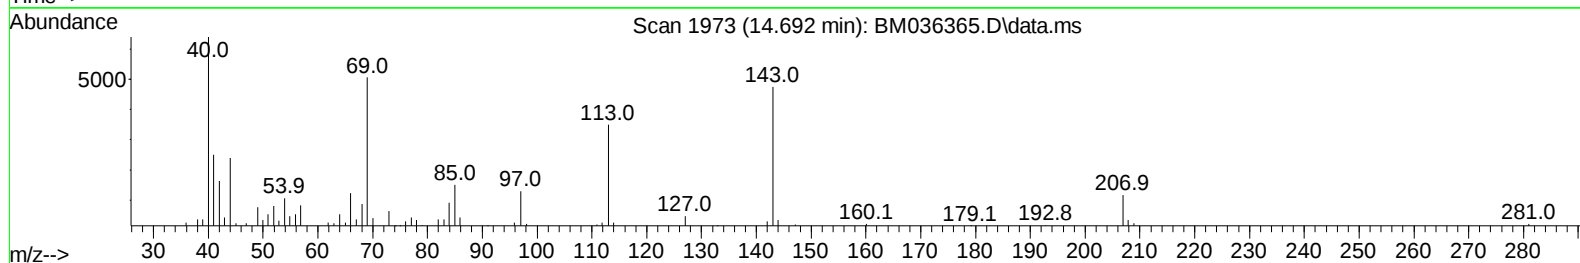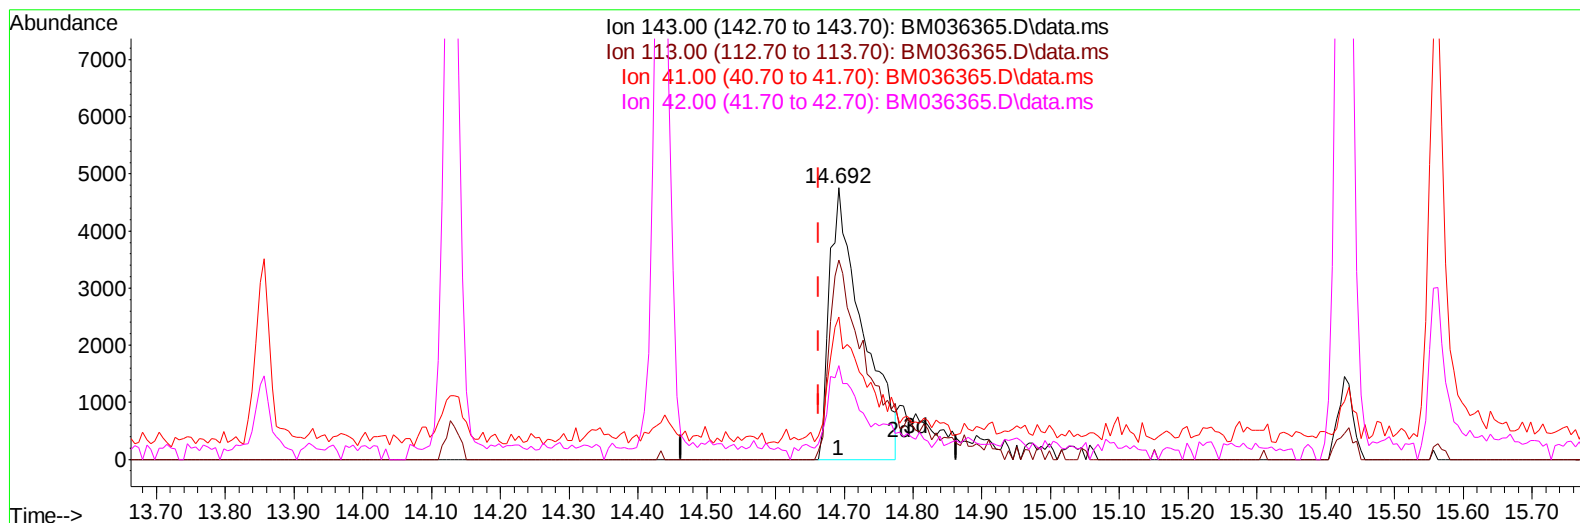

TIC: BM036365.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.692min (+ 0.030) 2.27 ng/ul m

response 15809

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	61.40	73.54
41.00	41.00	52.59#
42.00	29.30	34.52

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036365.D
 Acq On : 22 Aug 2022 14:25
 Operator : CG/JU
 Sample : N4251-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGN68

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/23/2022
 Supervised By :Sohil Jodhani 08/24/2022

Quant Time: Aug 23 01:01:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 23 00:55:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.792	152	261176	20.000	ng/ul	0.00
20) Naphthalene-d8	10.592	136	1106939	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.433	164	582116	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.180	188	1014513	20.000	ng/ul	0.00
79) Chrysene-d12	21.362	240	891753	20.000	ng/ul	0.00
88) Perylene-d12	23.691	264	965501	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	28846	4.209	ng/uL	0.00
4) Pyridine-d5	3.634	84	165153	8.739	ng/ul	0.00
7) Phenol-d5	6.975	99	110082	4.938	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	410274	29.237	ng/ul	0.00
11) 2-Chlorophenol-d4	7.328	132	348973	19.923	ng/ul	0.00
15) 4-Methylphenol-d8	8.516	113	204950	12.312	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	236129	28.135	ng/ul	0.00
24) 2-Nitrophenol-d4	9.681	143	206102	24.210	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	330969	21.758	ng/ul	0.00
31) 4-Chloroaniline-d4	10.745	131	530188	22.484	ng/ul	0.00
46) Dimethylphthalate-d6	13.857	166	1123178	30.499	ng/ul	0.00
49) Acenaphthylene-d8	14.127	160	1366890	29.759	ng/ul	0.00
54) 4-Nitrophenol-d4	14.692	143	15809m	2.266	ng/ul	0.03
60) Fluorene-d10	15.427	176	1060748	31.875	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	111336	21.346	ng/ul	0.00
73) Anthracene-d10	17.280	188	1767048	39.172	ng/ul	0.00
81) Pyrene-d10	19.574	212	1870298	40.431	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.539	264	1864779	39.393	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036365.D
Acq On : 22 Aug 2022 14:25
Operator : CG/JU
Sample : N4251-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN68

Manual IntegrationsAPPROVED

Quant Time: Aug 23 01:01:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 23 00:55:01 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/23/2022
Supervised By :Sohil Jodhani 08/24/2022

