




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036376.D
 Acq On : 22 Aug 2022 21:08
 Operator : CG/JU
 Sample : N4251-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGN90

Manual IntegrationsAPPROVED

Quant Time: Aug 23 01:06:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 23 00:55:01 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/23/2022
 Supervised By :Sohil Jodhani 08/24/2022

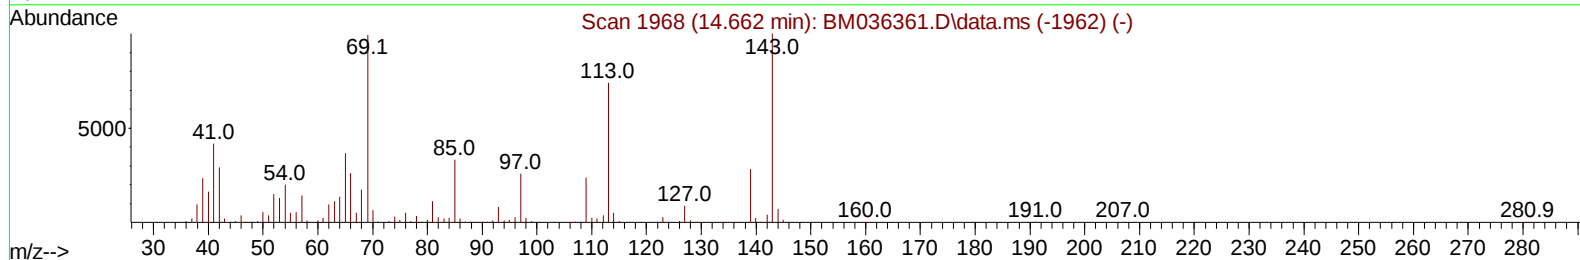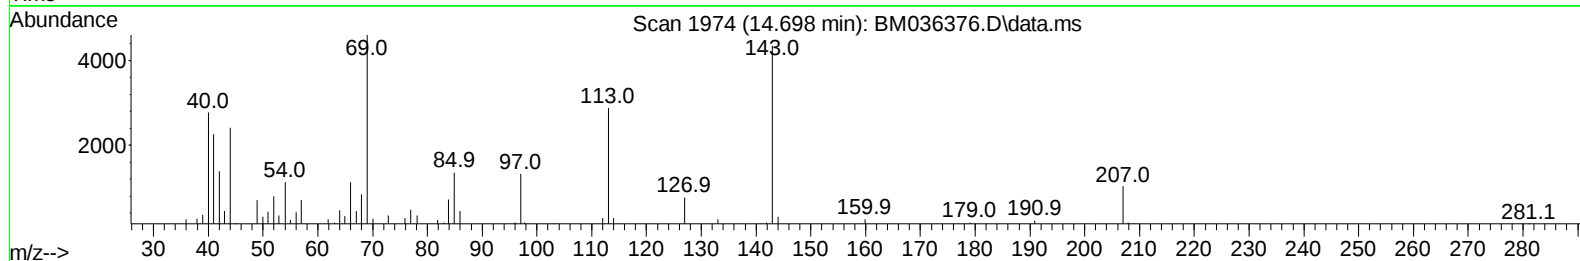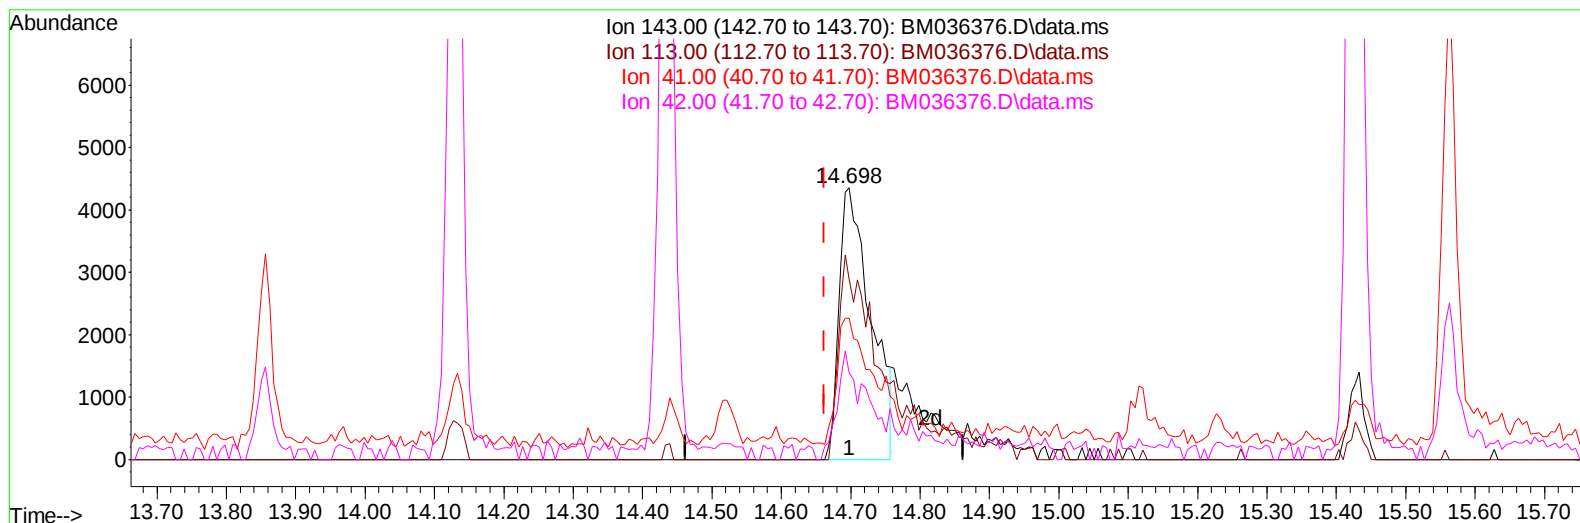

TIC: BM036376.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.698min (+ 0.035) 2.11 ng/u1

response 13759

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	61.40	66.29
41.00	41.00	51.95#
42.00	29.30	32.03




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036376.D
Acq On : 22 Aug 2022 21:08
Operator : CG/JU
Sample : N4251-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN90

Manual IntegrationsAPPROVED

Quant Time: Aug 23 01:06:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 23 00:55:01 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/23/2022
Supervised By :Sohil Jodhani 08/24/2022

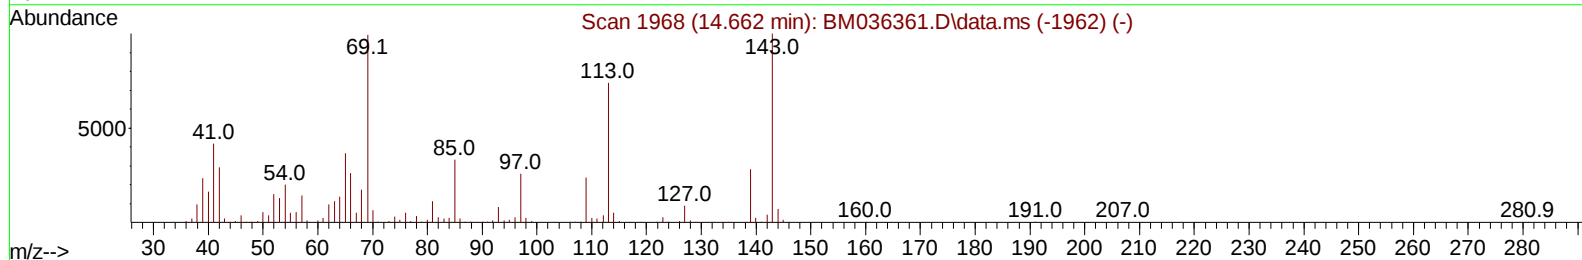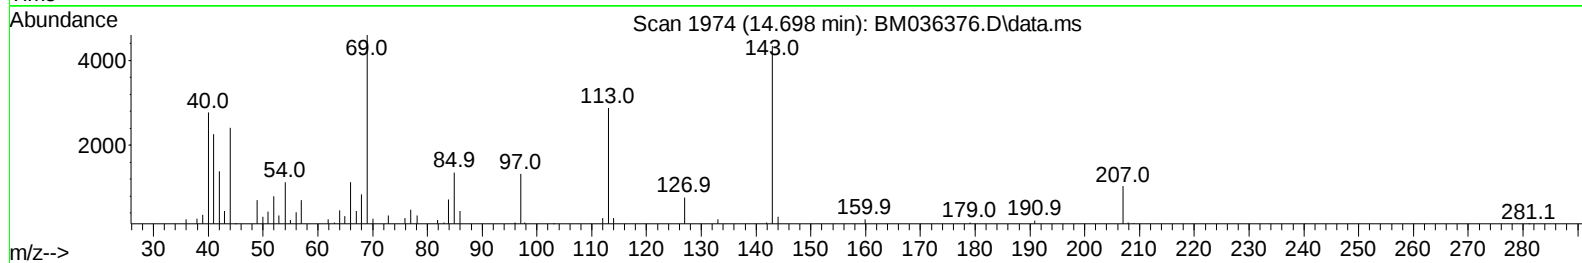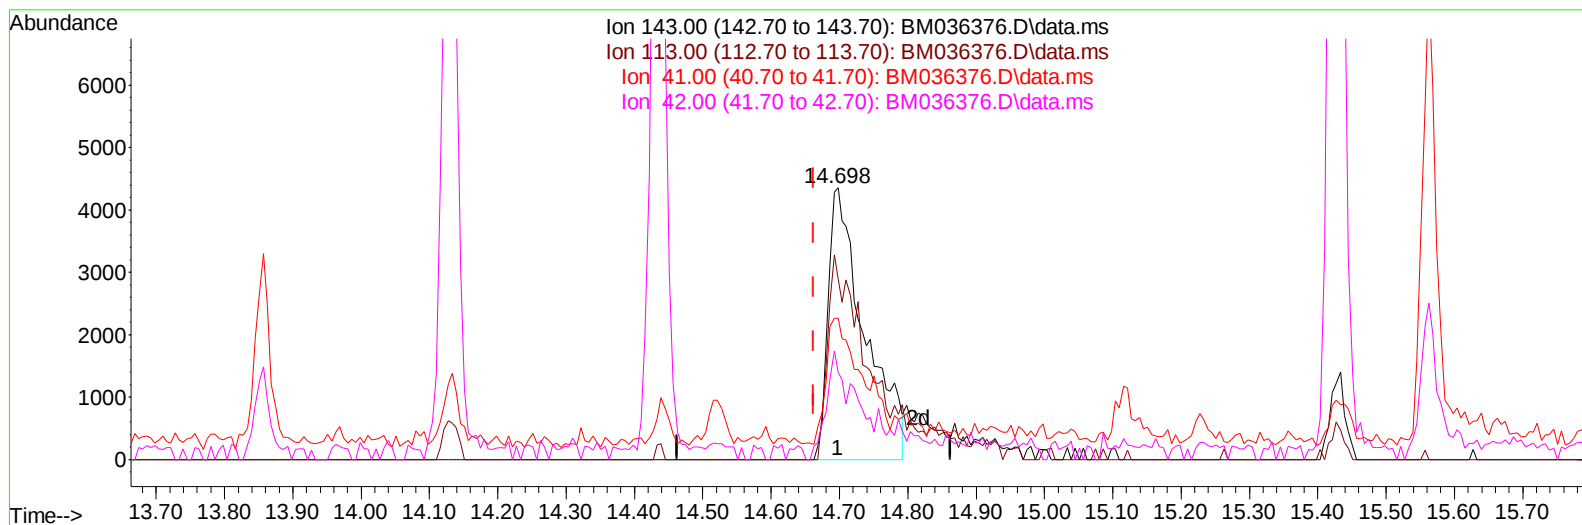

TIC: BM036376.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.698min (+ 0.035) 2.47 ng/ul m

response 16108

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	61.40	66.29
41.00	41.00	51.95#
42.00	29.30	32.03

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036376.D
 Acq On : 22 Aug 2022 21:08
 Operator : CG/JU
 Sample : N4251-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGN90

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/23/2022
 Supervised By :Sohil Jodhani 08/24/2022

Quant Time: Aug 23 01:06:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 23 00:55:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	235174	20.000	ng/ul	0.00
20) Naphthalene-d8	10.592	136	1026674	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.433	164	543154	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.180	188	915323	20.000	ng/ul	0.00
79) Chrysene-d12	21.362	240	728528	20.000	ng/ul	0.00
88) Perylene-d12	23.686	264	784254	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	30727	4.979	ng/uL	0.00
4) Pyridine-d5	3.640	84	83741	4.921	ng/ul	0.01
7) Phenol-d5	6.975	99	112556	5.607	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	407427	32.244	ng/ul	0.00
11) 2-Chlorophenol-d4	7.328	132	349898	22.184	ng/ul	0.00
15) 4-Methylphenol-d8	8.516	113	210632	14.053	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	230911	29.664	ng/ul	0.00
24) 2-Nitrophenol-d4	9.681	143	206682	26.176	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	343547	24.351	ng/ul	0.00
31) 4-Chloroaniline-d4	10.745	131	515772	23.582	ng/ul	0.00
46) Dimethylphthalate-d6	13.857	166	1109990	32.303	ng/ul	0.00
49) Acenaphthylene-d8	14.133	160	1321894	30.843	ng/ul	0.00
54) 4-Nitrophenol-d4	14.698	143	16108m	2.474	ng/ul	0.04
60) Fluorene-d10	15.427	176	979624	31.549	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	96450	20.496	ng/ul	0.00
73) Anthracene-d10	17.280	188	1592090	39.118	ng/ul	0.00
81) Pyrene-d10	19.574	212	1590842	42.095	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.539	264	1476135	38.389	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036376.D
Acq On : 22 Aug 2022 21:08
Operator : CG/JU
Sample : N4251-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN90

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/23/2022
Supervised By :Sohil Jodhani 08/24/2022

Quant Time: Aug 23 01:06:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 23 00:55:01 2022
Response via : Initial Calibration

