

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036370.D
 Acq On : 22 Aug 2022 17:28
 Operator : CG/JU
 Sample : N4231-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0KN4

Quant Time: Aug 23 01:04:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 23 00:55:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	220671	20.000	ng/u1	0.00
20) Naphthalene-d8	10.592	136	956041	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.439	164	524781	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.180	188	910760	20.000	ng/u1	0.00
79) Chrysene-d12	21.362	240	766356	20.000	ng/u1	0.00
88) Perylene-d12	23.692	264	807023	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	38920	6.722	ng/uL	0.00
4) Pyridine-d5	3.634	84	203158	12.723	ng/u1	0.00
7) Phenol-d5	6.975	99	188053	9.984	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	555786	46.876	ng/u1	0.00
11) 2-Chlorophenol-d4	7.328	132	504953	34.119	ng/u1	0.00
15) 4-Methylphenol-d8	8.516	113	339727	24.155	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	334240	46.111	ng/u1	0.00
24) 2-Nitrophenol-d4	9.687	143	319496	43.454	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	518280	39.450	ng/u1	0.00
31) 4-Chloroaniline-d4	10.745	131	752474	36.946	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	1644829	49.543	ng/u1	0.00
49) Acenaphthylene-d8	14.133	160	2066293	49.900	ng/u1	0.00
54) 4-Nitrophenol-d4	14.680	143	40639	6.460	ng/u1	0.02
60) Fluorene-d10	15.427	176	1467507	48.916	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	168572	36.002	ng/u1	0.00
73) Anthracene-d10	17.280	188	2077336	51.296	ng/u1	0.00
81) Pyrene-d10	19.574	212	2166828	54.506	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.539	264	2050088	51.812	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.240	88	703499	115.352	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036370.D
Acq On : 22 Aug 2022 17:28
Operator : CG/JU
Sample : N4231-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KN4

Quant Time: Aug 23 01:04:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 23 00:55:01 2022
Response via : Initial Calibration

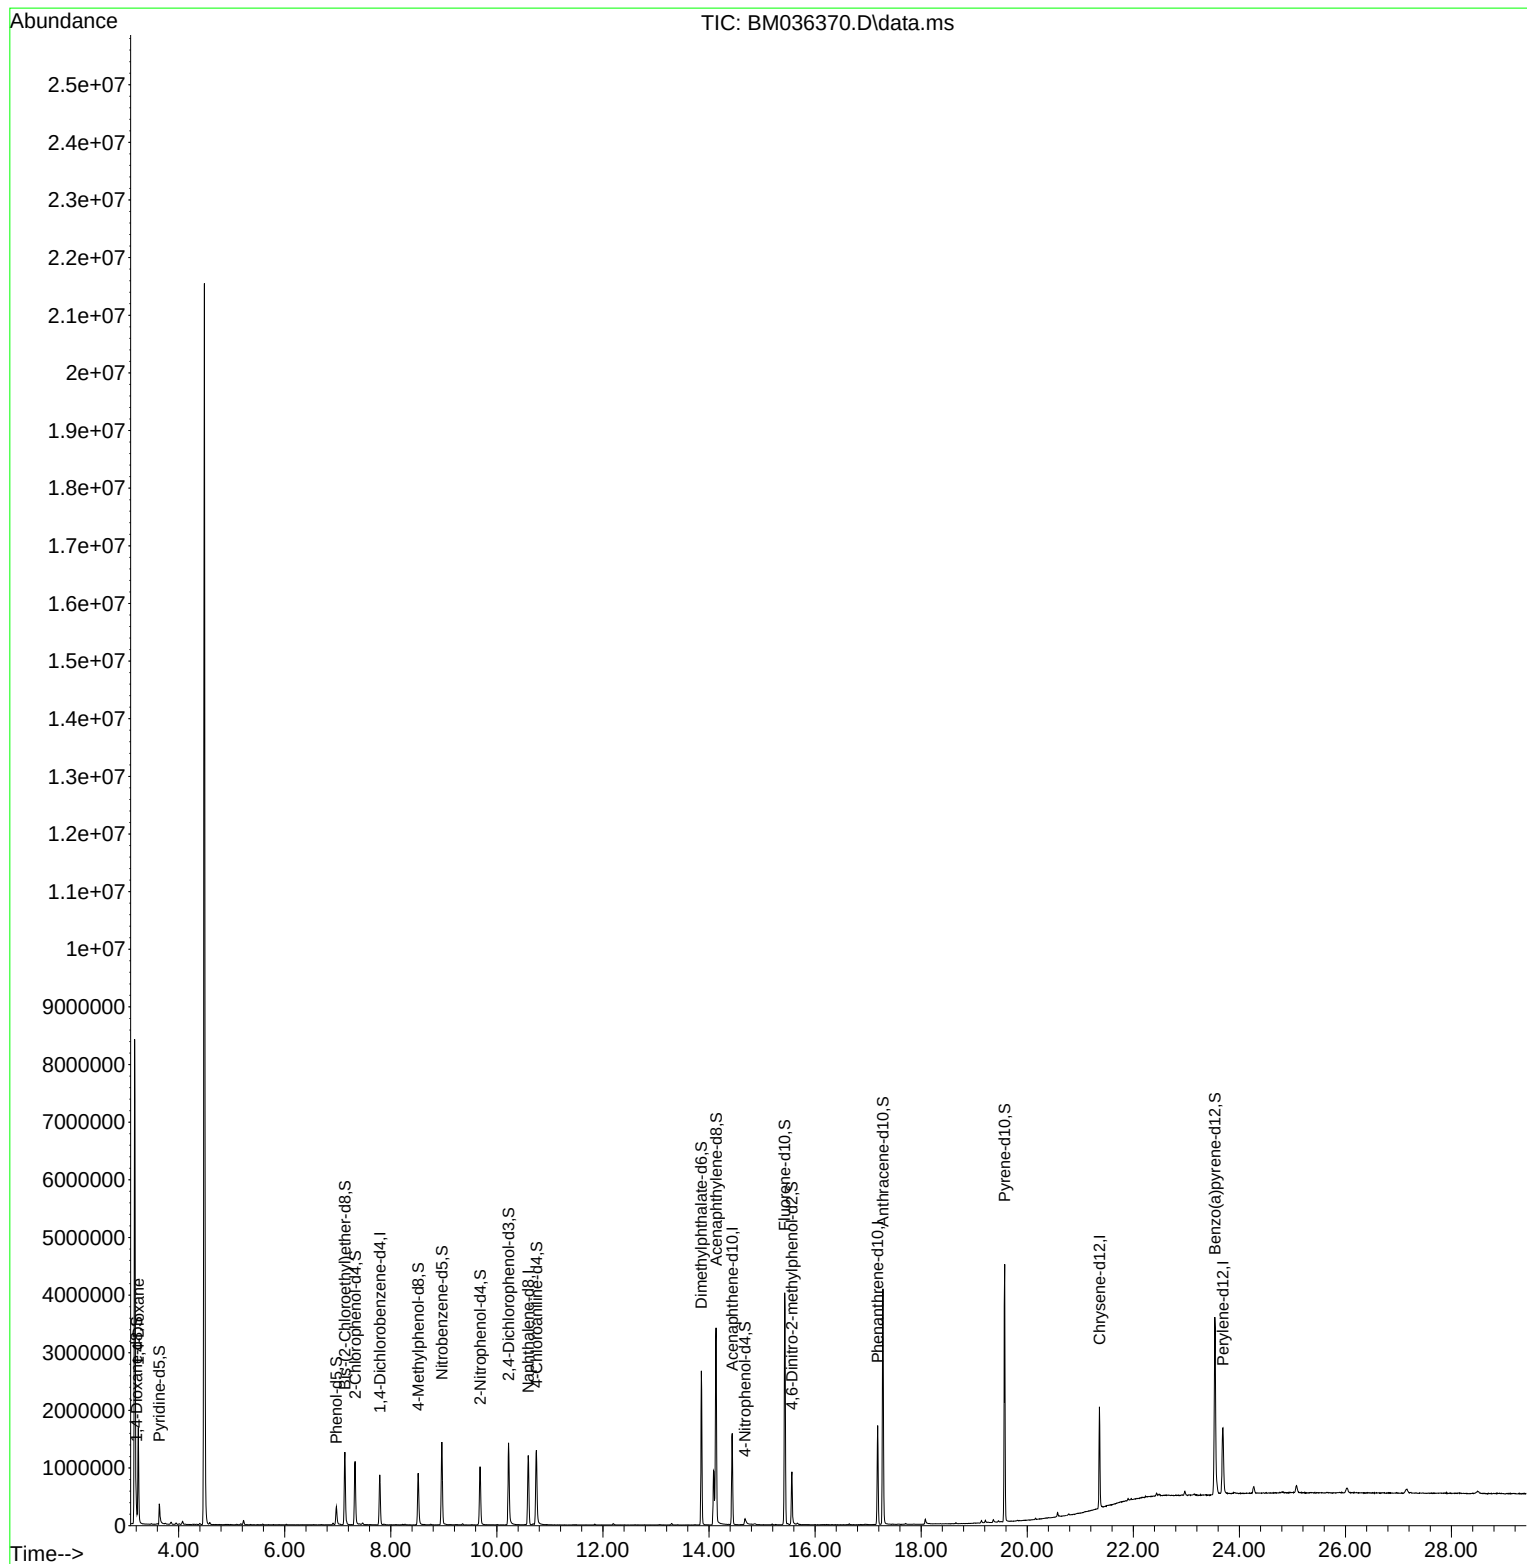

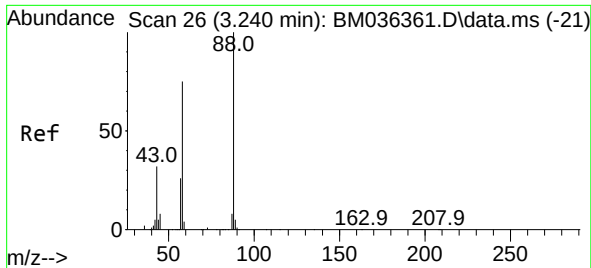

#2
 1,4-Dioxane
 Concen: 115.352 ng/uL
 RT: 3.240 min Scan# 20
 Delta R.T. 0.000 min
 Lab File: BM036370.D
 Acq: 22 Aug 2022 17:28

Instrument :
 BNA_M
 ClientSampleId :
 C0KN4

Tgt Ion: 88 Resp: 703499

Ion	Ratio	Lower	Upper
88	100		
43	31.4	27.8	41.8
58	74.8	61.8	92.8

