

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036362.D
 Acq On : 22 Aug 2022 12:36
 Operator : CG/JU
 Sample : PB147153BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK153

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036362.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	28	rBV	79968	98650	2.59%	0.195%
2	3.628	89	92	115	rBV	931055	1468287	38.56%	2.896%
3	3.952	144	147	152	rVB	19436	28499	0.75%	0.056%
4	4.640	262	264	266	rVB2	4778	3917	0.10%	0.008%
5	5.828	464	466	470	rVB	4423	3963	0.10%	0.008%
6	6.969	654	660	676	rBV	1029697	1730266	45.44%	3.413%
7	7.134	681	688	698	rVV	954306	1466379	38.51%	2.892%
8	7.322	714	720	734	rBV	1060415	1703145	44.73%	3.359%
9	7.793	793	800	809	rBV	916308	1429924	37.55%	2.820%
10	7.928	821	823	828	rVB5	3151	3887	0.10%	0.008%
11	8.110	852	854	858	rVB3	3808	5248	0.14%	0.010%
12	8.375	895	899	902	rBV5	2462	4528	0.12%	0.009%
13	8.516	916	923	938	rBV	1234787	2057065	54.02%	4.057%
14	8.963	992	999	1014	rBV	1026347	1716050	45.07%	3.384%
15	9.681	1114	1121	1136	rBV	717081	1227278	32.23%	2.421%
16	9.899	1155	1158	1160	rBV	5209	4066	0.11%	0.008%
17	10.222	1205	1213	1235	rBV	1029101	1874758	49.24%	3.698%
18	10.593	1268	1276	1289	rVB	1279315	2112973	55.49%	4.167%
19	10.746	1293	1302	1321	rBV	1083075	2142770	56.27%	4.226%
20	12.204	1543	1550	1558	rBV4	16302	38006	1.00%	0.075%
21	12.398	1580	1583	1586	rBV5	2754	3858	0.10%	0.008%
22	13.416	1752	1756	1760	rVB7	4136	6163	0.16%	0.012%
23	13.857	1824	1831	1844	rBV	1787801	2495815	65.55%	4.922%
24	13.957	1847	1848	1853	rVB4	3916	4326	0.11%	0.009%
25	14.128	1869	1877	1891	rBV	2266733	3291260	86.44%	6.491%
26	14.228	1893	1894	1899	rVV3	6282	9729	0.26%	0.019%
27	14.286	1901	1904	1907	rVB2	3417	4054	0.11%	0.008%
28	14.434	1922	1929	1942	rBV	1625962	2393486	62.86%	4.721%
29	14.669	1962	1969	1991	rBV	272739	752304	19.76%	1.484%
30	15.428	2092	2098	2115	rBV	2757430	3755285	98.62%	7.406%
31	15.563	2115	2121	2135	rBV	338248	592495	15.56%	1.169%
32	15.663	2135	2138	2145	rVB6	13654	25777	0.68%	0.051%
33	15.939	2180	2185	2188	rBV5	2127	4372	0.11%	0.009%
34	16.786	2325	2329	2332	rVB3	3412	4036	0.11%	0.008%
35	16.857	2339	2341	2346	rBV4	4394	5278	0.14%	0.010%
36	16.957	2355	2358	2363	rBV3	4488	7924	0.21%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036362.D
 Acq On : 22 Aug 2022 12:36
 Operator : CG/JU
 Sample : PB147153BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK153

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

37	17.039	2369	2372	2375	rBV2	3171	4066	0.11%	0.008%
38	17.180	2389	2396	2405	rBV	1680210	2310734	60.68%	4.557%
39	17.280	2406	2413	2425	rVV	2473794	3602415	94.61%	7.105%
40	17.963	2526	2529	2533	rBV3	3795	5151	0.14%	0.010%
41	18.421	2604	2607	2609	rBV4	3116	3847	0.10%	0.008%
42	19.063	2714	2716	2718	rBV3	5578	5806	0.15%	0.011%
43	19.139	2725	2729	2735	rBV3	27154	38658	1.02%	0.076%
44	19.210	2738	2741	2746	rVV2	19819	28719	0.75%	0.057%
45	19.574	2797	2803	2817	rBV	2789999	3776946	99.19%	7.449%
46	20.574	2970	2973	2979	rBV3	57734	83354	2.19%	0.164%
47	21.362	3102	3107	3117	rBV	1649089	2259767	59.35%	4.457%
48	23.539	3471	3477	3494	rVB2	2017626	3807767	100.00%	7.510%
49	23.692	3497	3503	3515	rVB2	1158629	2300302	60.41%	4.537%




Sum of corrected areas: 50703353

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036362.D
Acq On : 22 Aug 2022 12:36
Operator : CG/JU
Sample : PB147153BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK153

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

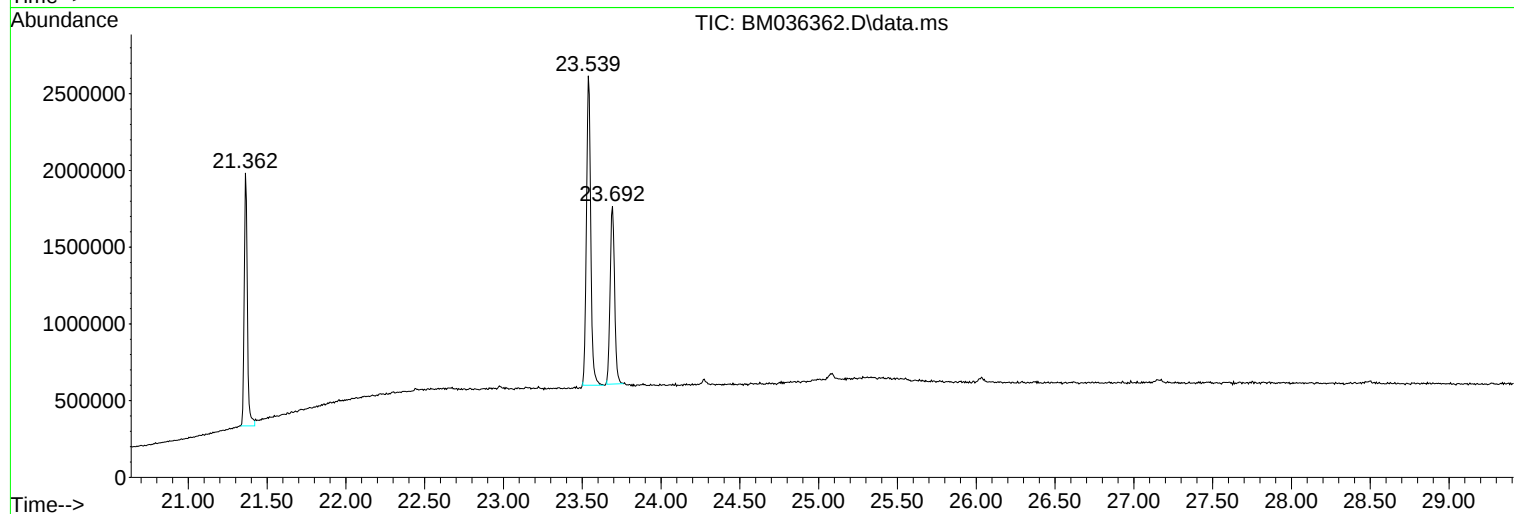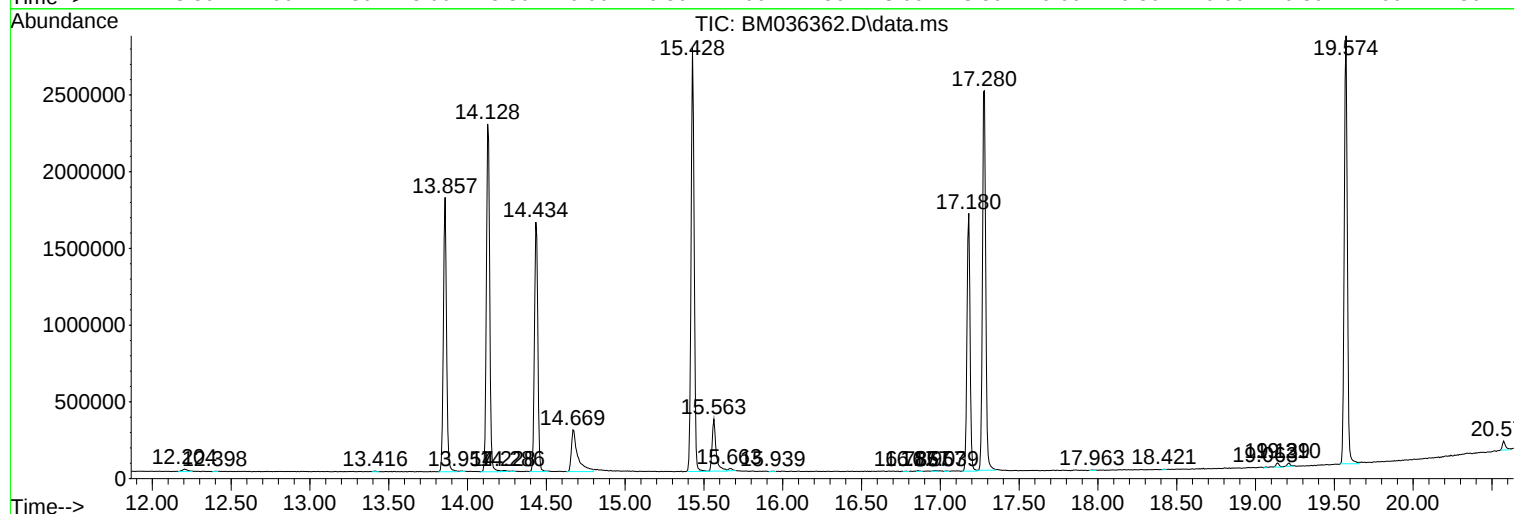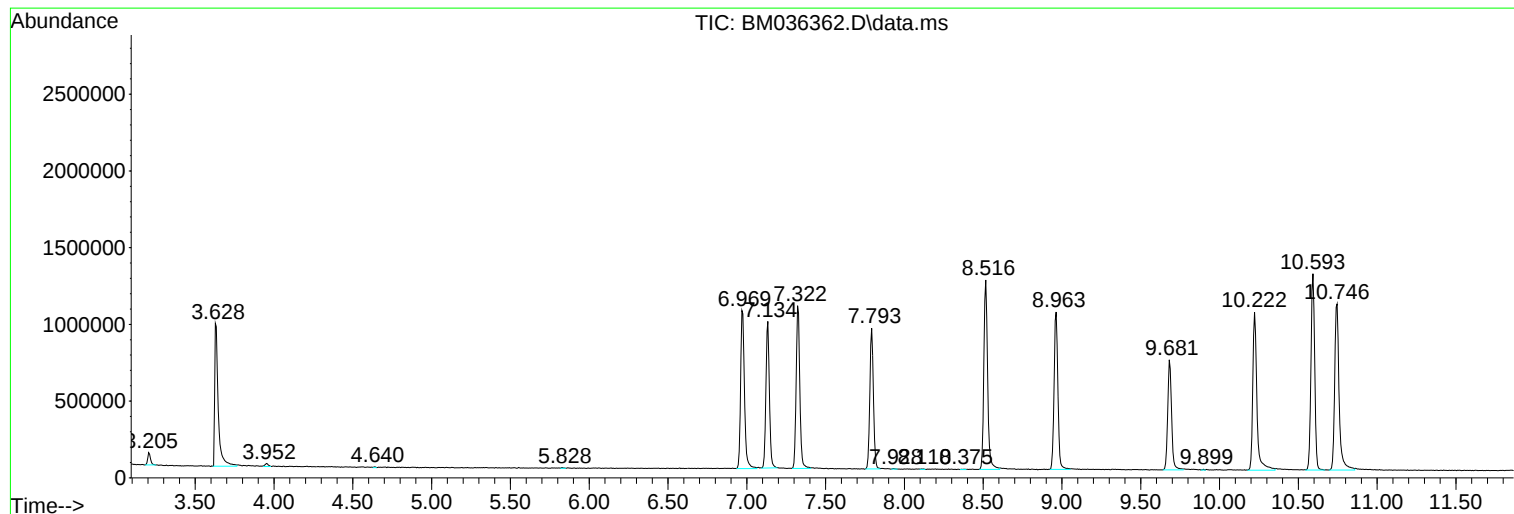

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036362.D
Acq On : 22 Aug 2022 12:36
Operator : CG/JU
Sample : PB147153BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK153

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036362.D
Acq On : 22 Aug 2022 12:36
Operator : CG/JU
Sample : PB147153BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK153

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc