

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036363.D
 Acq On : 22 Aug 2022 13:13
 Operator : CG/JU
 Sample : N4251-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGN66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	17	20	27	rVB	56914	69425	1.36%	0.146%
2	3.634	90	93	116	rBV	296866	512572	10.06%	1.079%
3	3.858	126	131	138	rVB	35678	48579	0.95%	0.102%
4	3.952	144	147	153	rVB2	17885	22209	0.44%	0.047%
5	4.340	211	213	216	rVB	6621	5588	0.11%	0.012%
6	4.399	220	223	226	rVB	10551	10368	0.20%	0.022%
7	6.975	655	661	673	rBV	181052	323986	6.36%	0.682%
8	7.134	681	688	700	rBV	902747	1440301	28.26%	3.032%
9	7.322	714	720	731	rBV	756630	1236693	24.26%	2.603%
10	7.622	767	771	775	rVB3	3776	5579	0.11%	0.012%
11	7.793	792	800	810	rBV	814942	1282179	25.16%	2.699%
12	8.516	916	923	941	rBV	543961	940572	18.45%	1.980%
13	8.963	991	999	1011	rBV	983325	1645304	32.28%	3.463%
14	9.351	1061	1065	1069	rVB3	5809	7081	0.14%	0.015%
15	9.681	1114	1121	1134	rBV	659432	1108423	21.75%	2.333%
16	10.222	1205	1213	1237	rBV	834845	1608613	31.56%	3.386%
17	10.592	1267	1276	1288	rBV	1123434	1809233	35.50%	3.808%
18	10.745	1294	1302	1320	rBV	836985	1656124	32.49%	3.486%
19	12.157	1534	1542	1544	rBV6	7431	14067	0.28%	0.030%
20	12.204	1544	1550	1555	rVV4	13011	25784	0.51%	0.054%
21	13.057	1689	1695	1696	rBV5	3211	6052	0.12%	0.013%
22	13.416	1750	1756	1759	rBV5	4883	5989	0.12%	0.013%
23	13.857	1824	1831	1843	rBV	1877848	2588432	50.78%	5.449%
24	14.127	1869	1877	1894	rBV	2143689	3235165	63.47%	6.810%
25	14.433	1923	1929	1938	rBV	1372236	2023384	39.70%	4.259%
26	14.692	1967	1973	1984	rBV4	30803	105317	2.07%	0.222%
27	15.263	2068	2070	2073	rBV3	3956	5666	0.11%	0.012%
28	15.427	2091	2098	2111	rBV	2879539	4013185	78.73%	8.448%
29	15.563	2115	2121	2133	rBV	517841	821474	16.12%	1.729%
30	15.669	2136	2139	2144	rVB3	17502	26498	0.52%	0.056%
31	16.857	2333	2341	2344	rBV10	4624	9293	0.18%	0.020%
32	17.180	2390	2396	2406	rBV	1431479	2002894	39.29%	4.216%
33	17.280	2406	2413	2432	rVV	3080592	4454338	87.39%	9.376%
34	17.404	2432	2434	2440	rVV7	6377	8706	0.17%	0.018%
35	17.857	2507	2511	2514	rVB3	13382	17163	0.34%	0.036%
36	18.080	2545	2549	2556	rBV4	29233	52525	1.03%	0.111%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036363.D
Acq On : 22 Aug 2022 13:13
Operator : CG/JU
Sample : N4251-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN66

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Title : SVOA CALIBRATION

37	19.139	2725	2729	2732	rBV4	32598	43751	0.86%	0.092%
38	19.209	2736	2741	2746	rBV2	34099	51650	1.01%	0.109%
39	19.362	2765	2767	2771	rBV5	14023	18523	0.36%	0.039%
40	19.574	2797	2803	2815	rBV	3617124	4767785	93.54%	10.036%
41	20.574	2970	2973	2977	rBV2	63070	65655	1.29%	0.138%
42	21.362	3102	3107	3118	rBV	1560748	2107598	41.35%	4.437%
43	23.539	3470	3477	3490	rBV2	2627290	5097096	100.00%	10.729%
44	23.692	3497	3503	3515	rVB2	1076712	2205026	43.26%	4.642%




Sum of corrected areas: 47505845

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036363.D
Acq On : 22 Aug 2022 13:13
Operator : CG/JU
Sample : N4251-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

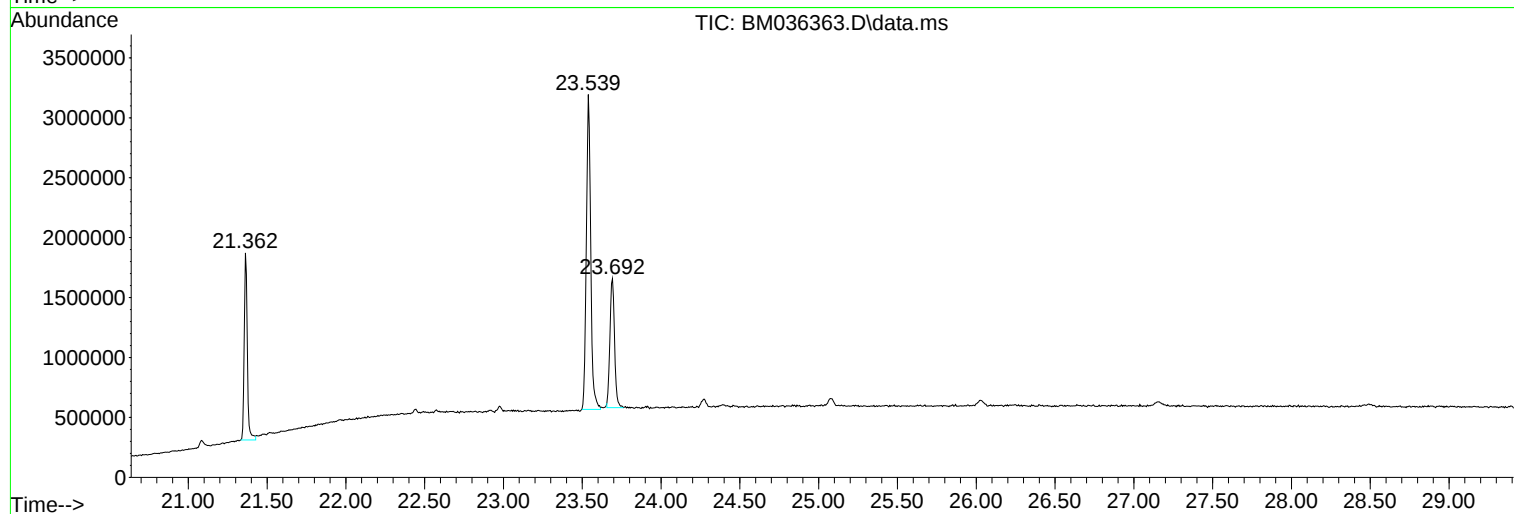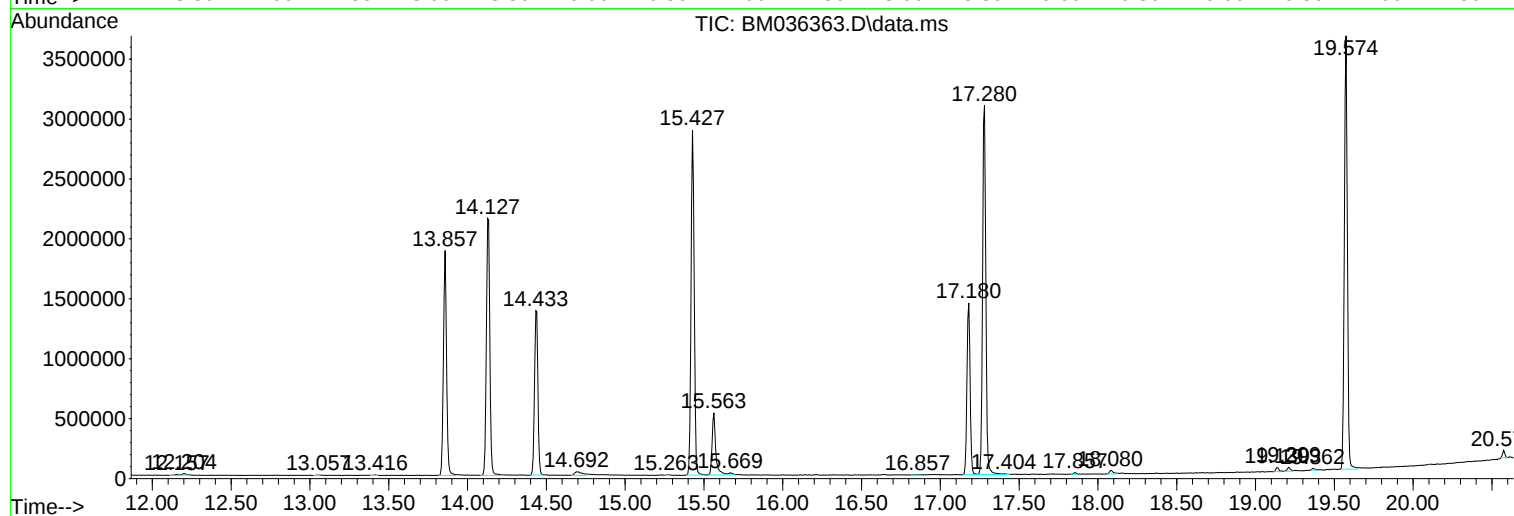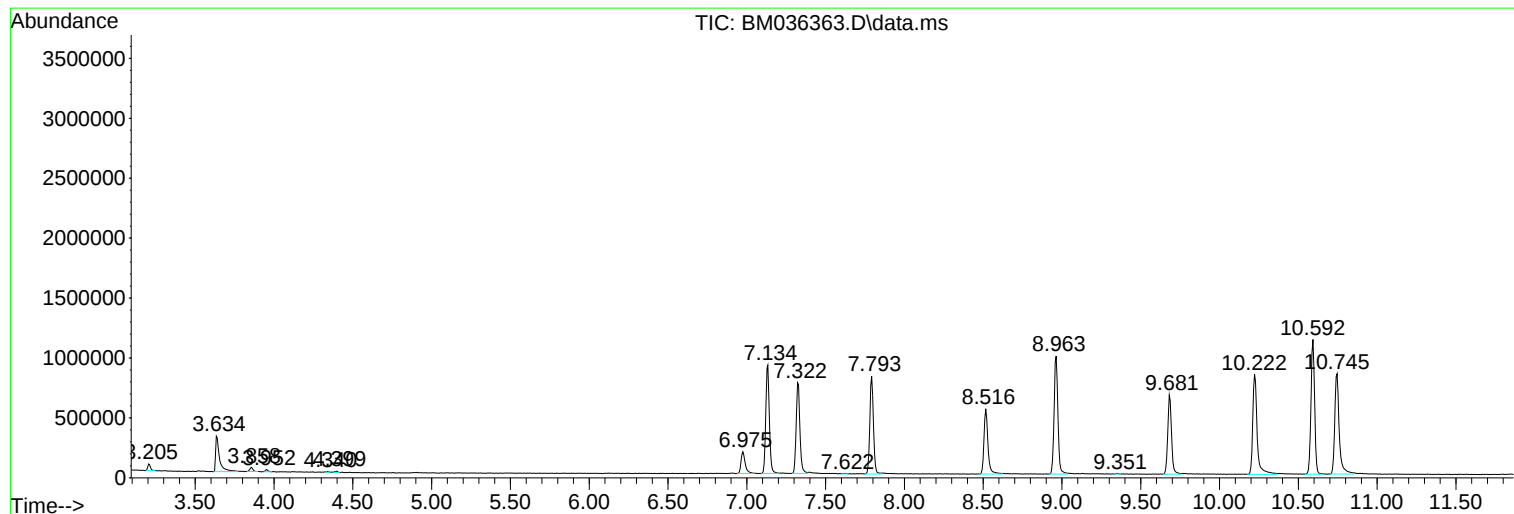

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036363.D
Acq On : 22 Aug 2022 13:13
Operator : CG/JU
Sample : N4251-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036363.D
Acq On : 22 Aug 2022 13:13
Operator : CG/JU
Sample : N4251-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc