

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036366.D
 Acq On : 22 Aug 2022 15:02
 Operator : CG/JU
 Sample : N4251-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGN89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036366.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	29	rVB	61630	75329	1.37%	0.143%
2	3.634	90	93	111	rBV	285096	479010	8.72%	0.911%
3	3.857	126	131	138	rVB	38379	56293	1.03%	0.107%
4	3.952	142	147	151	rBV	22408	28514	0.52%	0.054%
5	4.328	208	211	218	rVB3	22710	32959	0.60%	0.063%
6	4.399	220	223	226	rVB2	10426	12120	0.22%	0.023%
7	4.916	308	311	316	rVB4	3550	5608	0.10%	0.011%
8	5.846	465	469	473	rBV4	7745	12719	0.23%	0.024%
9	6.910	646	650	653	rBV3	5308	7816	0.14%	0.015%
10	6.975	653	661	675	rVV	215231	396642	7.22%	0.755%
11	7.128	681	687	704	rVB	962911	1531422	27.89%	2.913%
12	7.322	714	720	730	rBV	838713	1364442	24.85%	2.596%
13	7.793	792	800	808	rBV	858893	1344134	24.48%	2.557%
14	7.863	808	812	821	rVB2	16792	31135	0.57%	0.059%
15	8.010	832	837	841	rVB8	4907	8328	0.15%	0.016%
16	8.516	915	923	938	rBV	626320	1081365	19.69%	2.057%
17	8.634	938	943	950	rVB3	15795	31801	0.58%	0.060%
18	8.898	983	988	992	rBV7	6372	8689	0.16%	0.017%
19	8.963	992	999	1012	rBV	1071094	1779065	32.40%	3.384%
20	9.128	1022	1027	1031	rBV5	8889	13345	0.24%	0.025%
21	9.351	1059	1065	1071	rBV7	7280	14362	0.26%	0.027%
22	9.681	1112	1121	1133	rBV	735666	1235421	22.50%	2.350%
23	10.075	1186	1188	1193	rBV5	4432	7270	0.13%	0.014%
24	10.222	1206	1213	1233	rBV	955648	1757506	32.01%	3.343%
25	10.375	1236	1239	1247	rVB9	9615	20312	0.37%	0.039%
26	10.592	1268	1276	1283	rBV	1167311	1927542	35.10%	3.667%
27	10.745	1293	1302	1325	rBV	979786	1907149	34.73%	3.628%
28	10.904	1327	1329	1335	rVB7	5407	9445	0.17%	0.018%
29	11.298	1390	1396	1400	rBV8	3071	5819	0.11%	0.011%
30	12.204	1544	1550	1561	rVB3	16003	35325	0.64%	0.067%
31	12.798	1647	1651	1654	rBV6	5018	7547	0.14%	0.014%
32	13.051	1689	1694	1703	rVB6	9329	20203	0.37%	0.038%
33	13.292	1730	1735	1738	rBV2	4856	6350	0.12%	0.012%
34	13.339	1738	1743	1749	rVB8	5026	9412	0.17%	0.018%
35	13.410	1749	1755	1760	rBV7	11728	18933	0.34%	0.036%
36	13.857	1823	1831	1846	rBV	1993684	2700341	49.18%	5.137%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036366.D
 Acq On : 22 Aug 2022 15:02
 Operator : CG/JU
 Sample : N4251-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGN89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

37	14.133	1870	1878	1889	rBV	2353335	3453638	62.90%	6.570%
38	14.433	1923	1929	1942	rBV	1510372	2229598	40.60%	4.241%
39	14.686	1966	1972	1995	rBV3	44409	188491	3.43%	0.359%
40	14.886	2002	2006	2010	rVB7	4840	6771	0.12%	0.013%
41	15.116	2041	2045	2049	rBV6	4864	8275	0.15%	0.016%
42	15.233	2059	2065	2067	rBV5	6455	7544	0.14%	0.014%
43	15.427	2089	2098	2114	rBV	3118473	4399746	80.13%	8.369%
44	15.563	2115	2121	2135	rVV	616874	967850	17.63%	1.841%
45	15.674	2136	2140	2145	rVV2	22630	45833	0.83%	0.087%
46	15.710	2145	2146	2153	rVV6	7386	13428	0.24%	0.026%
47	15.804	2157	2162	2172	rVB7	8761	21013	0.38%	0.040%
48	16.145	2216	2220	2228	rBV5	6225	12921	0.24%	0.025%
49	16.327	2243	2251	2254	rBV9	3953	9076	0.17%	0.017%
50	16.933	2352	2354	2358	rBV4	5525	8311	0.15%	0.016%
51	16.980	2358	2362	2365	rVB5	4076	6721	0.12%	0.013%
52	17.180	2390	2396	2406	rBV	1635947	2244170	40.87%	4.269%
53	17.280	2406	2413	2425	rBV	3559470	5025934	91.53%	9.561%
54	17.392	2430	2432	2436	rVB4	10321	13395	0.24%	0.025%
55	17.468	2442	2445	2450	rBV4	7573	11096	0.20%	0.021%
56	17.680	2477	2481	2484	rBV5	4912	6218	0.11%	0.012%
57	17.715	2484	2487	2489	rVB4	5296	5898	0.11%	0.011%
58	17.851	2505	2510	2516	rBV	119358	155598	2.83%	0.296%
59	18.086	2545	2550	2557	rBV3	23902	48001	0.87%	0.091%
60	18.157	2558	2562	2572	rVB	11400	22560	0.41%	0.043%
61	19.139	2725	2729	2736	rBV2	37427	55349	1.01%	0.105%
62	19.209	2737	2741	2746	rBV	33829	47912	0.87%	0.091%
63	19.368	2766	2768	2772	rBV4	9322	11213	0.20%	0.021%
64	19.574	2797	2803	2819	rBV	4231168	5391738	98.19%	10.256%
65	20.574	2970	2973	2976	rBV2	71458	77087	1.40%	0.147%
66	21.362	3103	3107	3118	rBV	1688104	2241534	40.82%	4.264%
67	23.544	3471	3478	3490	rBV	2851014	5491045	100.00%	10.445%
68	23.691	3497	3503	3515	rVB2	1201782	2357840	42.94%	4.485%




Sum of corrected areas: 52569477

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036366.D
Acq On : 22 Aug 2022 15:02
Operator : CG/JU
Sample : N4251-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN89

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

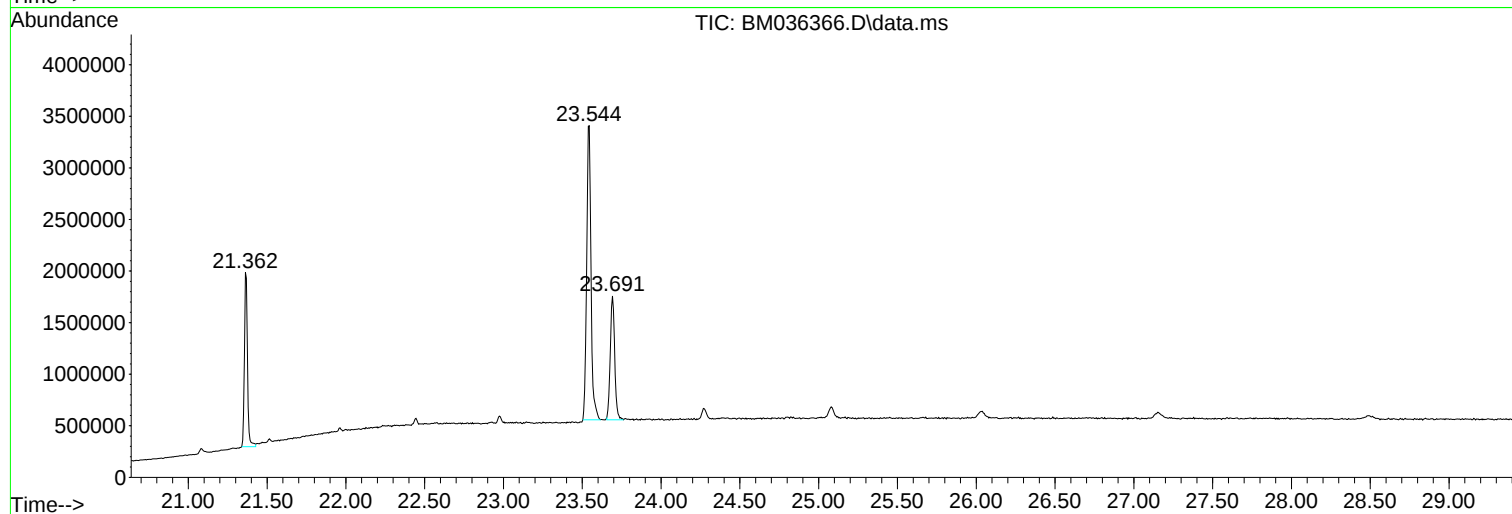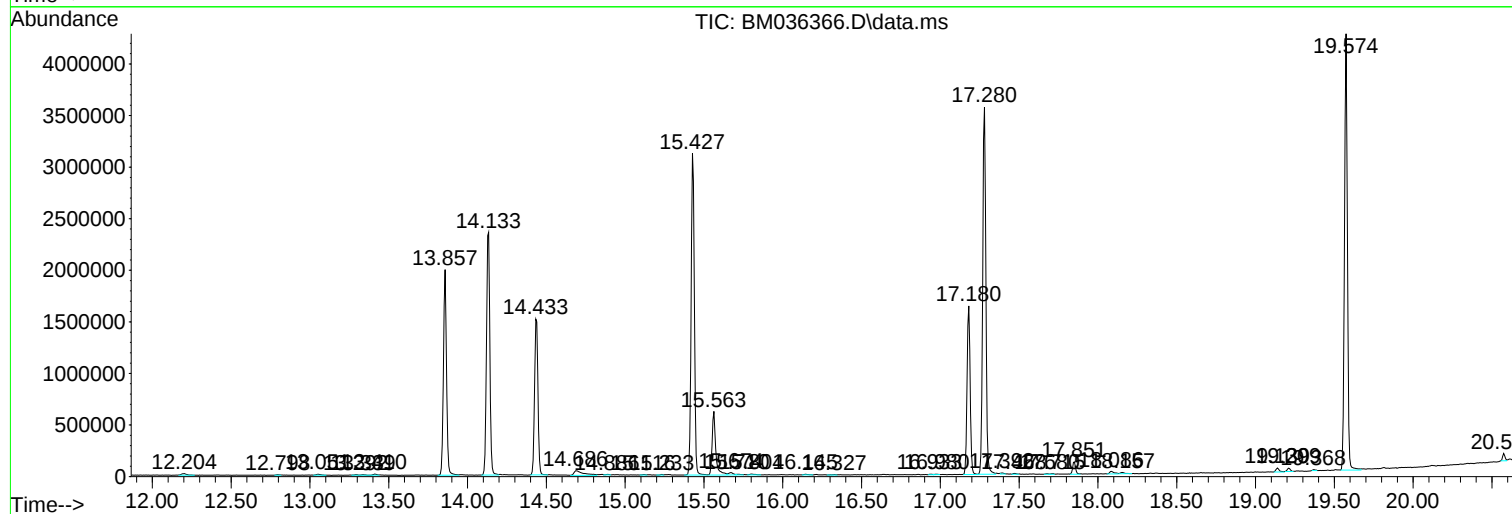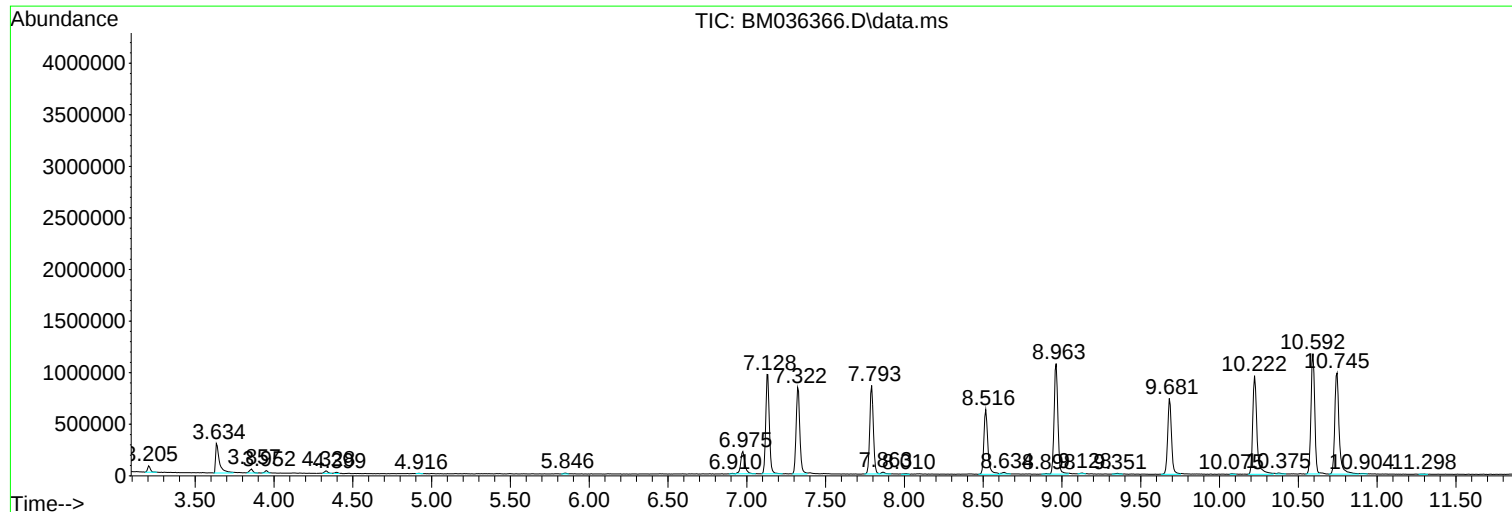

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036366.D
Acq On : 22 Aug 2022 15:02
Operator : CG/JU
Sample : N4251-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN89

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036366.D
Acq On : 22 Aug 2022 15:02
Operator : CG/JU
Sample : N4251-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN89

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc