

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036369.D
 Acq On : 22 Aug 2022 16:51
 Operator : CG/JU
 Sample : PB147152BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK152

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036369.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	30	rVB	83772	109194	2.59%	0.204%
2	3.628	90	92	111	rBV	944888	1461385	34.69%	2.725%
3	3.952	143	147	152	rVB	19119	25913	0.62%	0.048%
4	6.975	654	661	678	rBV	1088952	1820334	43.21%	3.394%
5	7.134	682	688	701	rVV	991579	1539565	36.54%	2.871%
6	7.328	714	721	731	rBV	1107430	1803578	42.81%	3.363%
7	7.792	793	800	813	rBV	863214	1344591	31.91%	2.507%
8	8.516	916	923	936	rBV	1338433	2195021	52.10%	4.093%
9	8.963	991	999	1016	rBV	1099752	1809808	42.96%	3.375%
10	9.681	1114	1121	1135	rBV	800375	1388047	32.95%	2.588%
11	10.222	1206	1213	1243	rBV	1128736	2103660	49.93%	3.923%
12	10.592	1269	1276	1287	rBV	1227875	1992666	47.30%	3.716%
13	10.745	1294	1302	1326	rBV	1189243	2266006	53.78%	4.225%
14	12.204	1543	1550	1560	rBV	16839	40531	0.96%	0.076%
15	13.416	1752	1756	1760	rBV3	4092	6325	0.15%	0.012%
16	13.857	1824	1831	1846	rBV	2030211	2764192	65.61%	5.154%
17	14.133	1871	1878	1894	rBV	2418654	3558709	84.47%	6.636%
18	14.439	1923	1930	1943	rBV	1537814	2326909	55.23%	4.339%
19	14.669	1962	1969	1989	rBV	383366	972405	23.08%	1.813%
20	15.427	2092	2098	2113	rBV	2915356	4130843	98.05%	7.703%
21	15.563	2115	2121	2136	rBV	490350	827037	19.63%	1.542%
22	15.668	2136	2139	2146	rVB7	18890	31181	0.74%	0.058%
23	16.639	2302	2304	2311	rVB7	3874	5032	0.12%	0.009%
24	16.968	2357	2360	2367	rBV4	3835	5848	0.14%	0.011%
25	17.180	2389	2396	2406	rBV	1660270	2272105	53.93%	4.237%
26	17.280	2406	2413	2428	rVV	2900768	4005971	95.08%	7.470%
27	19.139	2725	2729	2735	rBV3	28967	44069	1.05%	0.082%
28	19.209	2738	2741	2746	rVV2	25008	33671	0.80%	0.063%
29	19.574	2797	2803	2816	rBV	3199295	4213181	100.00%	7.856%
30	20.574	2970	2973	2979	rBV	69560	83991	1.99%	0.157%
31	21.362	3102	3107	3116	rBV	1684559	2170028	51.51%	4.046%
32	23.539	3471	3477	3492	rVB2	2155993	4117476	97.73%	7.678%
33	23.691	3497	3503	3514	rVB2	1076530	2159583	51.26%	4.027%




Sum of corrected areas: 53628855

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036369.D
Acq On : 22 Aug 2022 16:51
Operator : CG/JU
Sample : PB147152BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK152

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

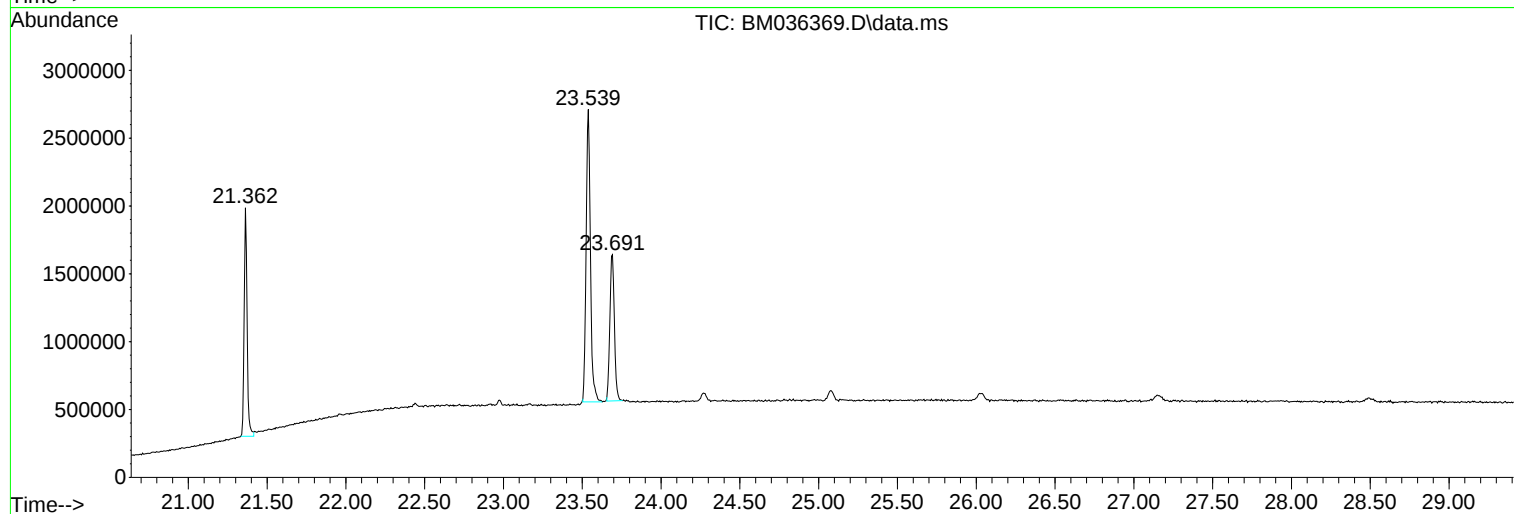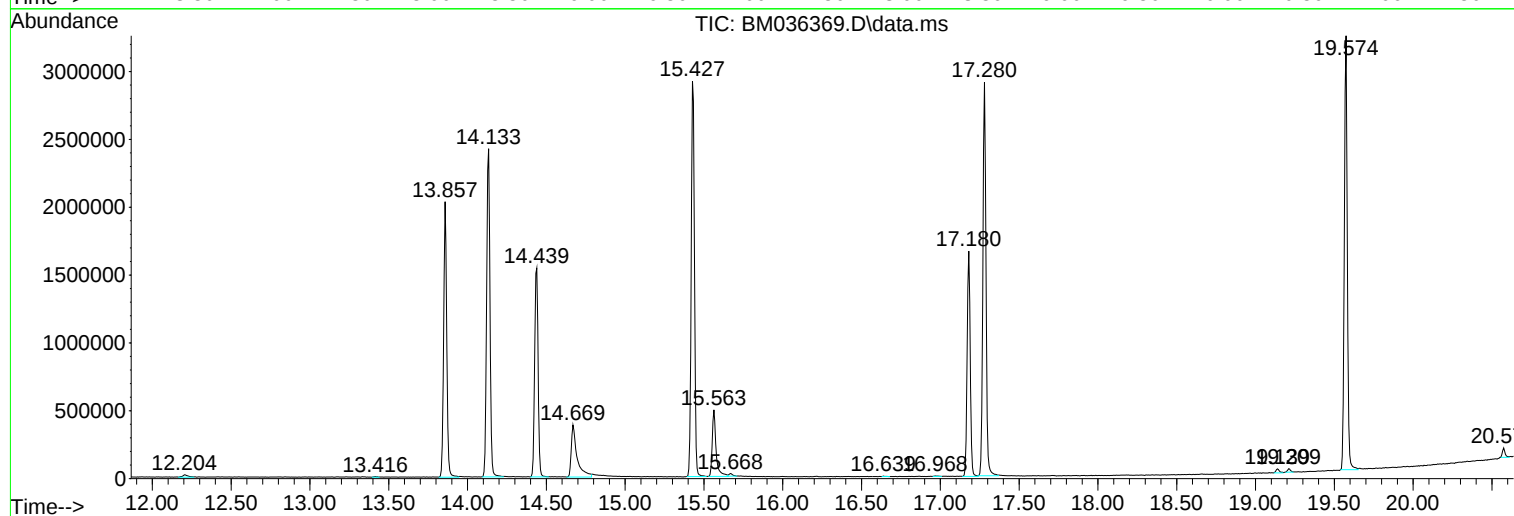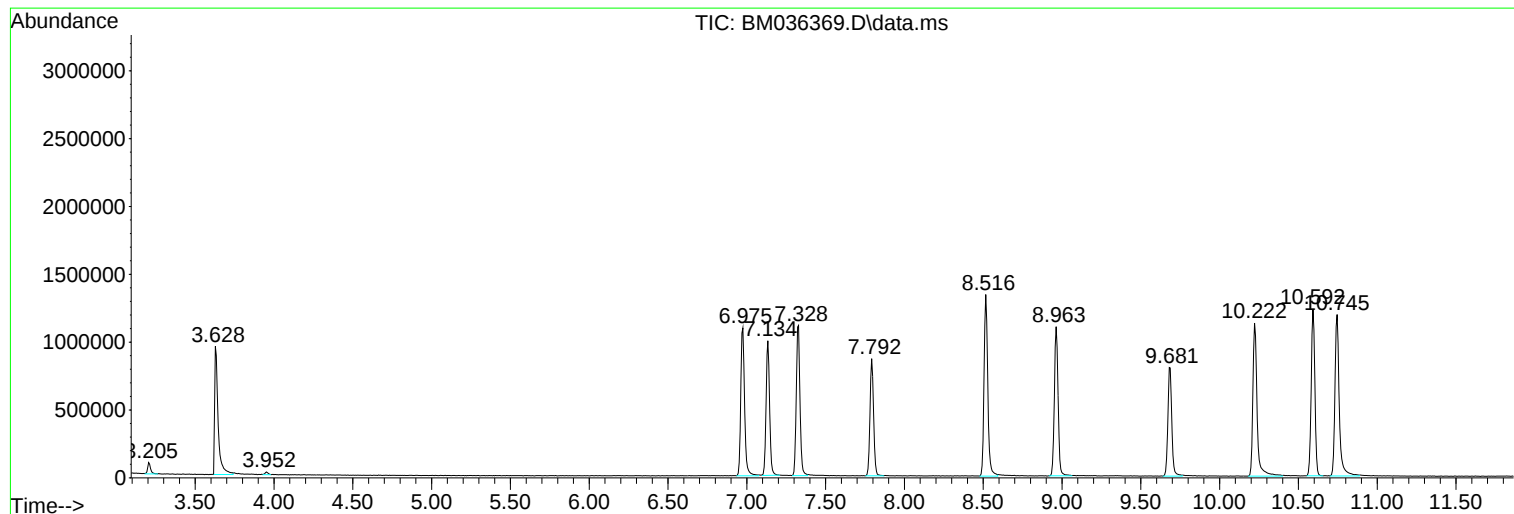

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036369.D
Acq On : 22 Aug 2022 16:51
Operator : CG/JU
Sample : PB147152BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK152

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036369.D
Acq On : 22 Aug 2022 16:51
Operator : CG/JU
Sample : PB147152BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK152

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc