

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036370.D
 Acq On : 22 Aug 2022 17:28
 Operator : CG/JU
 Sample : N4231-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COKN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036370.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	9	14	22	rBV	8401786	11017969	35.28%	10.187%
2	3.240	22	26	42	rVB	1674856	2078943	6.66%	1.922%
3	3.634	91	93	110	rBV	354873	572738	1.83%	0.530%
4	3.857	126	131	137	rVB	36761	57183	0.18%	0.053%
5	4.075	162	168	172	rBV2	51458	79223	0.25%	0.073%
6	4.487	231	238	251	rVV	21533367	31231760	100.00%	28.875%
7	4.587	251	255	264	rVB	34974	53772	0.17%	0.050%
8	5.169	347	354	359	rBV2	16989	31879	0.10%	0.029%
9	5.222	359	363	370	rVB	72992	105020	0.34%	0.097%
10	6.910	644	650	654	rBV	29945	44359	0.14%	0.041%
11	6.975	655	661	669	rVV	310679	509662	1.63%	0.471%
12	7.134	680	688	707	rBV	1260140	1990793	6.37%	1.841%
13	7.328	714	721	731	rBV	1098118	1789152	5.73%	1.654%
14	7.469	741	745	750	rVB2	30882	49551	0.16%	0.046%
15	7.793	793	800	809	rBV	868604	1336640	4.28%	1.236%
16	8.516	916	923	938	rBV	896713	1506468	4.82%	1.393%
17	8.963	991	999	1018	rBV	1435211	2335808	7.48%	2.160%
18	9.681	1109	1121	1136	rBV	1005340	1741444	5.58%	1.610%
19	10.222	1206	1213	1231	rBV	1423273	2477346	7.93%	2.290%
20	10.592	1269	1276	1287	rBV	1199008	1962423	6.28%	1.814%
21	10.745	1295	1302	1318	rBV	1289499	2359107	7.55%	2.181%
22	12.192	1544	1548	1559	rBV2	21328	41556	0.13%	0.038%
23	13.298	1730	1736	1745	rBV3	27560	49123	0.16%	0.045%
24	13.857	1824	1831	1845	rBV	2675556	3642879	11.66%	3.368%
25	14.086	1863	1870	1873	rBV	940577	1455793	4.66%	1.346%
26	14.133	1873	1878	1895	rVB	3405360	5141825	16.46%	4.754%
27	14.439	1923	1930	1939	rBV	1580781	2333254	7.47%	2.157%
28	14.680	1966	1971	1985	rBV2	103705	266852	0.85%	0.247%
29	14.863	1997	2002	2010	rVB10	16352	38915	0.12%	0.036%
30	15.427	2089	2098	2105	rBV	4026314	5617638	17.99%	5.194%
31	15.480	2105	2107	2114	rVV5	22223	37574	0.12%	0.035%
32	15.563	2114	2121	2134	rVV	913764	1341852	4.30%	1.241%
33	15.668	2134	2139	2144	rVB2	23471	38616	0.12%	0.036%
34	17.180	2389	2396	2403	rBV	1719411	2299858	7.36%	2.126%
35	17.280	2406	2413	2425	rBV	4085372	5538071	17.73%	5.120%
36	18.080	2544	2549	2558	rBV3	86617	158717	0.51%	0.147%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036370.D
Acq On : 22 Aug 2022 17:28
Operator : CG/JU
Sample : N4231-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M

Title : SVOA CALIBRATION

37	19.139	2725	2729	2733	rBV2	39148	49325	0.16%	0.046%
38	19.209	2737	2741	2745	rBV	41460	56815	0.18%	0.053%
39	19.362	2763	2767	2776	rBV3	47964	81021	0.26%	0.075%
40	19.456	2780	2783	2788	rBV5	23483	34605	0.11%	0.032%
41	19.574	2797	2803	2814	rBV	4467033	5878551	18.82%	5.435%
42	20.574	2970	2973	2977	rBV	65094	71535	0.23%	0.066%
43	21.362	3102	3107	3116	rBV	1766108	2314418	7.41%	2.140%
44	23.539	3470	3477	3491	rBV2	3072051	5985473	19.16%	5.534%
45	23.692	3497	3503	3517	rVB2	1143015	2356805	7.55%	2.179%




Sum of corrected areas: 108162311

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036370.D
Acq On : 22 Aug 2022 17:28
Operator : CG/JU
Sample : N4231-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KN4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

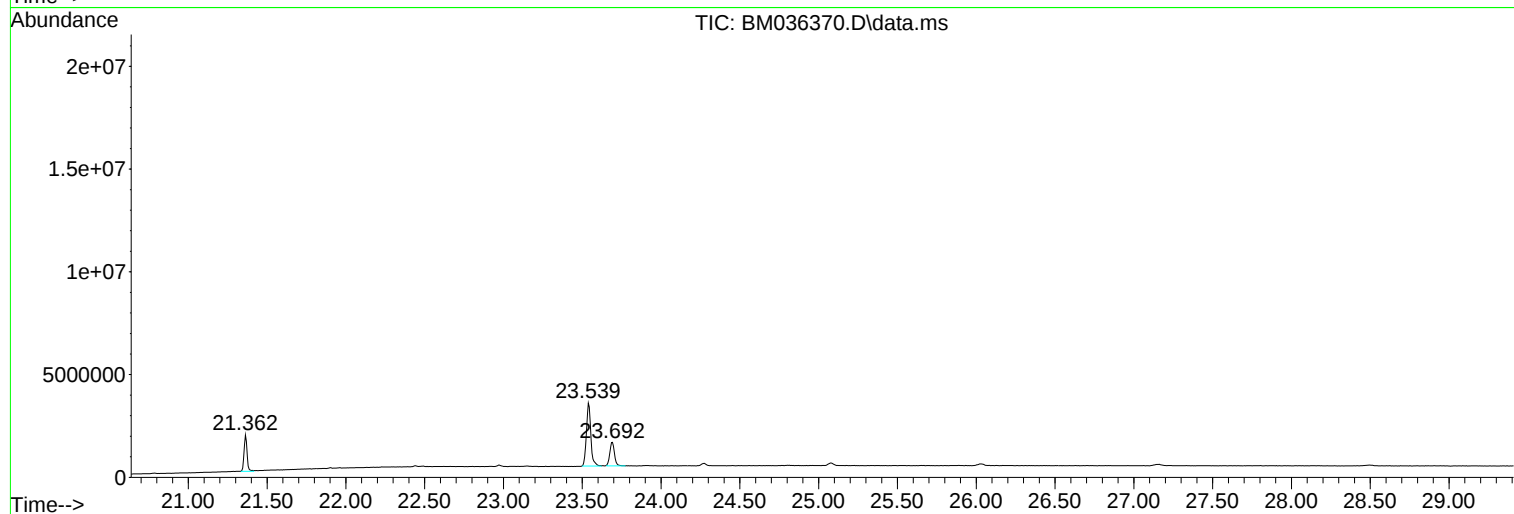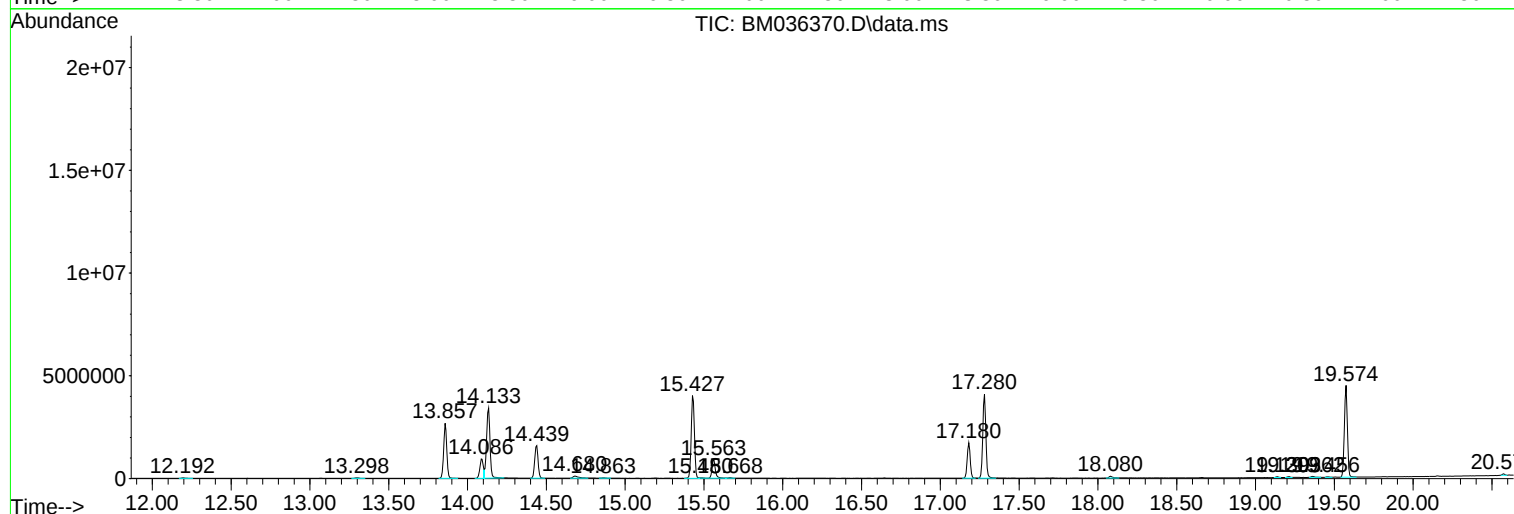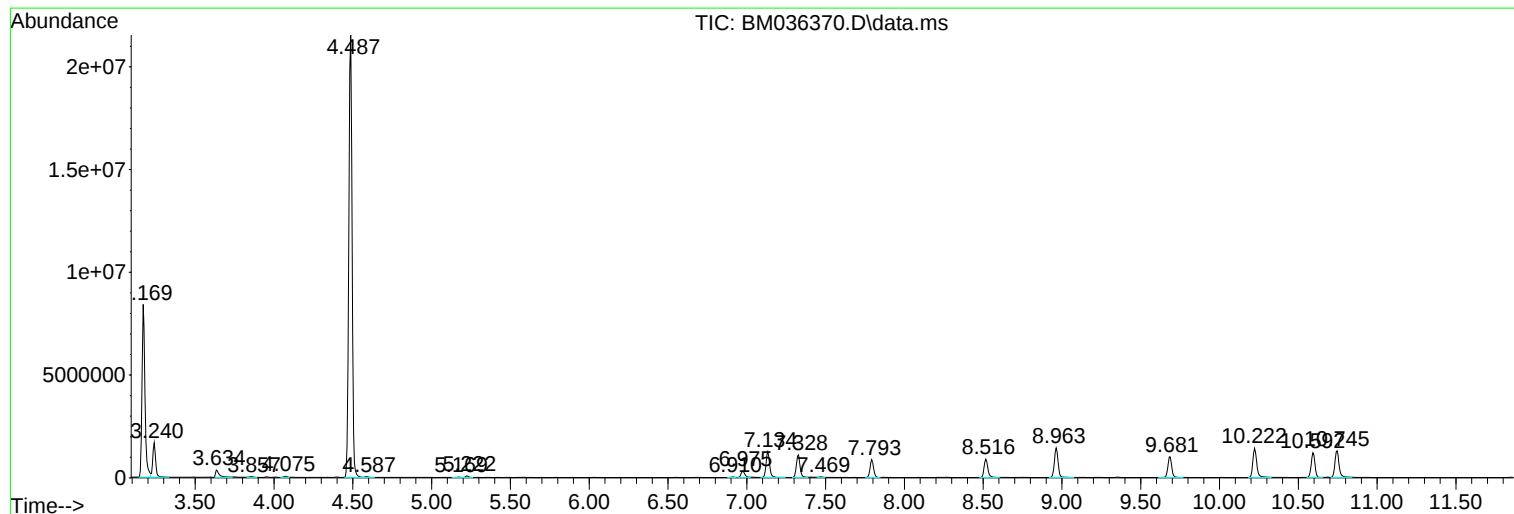

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036370.D
Acq On : 22 Aug 2022 17:28
Operator : CG/JU
Sample : N4231-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KN4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036370.D
Acq On : 22 Aug 2022 17:28
Operator : CG/JU
Sample : N4231-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KN4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc