

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036376.D
 Acq On : 22 Aug 2022 21:08
 Operator : CG/JU
 Sample : N4251-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGN90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036376.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	29	rBV	66838	83066	1.91%	0.176%
2	3.640	92	94	114	rBV	139796	253378	5.84%	0.536%
3	3.857	126	131	137	rVB	35012	52979	1.22%	0.112%
4	3.952	143	147	154	rVB	24728	34540	0.80%	0.073%
5	4.334	207	212	218	rVV2	23615	35172	0.81%	0.074%
6	4.399	219	223	227	rVB	10707	14568	0.34%	0.031%
7	5.793	457	460	464	rVB6	3223	5022	0.12%	0.011%
8	5.846	464	469	474	rBV9	9352	17473	0.40%	0.037%
9	6.910	646	650	653	rBV5	6600	10480	0.24%	0.022%
10	6.975	653	661	676	rVB	184838	346235	7.97%	0.733%
11	7.134	681	688	702	rBV	887306	1427777	32.88%	3.022%
12	7.322	714	720	730	rBV	740037	1225712	28.23%	2.595%
13	7.793	792	800	808	rBV	929977	1440698	33.18%	3.050%
14	7.863	808	812	819	rVB2	18736	33407	0.77%	0.071%
15	8.004	832	836	839	rBV6	2897	4387	0.10%	0.009%
16	8.092	848	851	858	rVB8	3377	5799	0.13%	0.012%
17	8.416	902	906	910	rVB7	3066	4564	0.11%	0.010%
18	8.516	916	923	938	rBV	549480	957786	22.06%	2.027%
19	8.628	938	942	949	rVB2	15800	30434	0.70%	0.064%
20	8.898	983	988	992	rBV6	5496	10853	0.25%	0.023%
21	8.963	992	999	1014	rVV	1000070	1638062	37.73%	3.468%
22	9.122	1023	1026	1033	rBV9	10708	18159	0.42%	0.038%
23	9.357	1062	1066	1069	rBV5	6182	7834	0.18%	0.017%
24	9.681	1114	1121	1137	rBV	672660	1148858	26.46%	2.432%
25	10.075	1185	1188	1194	rBV7	4786	9220	0.21%	0.020%
26	10.222	1205	1213	1233	rBV	901595	1656857	38.16%	3.507%
27	10.381	1236	1240	1246	rVB7	8546	16810	0.39%	0.036%
28	10.510	1259	1262	1268	rVB6	3752	6476	0.15%	0.014%
29	10.592	1268	1276	1283	rBV	1314873	2124240	48.92%	4.497%
30	10.639	1283	1284	1294	rVB9	14678	24989	0.58%	0.053%
31	10.745	1294	1302	1327	rBV	855739	1674556	38.57%	3.545%
32	11.851	1483	1490	1492	rBV6	2880	5610	0.13%	0.012%
33	12.198	1543	1549	1558	rBV2	15064	31716	0.73%	0.067%
34	12.822	1653	1655	1664	rVB6	2529	4903	0.11%	0.010%
35	13.051	1689	1694	1699	rBV2	7631	10417	0.24%	0.022%
36	13.292	1730	1735	1738	rVV	8719	11804	0.27%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036376.D
 Acq On : 22 Aug 2022 21:08
 Operator : CG/JU
 Sample : N4251-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGN90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

37	13.416	1749	1756	1763	rBV9	9570	18789	0.43%	0.040%
38	13.680	1798	1801	1807	rBV7	3092	4737	0.11%	0.010%
39	13.857	1824	1831	1846	rBV	1801053	2464229	56.75%	5.216%
40	14.133	1868	1878	1890	rBV	2111955	3124976	71.97%	6.615%
41	14.433	1922	1929	1942	rBV	1677891	2442197	56.25%	5.170%
42	14.521	1942	1944	1948	rVB4	8689	9419	0.22%	0.020%
43	14.692	1967	1973	1986	rBV4	33542	117426	2.70%	0.249%
44	14.892	2004	2007	2011	rVB6	4689	4753	0.11%	0.010%
45	15.116	2041	2045	2048	rBV2	8107	11080	0.26%	0.023%
46	15.233	2061	2065	2067	rBV	7550	9107	0.21%	0.019%
47	15.427	2090	2098	2115	rBV	2701739	3776869	86.99%	7.995%
48	15.563	2115	2121	2136	rVV	488237	784188	18.06%	1.660%
49	15.668	2136	2139	2150	rVB7	15635	35560	0.82%	0.075%
50	15.804	2158	2162	2168	rVB6	7467	12492	0.29%	0.026%
51	16.645	2300	2305	2310	rVB5	4846	8303	0.19%	0.018%
52	16.939	2350	2355	2358	rBV6	4137	6395	0.15%	0.014%
53	16.968	2358	2360	2365	rVB5	4286	5844	0.13%	0.012%
54	17.180	2389	2396	2406	rBV	1685312	2308462	53.17%	4.887%
55	17.280	2406	2413	2427	rVV	3046024	4251965	97.93%	9.001%
56	17.474	2441	2446	2449	rBV3	8859	11231	0.26%	0.024%
57	17.851	2505	2510	2515	rBV	160752	203739	4.69%	0.431%
58	18.098	2547	2552	2556	rBV7	10802	21275	0.49%	0.045%
59	18.151	2559	2561	2565	rBV	11065	12161	0.28%	0.026%
60	19.139	2725	2729	2736	rBV5	27855	43610	1.00%	0.092%
61	19.209	2737	2741	2746	rBV	26540	37617	0.87%	0.080%
62	19.574	2797	2803	2815	rBV	3223752	4341944	100.00%	9.191%
63	20.574	2970	2973	2977	rVB2	57054	61248	1.41%	0.130%
64	21.362	3102	3107	3118	rBV	1678922	2197408	50.61%	4.652%
65	23.539	3470	3477	3490	rBV2	2208636	4294440	98.91%	9.091%
66	23.686	3496	3502	3512	rVB2	1182373	2234074	51.45%	4.729%




Sum of corrected areas: 47240379

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036376.D
Acq On : 22 Aug 2022 21:08
Operator : CG/JU
Sample : N4251-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN90

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

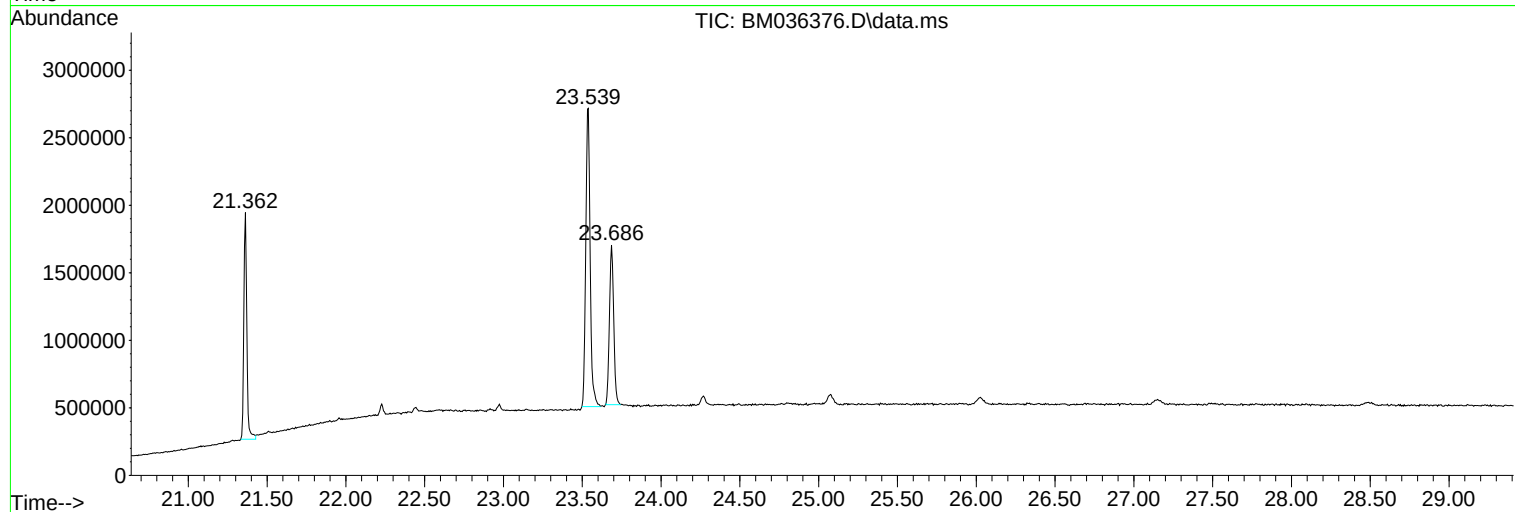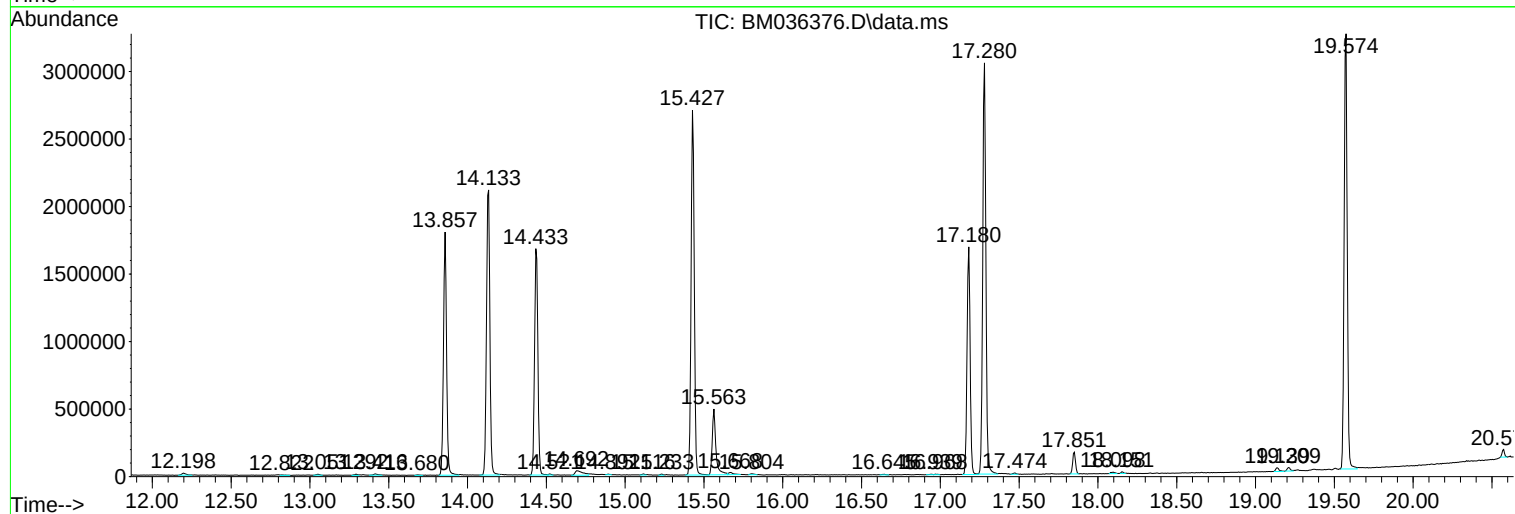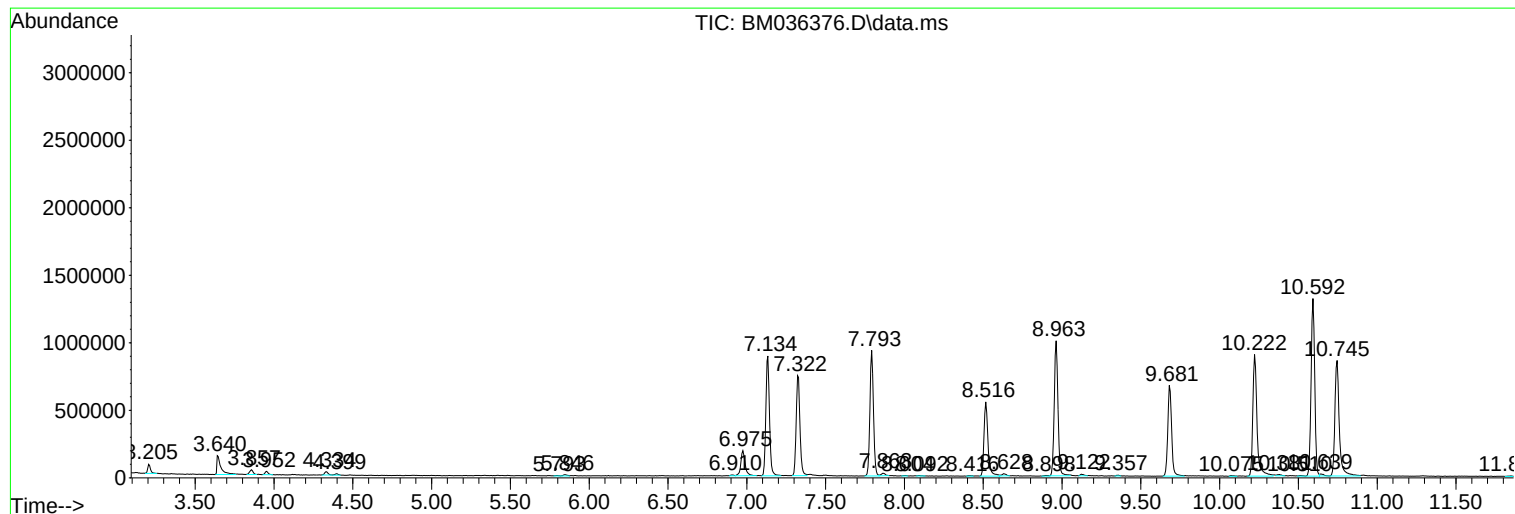

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036376.D
Acq On : 22 Aug 2022 21:08
Operator : CG/JU
Sample : N4251-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN90

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036376.D
Acq On : 22 Aug 2022 21:08
Operator : CG/JU
Sample : N4251-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN90

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc